

SME20557 — CHRISTUS Trinity Clinic MRI

Intelas · Siemens MRI · Palestine, TX · Jul 7 – Aug 6 monitor data (1,468 captures) · analyzed 2026-08-06

COMPRESSOR

ON

running continuously through the window

COLDHEAD

43.000 K

steady at base temperature

PRESSURE NOW

15.51 PSI

within the 14.4–16.4 PSI band · rising

EVENT PEAK

15.52 PSI


Jul 16 15:15Z · 0.88 PSI under threshold

HELIUM

93.1%

+0.00 pts · no loss · no quench

HE PRESSURE — JUL 7 → AUG 6 (daily range, PSI)

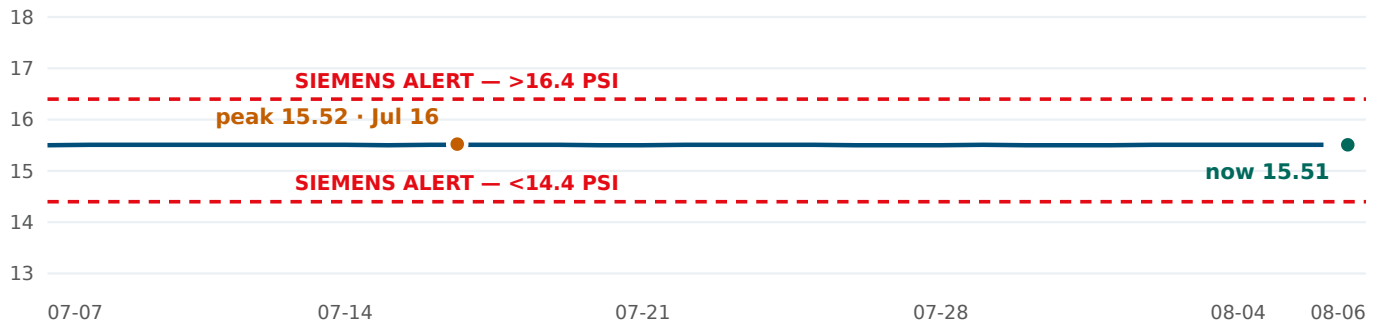

HELIUM LEVEL — JUL 7 → AUG 6 (daily reading, %)



Timeline (UTC): Baseline Jul 7 - Aug 6: coldhead at base temperature. No compressor events, alarms, or threshold breaches detected across 1,468 captures. Helium rose to **93.1%** (+0.00 vs baseline). No quench. Pressure now reads 15.51 PSI (Aug 6 13:45Z) — within the 14.4–16.4 PSI band.

CURRENT — AUG 6 (last readings)

Compressor ON. He pressure 15.51 PSI (13:45Z). Helium 93.1%.

RATES

Pressure +0.00 PSI vs baseline (15.51 → 15.51); peak 15.52. Helium +0.00 points.

DATA NOTES

1,468 captures · 1,468 valid pressure · 1,468 valid helium readings. Charts show the daily min-max range with the daily last value. EDU (1,468 captures): room 32.0–104.4 °F · probes 78.2–83.5 / 87.1–94.2 °F · humidity 0–31%. Host clock ~57 min off vs capture time — times shown use capture time.