

SME01133 — Piedmont Mountainside Hospital MRI

Piedmont HealthCare · GE MRI · Jasper, GA · Jul 7 – Aug 6 monitor data (1,469 captures) · analyzed 2026-08-06

COMPRESSOR

ON

running continuously through the window

COLDHEAD

4.104 K

steady at base temperature

PRESSURE NOW

0.998 PSI

within the 0.5–5.2 PSI band · easing

EVENT PEAK

1.038 PSI

Jul 7 22:45Z · 4.162 PSI under threshold

HELIUM


84.74%

+0.06 pts · no loss · no quench

HE PRESSURE — JUL 7 → AUG 6 (daily range, PSI)



HELIUM LEVEL — JUL 7 → AUG 6 (daily reading, %)

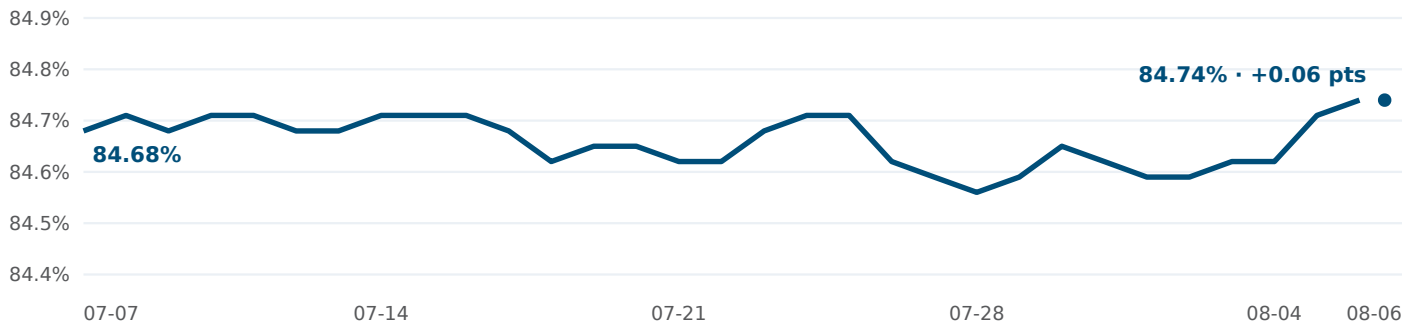

Timeline (UTC): Baseline Jul 7 – Aug 6: coldhead at base temperature. No compressor events, alarms, or threshold breaches detected across 1,469 captures. Helium rose to **84.74%** (+0.06 vs baseline). No quench. Pressure now reads 0.998 PSI (Aug 6 14:15Z) — within the 0.5–5.2 PSI band.

CURRENT — AUG 6 (last readings)

Compressor ON. He pressure 0.998 PSI (14:15Z). Helium 84.74%.

RATES

Pressure +0.000 PSI vs baseline (0.998 → 0.998); peak 1.038. Helium +0.06 points.

DATA NOTES

1,469 captures · 1,469 valid pressure · 1,469 valid helium readings. Charts show the daily min-max range with the daily last value. EDU (1,469 captures): room 61.3–75.7 °F · probes 51.7–59.8 / 57.0–77.1 °F · humidity 44–78%. Host clock ~236 min off vs capture time — times shown use capture time.