

SME15822 — Premier Radiology - Smyrna MRI

Althea USA · Philips MRI · Smyrna, TN · Jul 7 – Aug 6 monitor data (1,309 captures) · analyzed 2026-08-06

COMPRESSOR

ON

recovered Aug 4 15:48Z · 4 cycles from Jul 20 13:48Z

PRESSURE NOW

37 mbar

46% of the 80 mbar line · easing

EVENT PEAK

282 mbar

Jul 21 08:48Z · 202 mbar over threshold

TEMP ALARM

TRIGGERED


27 readings · Jul 20 13:48Z → Jul 21 04:48Z

HELIUM


75.8%

–0.60 pts · level falling

HE PRESSURE — JUL 7 → AUG 6 (daily range, mbar · orange shade = the event window)

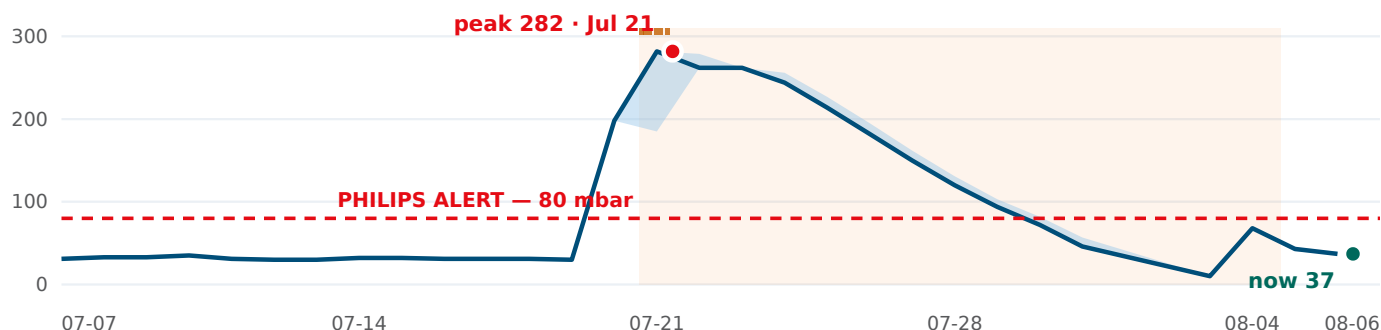

HELIUM LEVEL — JUL 7 → AUG 6 (daily reading, %)

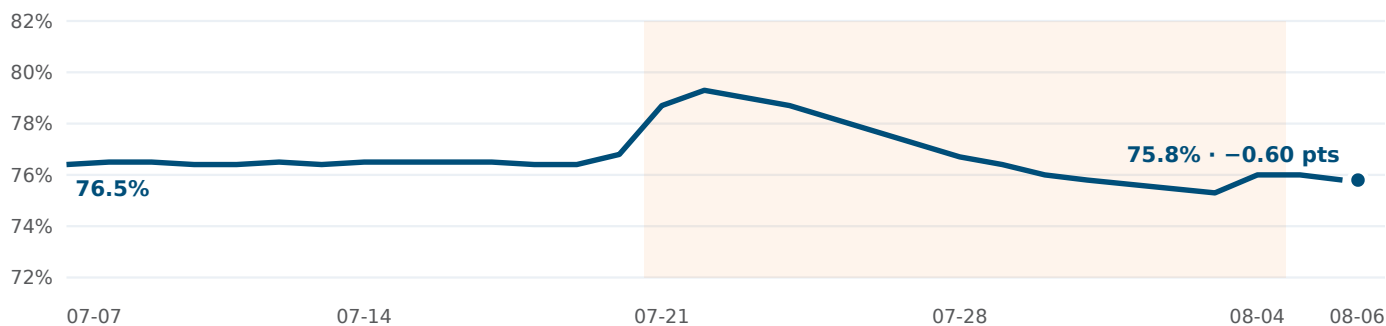

Timeline (UTC): Baseline Jul 7 – Jul 20: pressure held 30–35 mbar, helium 76.4–76.5%. **Jul 20 13:48Z: the compressor stopped** and then cycled on/off 4 times through Aug 4 15:48Z (38 readings off). A compressor temperature alarm was triggered Jul 20 13:48Z → Jul 21 04:48Z (27 readings — not continuous, it re-triggered 3 times; amber strip on the pressure chart). Room temperature held 73.6–74.8 °F over the alarm window. He pressure rose from 30 to a **peak of 282 mbar at Jul 21 08:48Z** — 202 mbar over the 80 mbar line (+13 mbar/h avg on the ramp). **The compressor recovered Aug 4 15:48Z** and has held since. Helium fell to **75.8%** (–0.60 vs baseline). No quench. Pressure now reads 37 mbar (Aug 6 08:48Z) — 46% of the line.

CURRENT — AUG 6 (last readings)

Compressor ON. He pressure 37 mbar (08:48Z). Helium 75.8%.

RATES

Pressure +7 mbar vs baseline (30 → 37); peak 282. Ramp averaged +13 mbar/h. Helium –0.60 points.

DATA NOTES

1,309 captures · 56 valid pressure · 60 valid helium readings. Charts show the daily min-max range with the daily last value. Tech Room Temp 16.4–21.7 °C in window. EDU (1,468 captures): room 70.9–80.2 °F · probes 60.7–70.0 / 61.1–81.3 °F · humidity 39–72%. Host clock ~61 min off vs capture time — times shown use capture time.