


SME01133 — Piedmont Mountainside Hospital MRI


Piedmont HealthCare · GE MRI · Jasper, GA · Jul 7 – Aug 6 monitor data (1,466 captures) · analyzed 2026-08-06

COMPRESSOR ON running continuously through the window	COLDHEAD 4.148 K steady at base temperature	PRESSURE NOW 0.998 PSI 20% of the 5 PSI line · easing	EVENT PEAK 1.038 PSI Jul 7 22:45Z · 3.962 PSI under threshold	HELIUM 84.74% +0.06 pts · no loss · no quench
---	---	---	---	---

HE PRESSURE — JUL 7 → AUG 6 (daily range, PSI)

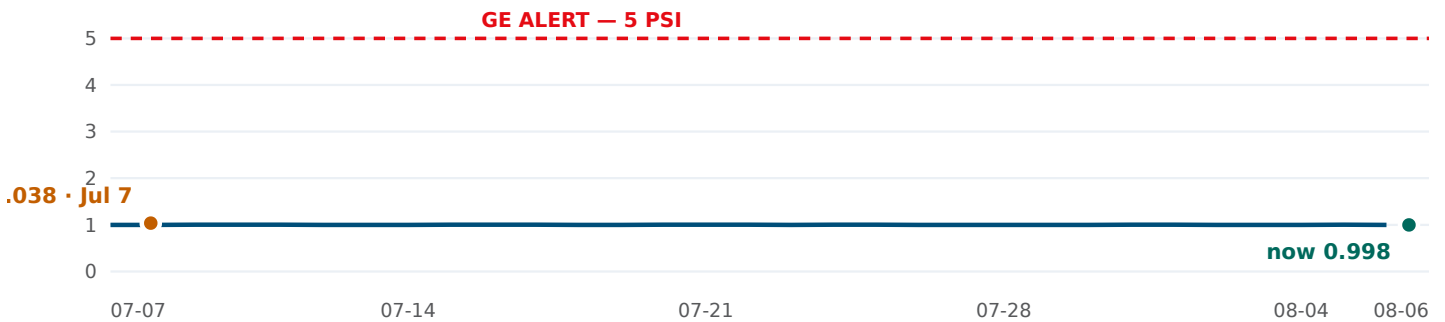

HELIUM LEVEL — JUL 7 → AUG 6 (daily reading, %)

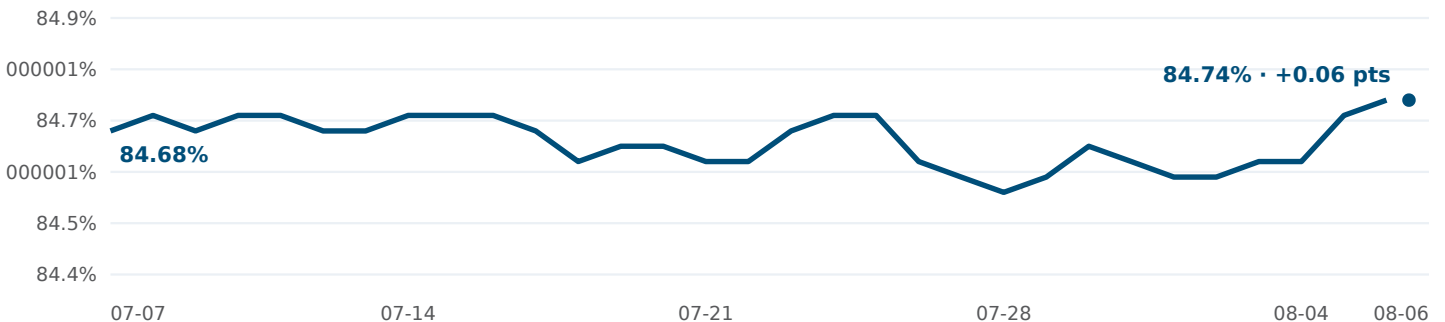

Timeline (UTC): Baseline Jul 7 - Aug 6: coldhead at base temperature. No compressor events, alarms, or threshold breaches detected across 1,466 captures. Helium rose to **84.74%** (+0.06 points vs baseline). No quench. Pressure now reads 0.998 PSI (Aug 6 12:45Z) — 20% of the line.

CURRENT — AUG 6 (last readings)

Compressor ON. He pressure 0.998 PSI (12:45Z). Helium 84.74%.

RATES

Pressure +0.000 PSI vs baseline (0.998 → 0.998); peak 1.038. Ramp averaged +0.002 PSI/h. Helium +0.06 points.

DATA NOTES

1,466 captures · 1,466 valid pressure · 1,466 valid helium readings. Charts show the daily min-max range with the daily last value. EDU (1,466 captures): room 61.3–75.7 °F · probes 51.7–59.8 / 57.0–77.1 °F · humidity 44–78%. Host clock ~236 min off vs capture time — times shown use capture time.