

SME01141 — Piedmont Rockdale Hospital MRI

Piedmont HealthCare · GE MRI · Conyers, GA · Jul 7 – Aug 6 monitor data (1,466 captures) · analyzed 2026-08-06

COMPRESSOR

RESTARTED

recovered Jul 13 22:15Z
· off ~0.0 h

COLDHEAD

4.121 K

from 12.7 K

PRESSURE NOW

1.002 PSI

20% of the 5 PSI
line · easing

EVENT PEAK

1.092 PSI


Jul 13 21:45Z ·
3.908 PSI under
threshold

HELIUM


74.93%

–0.14 pts · no loss ·
no quench

HE PRESSURE — JUL 7 → AUG 6 (daily range, PSI · orange shade = the event window)

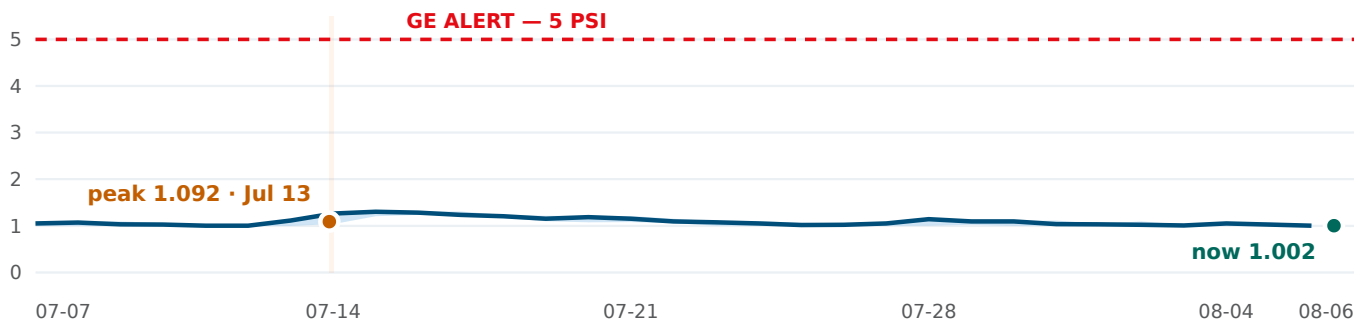

HELIUM LEVEL — JUL 7 → AUG 6 (daily reading, %)

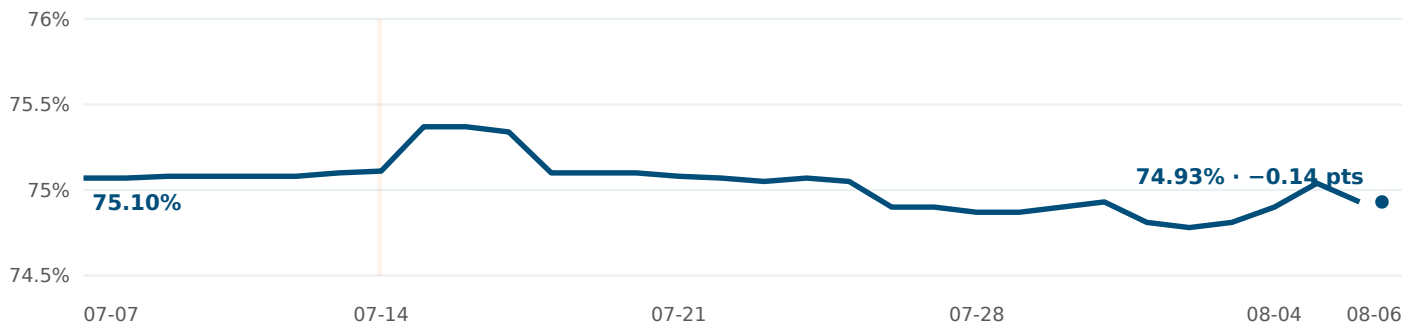

Timeline (UTC): Baseline Jul 7 – Jul 13: pressure held 0.998–1.101 PSI, helium 75.01–75.11%, coldhead at base temperature. **Jul 13 21:45Z: the compressor stopped** and stayed off ~0.0 h (1 readings off). He pressure rose from 1.079 to a **peak of 1.092 PSI at Jul 13 21:45Z** — never reached the 5 PSI threshold, 3.908 PSI below the line. **The compressor recovered Jul 13 22:15Z** and has held since. Helium fell to **74.93%** (–0.14 points vs baseline). No quench. Pressure now reads 1.002 PSI (Aug 6 12:45Z) — 20% of the line.

CURRENT — AUG 6 (last readings)

Compressor ON. He pressure 1.002 PSI (12:45Z). Helium 74.93%.

RATES

Pressure –0.077 PSI vs baseline (1.079 → 1.002); peak 1.092. Helium –0.14 points.

DATA NOTES

1,466 captures · 1,466 valid pressure · 1,466 valid helium readings. Charts show the daily min-max range with the daily last value. EDU (1,466 captures): room 79.7–84.6 °F · probes 57.4–68.3 / 62.9–84.2 °F · humidity 27–51%. Host clock ~745 min off vs capture time — times shown use capture time.