

SME02582 — Mississippi Baptist Medical Center MRI

Intelas · GE MRI · Jackson, MS · Jul 7 – Aug 6 monitor data (1,466 captures) · analyzed 2026-08-06

COMPRESSOR

OFF

stopped Jul 7 17:15Z
· off ~715.5 h

COLDHEAD

15.203 K

from 133.7 K

PRESSURE NOW

1.993 PSI

40% of the 5 PSI line
· easing

EVENT PEAK

3.782 PSI


Jul 25 13:15Z · 1.218
PSI under threshold

HELIUM


84.99%

+0.00 pts · no loss ·
no quench

HE PRESSURE — JUL 7 → AUG 6 (daily range, PSI · orange shade = the event window)

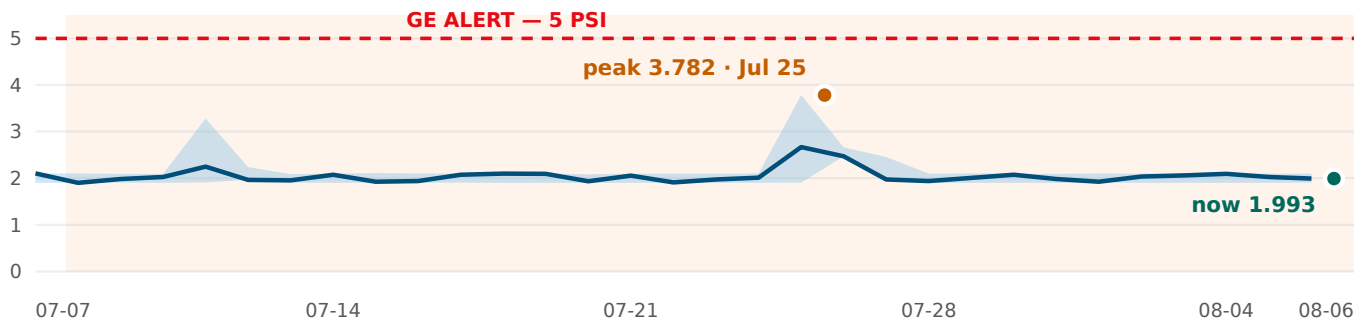

HELIUM LEVEL — JUL 7 → AUG 6 (daily reading, %)

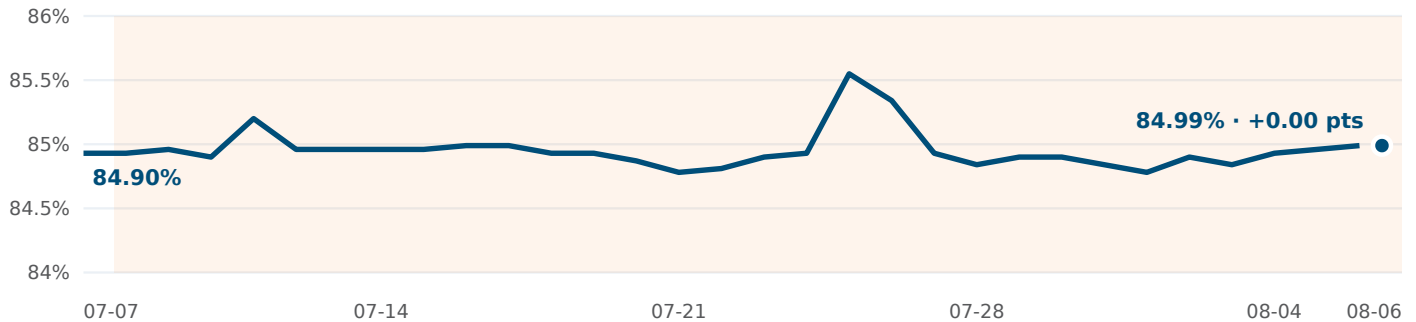

Timeline (UTC): Baseline Jul 7 - Jul 7: pressure held 1.903–2.093 PSI, helium 84.87–84.99%, coldhead at base temperature. **Jul 7 17:15Z: the compressor stopped and has not recovered** — off ~715.5 h at the last capture (74 readings off). He pressure rose from 2.034 to a **peak of 3.782 PSI at Jul 25 13:15Z** — never reached the 5 PSI threshold, 1.218 PSI below the line (+0.004 PSI/h avg on the ramp). Helium rose to **84.99%** (+0.00 points vs baseline). No quench. Pressure now reads 1.993 PSI (Aug 6 12:45Z) — 40% of the line. **Warming event OPEN at end of data.**

CURRENT — AUG 6 (last readings)

Compressor OFF. He pressure 1.993 PSI (12:45Z). Helium 84.99%.

RATES

Pressure –0.041 PSI vs baseline (2.034 → 1.993); peak 3.782. Ramp averaged +0.004 PSI/h. Helium +0.00 points.

DATA NOTES

1,466 captures · 1,466 valid pressure · 1,466 valid helium readings. Charts show the daily min-max range with the daily last value. EDU (1,466 captures): room 32.0–97.2 °F · probes 67.9–93.8 / 64.1–87.7 °F · humidity 0–57%. Host clock ~160 min off vs capture time — times shown use capture time.