


SME18368 — Premier Radiology - Hermitage MRI

Althea USA · Philips MRI · Hermitage, TN · Jul 7 – Aug 6 monitor data (1,465 captures) · analyzed 2026-08-06

COMPRESSOR ON running continuously through the window	PRESSURE NOW — no pressure data	EVENT PEAK — no pressure data	TEMP ALARM NONE no temperature alarm in window	HELIUM 78.5% +0.00 pts · no loss · no quench
---	--	--	--	--

HE PRESSURE — JUL 7 → AUG 6 (daily range, mbar)

HELIUM LEVEL — JUL 7 → AUG 6 (daily reading, %)

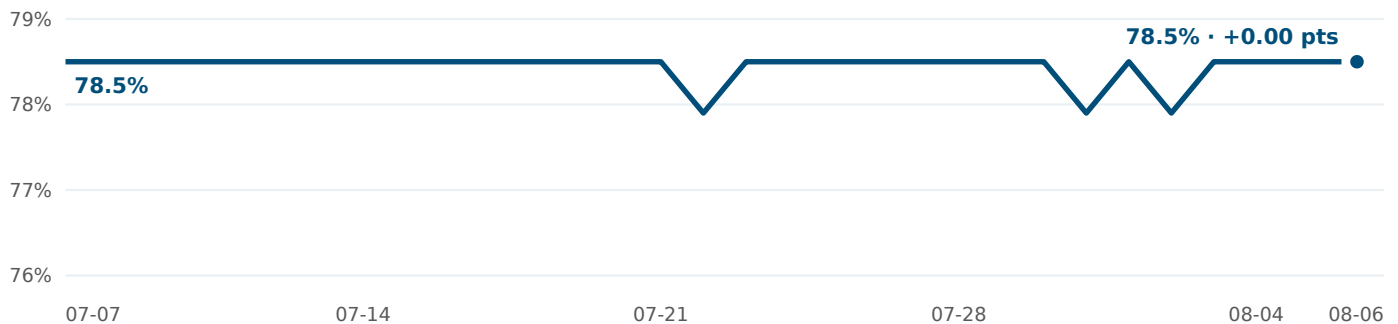

Timeline (UTC): No compressor events, alarms, or threshold breaches detected across 1,465 captures. Helium rose to **78.5%** (+0.00 points vs baseline). No quench.

CURRENT — AUG 6 (last readings) Compressor ON. Helium 78.5%.	RATES Helium +0.00 points.	DATA NOTES 1,465 captures · 0 valid pressure · 68 valid helium readings. Charts show the daily min-max range with the daily last value. Tech Room Temp 17.1–21.4 °C in window. EDU (1,466 captures): room 32.0–70.3 °F · probes 59.5–62.1 / 68.3–71.5 °F · humidity 0–84%. Host clock ~52 min off vs capture time — times shown use capture time.
--	--------------------------------------	---