

## SME01136 — Piedmont Newnan Hospital MRI

Piedmont HealthCare · Siemens MRI · Newnan, GA · Jul 7 – Aug 6 monitor data (1,471 captures) · analyzed 2026-08-06

### COMPRESSOR

**ON**

running continuously through the window

### SHIELD NOW

**41.0 K**

41% of the 100 K line · rising

### EVENT PEAK

**41.0 K**

Jul 7 06:15Z · 59.0 K under threshold

### CABINET

**24.8 °C**


23.6–25.4 °C in window · warn 38 · alarm 43 °C

### HELIUM


**79.4%**

–6.50 pts · level falling

### SHIELD TEMP — JUL 7 → AUG 6 (daily range, K)

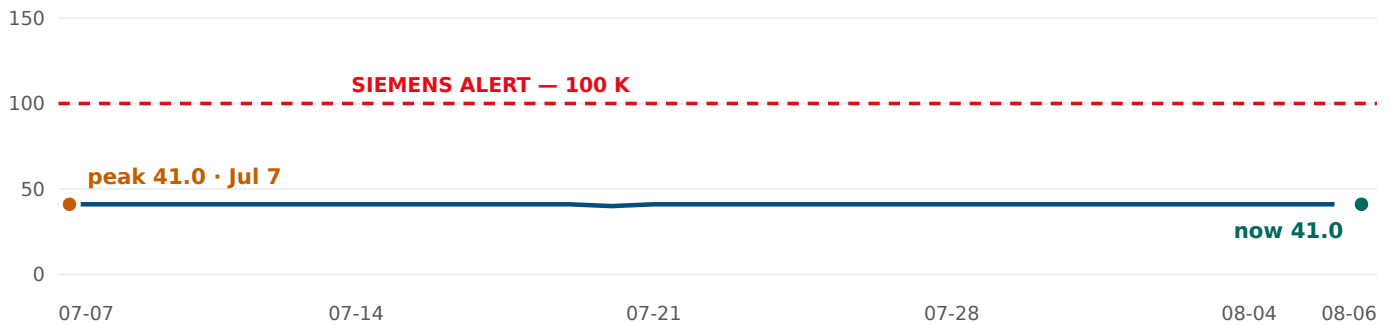

### HELIUM LEVEL — JUL 7 → AUG 6 (daily reading, %)

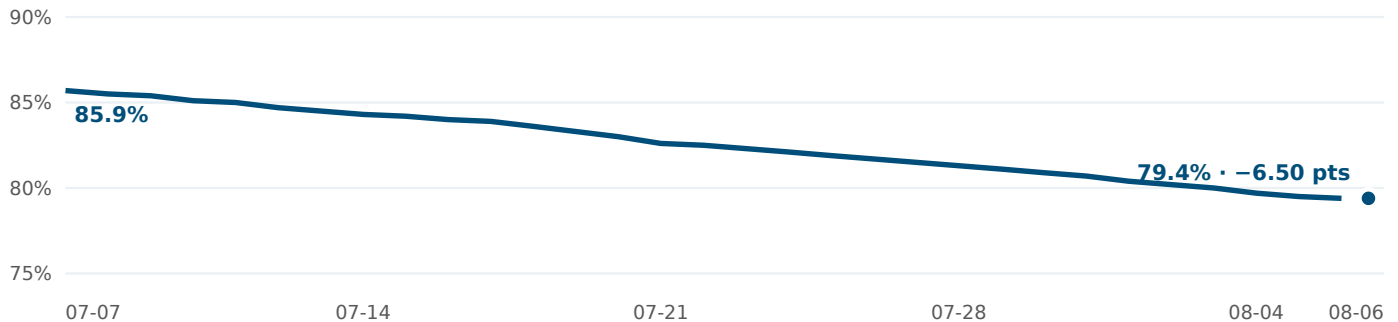

**Timeline (UTC):** No compressor events, alarms, or threshold breaches detected across 1,471 captures. Helium fell to **79.4%** (–6.50 vs baseline). No quench. Shield temp now reads 41.0 K (Aug 6 15:15Z) — 41% of the line.

### CURRENT — AUG 6 (last readings)

Compressor ON. Shield temp 41.0 K (15:15Z). Helium 79.4%.

### RATES

Shield temp +1.0 K vs baseline (40.0 → 41.0); peak 41.0. Helium –6.50 points.

### DATA NOTES

1,471 captures · 1,471 valid pressure · 1,471 valid helium readings. Charts show the daily min-max range with the daily last value. EDU (1,471 captures): room 73.8–73.8 °F · probes 74.5–74.5 / 76.0–76.0 °F · humidity 51–51%.