

SME10756 — Brook Park Imaging Center MRI

Network Imaging Associates LLC · Siemens MRI · Brook Park, OH · Jul 7 – Aug 6 monitor data (1,471 captures)

COMPRESSOR

ON

recovered Jul 27
16:15Z · 3 cycles
from Jul 21 17:45Z

SHIELD NOW

52.0 K

52% of the 100 K
line · rising

EVENT PEAK

51.0 K

Jul 23 20:45Z · 49.0
K under threshold

CABINET

22.1 °C


15.8–22.4 °C in
window · warn 38 ·
alarm 43 °C

HELIUM


55.5%

below the 60%
warning level

SHIELD TEMP — JUL 7 → AUG 6 (daily range, K · orange shade = the event window)

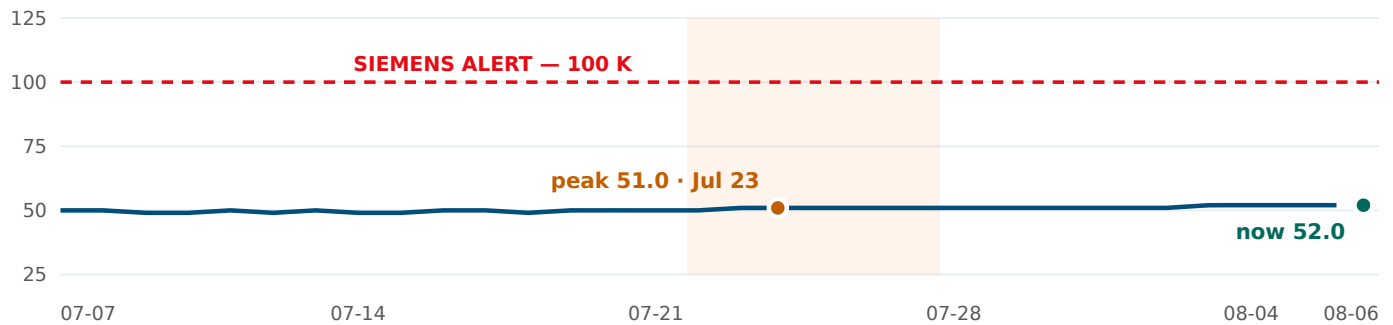

HELIUM LEVEL — JUL 7 → AUG 6 (daily reading, %)

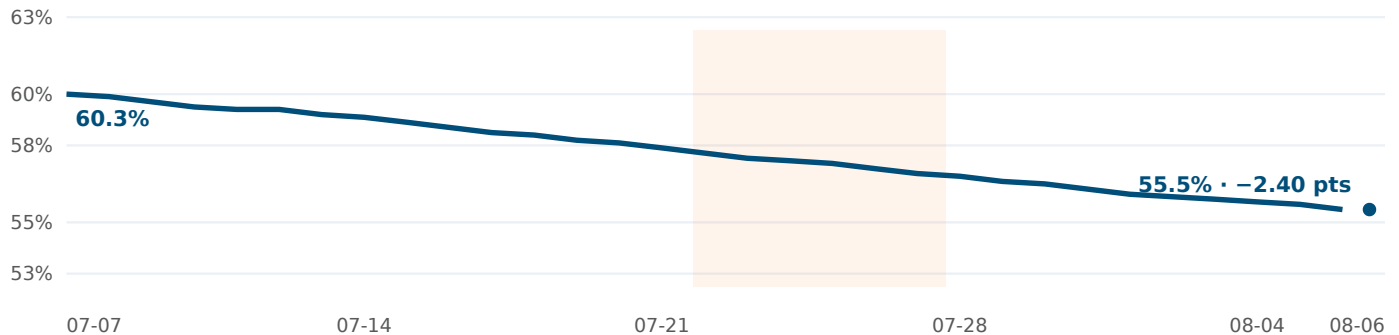

Timeline (UTC): Baseline Jul 7 - Jul 21: shield temp held 49.0–51.0 K, helium 57.9–60.3%. **Jul 21 17:45Z: the compressor stopped** (per EDU vibration sensor) and then cycled on/off 3 times through Jul 27 16:15Z (3 readings off). Shield temp rose from 50.0 to a **peak of 51.0 K at Jul 23 20:45Z** — never reached the 100 K threshold, 49.0 K below the line (+0.0 K/h avg on the ramp). **The compressor recovered Jul 27 16:15Z** and has held since. Helium fell to **55.5%** (–2.40 vs baseline). No quench. Shield temp now reads 52.0 K (Aug 6 15:15Z) — 52% of the line.

CURRENT — AUG 6 (last readings)

Compressor ON. Shield temp 52.0 K (15:15Z). Helium 55.5%.

RATES

Shield temp +2.0 K vs baseline (50.0 → 52.0); peak 51.0. Ramp averaged +0.0 K/h. Helium –2.40 points.

DATA NOTES

1,471 captures · 1,471 valid pressure · 1,471 valid helium readings. Charts show the daily min-max range with the daily last value. EDU (1,471 captures): room 71.1–78.1 °F · probes –196.6–60.0 / 54.8–68.7 °F · humidity 33–65%.