

SME11139 — Piedmont Orthopedics | OrthoAtlanta

Johns Creek MRI

Piedmont HealthCare · Siemens MRI · Johns Creek, GA · Jul 7 – Aug 6 monitor data (1,471 captures) · analyzed

COMPRESSOR

ON

running continuously through the window

SHIELD NOW

60.0 K

60% of the 100 K line

EVENT PEAK

60.0 K

Jul 7 00:15Z · 40.0 K under threshold

CABINET

26.3 °C

24.1–29.5 °C in window · warn 38 · alarm 43 °C

HELIUM


83.5%

+21.80 pts · no loss · no quench

SHIELD TEMP — JUL 7 → AUG 6 (daily range, K)



HELIUM LEVEL — JUL 7 → AUG 6 (daily reading, %)

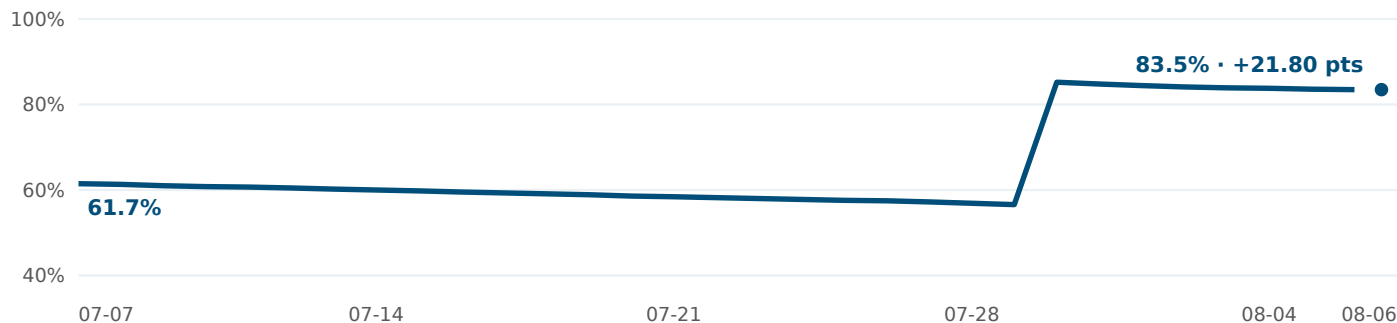

Timeline (UTC): No compressor events, alarms, or threshold breaches detected across 1,471 captures. Helium rose to **83.5%** (+21.80 vs baseline). No quench. Shield temp now reads 60.0 K (Aug 6 15:15Z) — 60% of the line.

CURRENT — AUG 6 (last readings)

Compressor ON. Shield temp 60.0 K (15:15Z). Helium 83.5%.

RATES

Shield temp +0.0 K vs baseline (60.0 → 60.0); peak 60.0. Helium +21.80 points.

DATA NOTES

1,471 captures · 1,471 valid pressure · 1,471 valid helium readings. Charts show the daily min-max range with the daily last value. EDU (1,471 captures): room 77.2–77.2 °F · probes -196.6–82.2 / 66.4–75.4 °F · humidity 38–38%.