

SME20758 — NYC Health and Hospitals - Lincoln MRI

Intelas · Siemens MRI · Bronx, NY · Jul 7 – Aug 6 monitor data (1,471 captures) · analyzed 2026-08-06

COMPRESSOR

ON

running continuously through the window

SHIELD NOW

44.0 K

44% of the 100 K line · easing

EVENT PEAK

45.0 K

Jul 17 06:45Z · 55.0 K under threshold

CABINET

23.6 °C


20.5–26.7 °C in window · warn 38 · alarm 43 °C

HELIUM


63.7%

–5.30 pts · level falling

SHIELD TEMP — JUL 7 → AUG 6 (daily range, K)

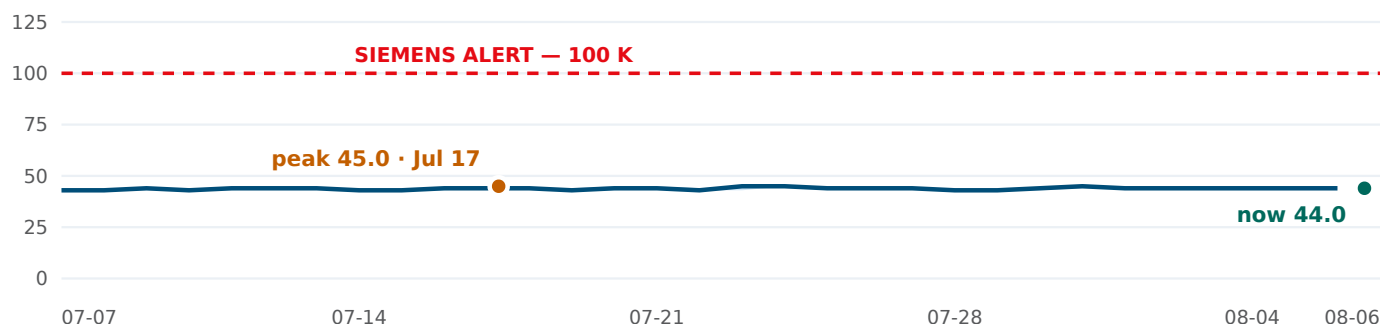

HELIUM LEVEL — JUL 7 → AUG 6 (daily reading, %)

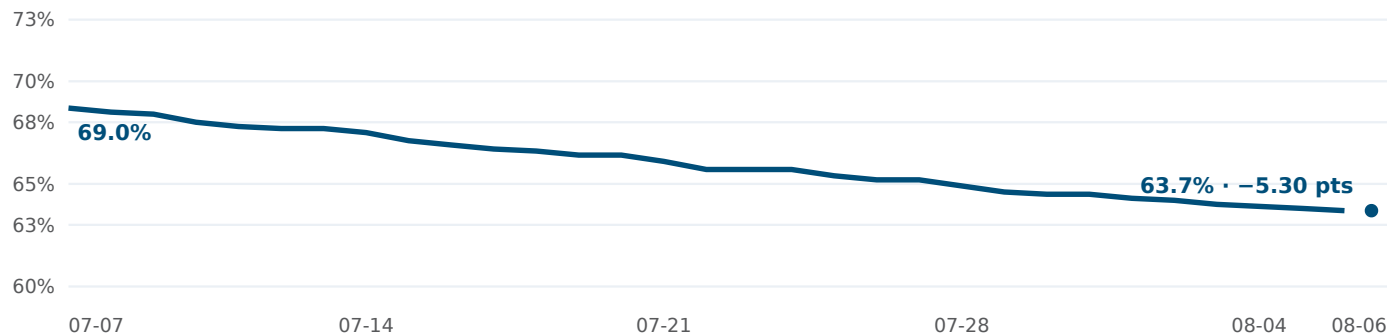

Timeline (UTC): No compressor events, alarms, or threshold breaches detected across 1,471 captures. Helium fell to **63.7%** (–5.30 vs baseline). No quench. Shield temp now reads 44.0 K (Aug 6 15:15Z) — 44% of the line.

CURRENT — AUG 6 (last readings)

Compressor ON. Shield temp 44.0 K (15:15Z). Helium 63.7%.

RATES

Shield temp +0.0 K vs baseline (44.0 → 44.0); peak 45.0. Helium –5.30 points.

DATA NOTES

1,471 captures · 1,471 valid pressure · 1,471 valid helium readings. Charts show the daily min-max range with the daily last value. EDU (1,471 captures): room 32.0–89.6 °F · probes 52.0–55.6 / 54.5–65.6 °F · humidity 0–62%. Host clock ~21 min off vs capture time — times shown use capture time.