


SME01136 — Piedmont Newnan Hospital MRI


Piedmont HealthCare · Siemens MRI · Newnan, GA · Jul 7 – Aug 6 monitor data (1,478 captures) · analyzed 2026-08-06

COMPRESSOR ON running continuously through the window	SHIELD NOW 41.0 K 41% of the 100 K line · rising	EVENT PEAK 41.0 K Jul 7 06:15Z · 59.0 K under threshold	CABINET 24.7 °C 23.6–25.4 °C in window · warn 38 · alarm 43 °C	HELIUM 79.4% –6.50 pts · level falling
---	--	---	--	--

SHIELD TEMP — JUL 7 → AUG 6 (daily range, K)

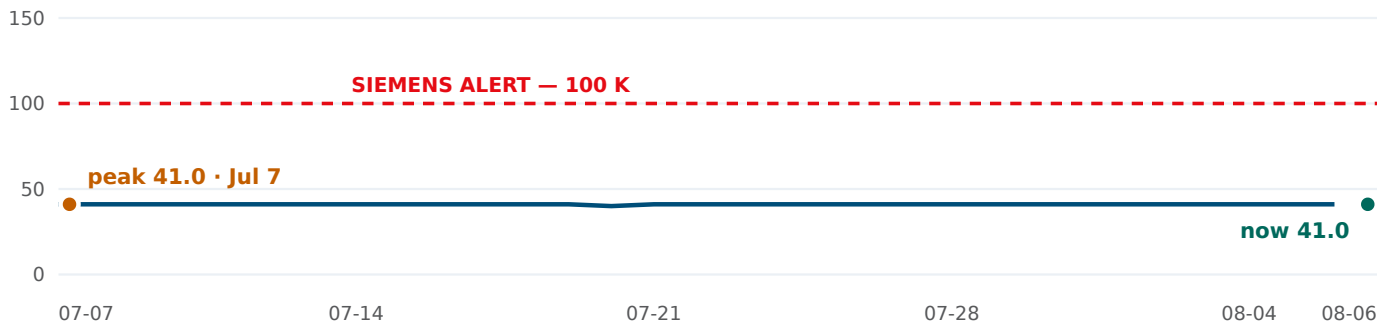

HELIUM LEVEL — JUL 7 → AUG 6 (daily reading, %)

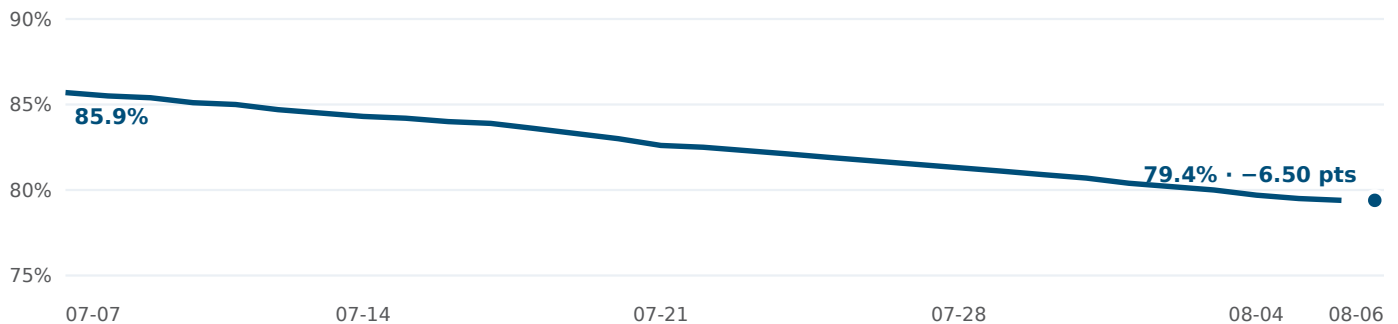

Timeline (UTC): No compressor events, alarms, or threshold breaches detected across 1,478 captures. Helium fell to **79.4%** (–6.50 vs baseline). No quench. Shield temp now reads 41.0 K (Aug 6 18:45Z) — 41% of the line.

CURRENT — AUG 6 (last readings)

Compressor ON. Shield temp 41.0 K (18:45Z). Helium 79.4%.

RATES

Shield temp +1.0 K vs baseline (40.0 → 41.0); peak 41.0. Helium –6.50 points.

DATA NOTES

1,478 captures · 1,478 valid pressure · 1,478 valid helium readings. Charts show the daily min-max range with the daily last value. EDU (1,478 captures): room 73.8–73.8 °F · probes 74.5–74.5 / 76.0–76.0 °F · humidity 51–51%.