




CNN for PH01-00 using uncalibrated pressure values

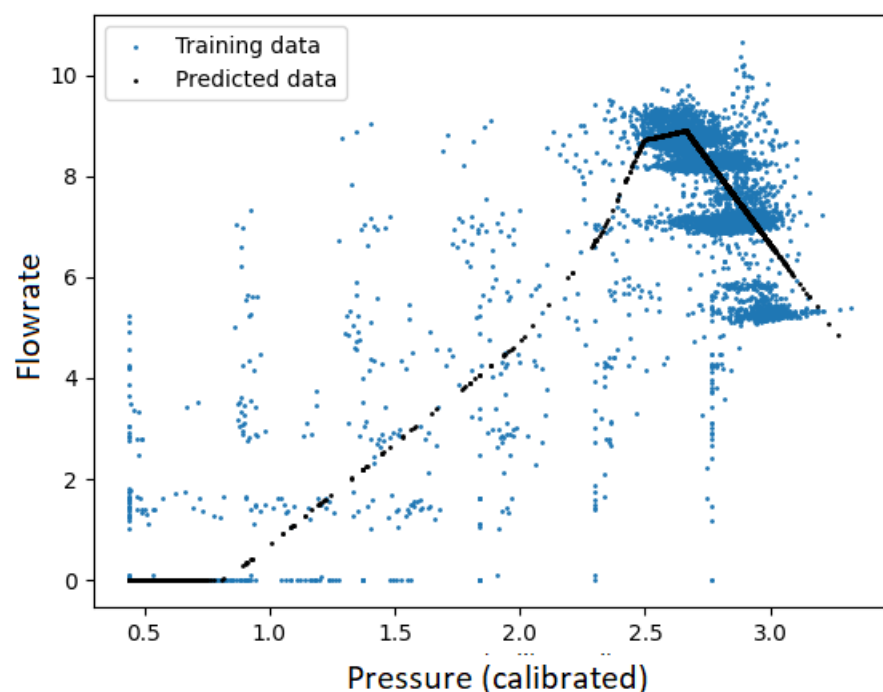

CNN for PH01-00 using calibrated pressure values

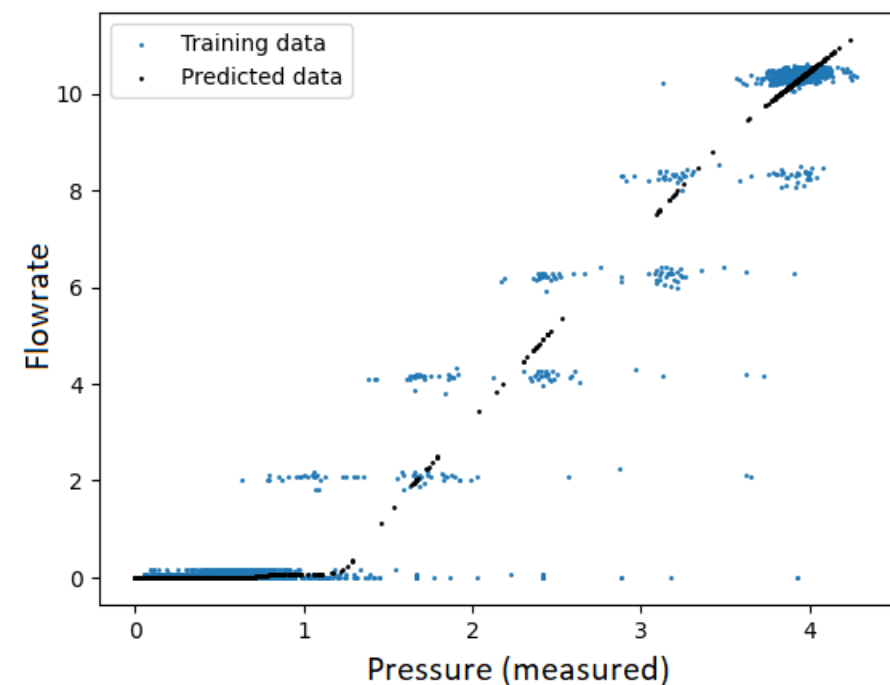

CNN for PH03-02 using uncalibrated pressure values

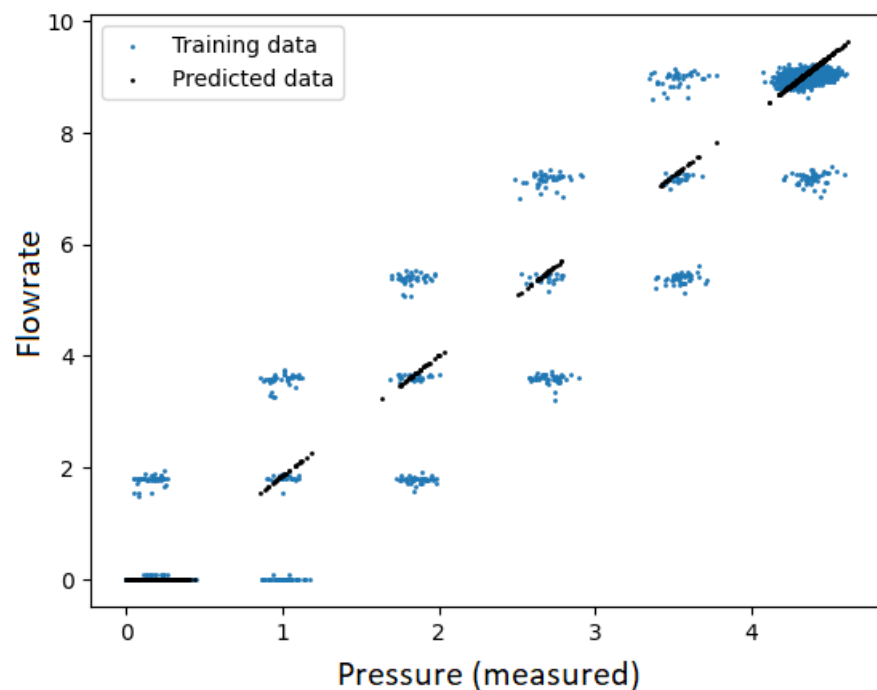

CNN for PH03-03 using uncalibrated pressure values