





Phase 4 — Calibration & Statistical Validation

Calibration Quality: 91.5/100 Statistical Rigor: 100.0/100


score_skew_diagnosis

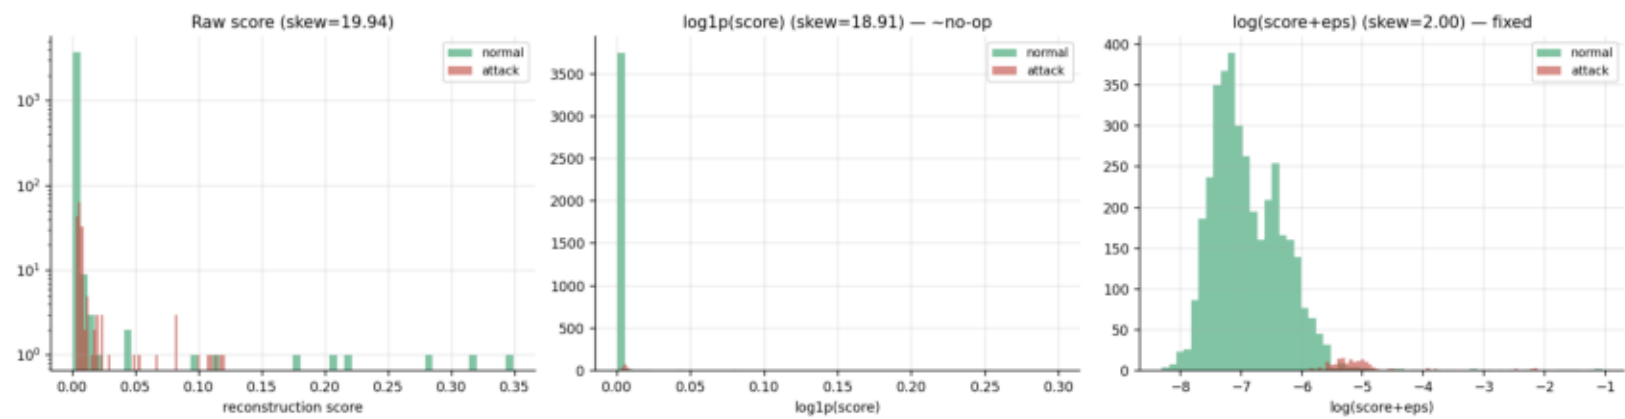


diagnosis_reliability

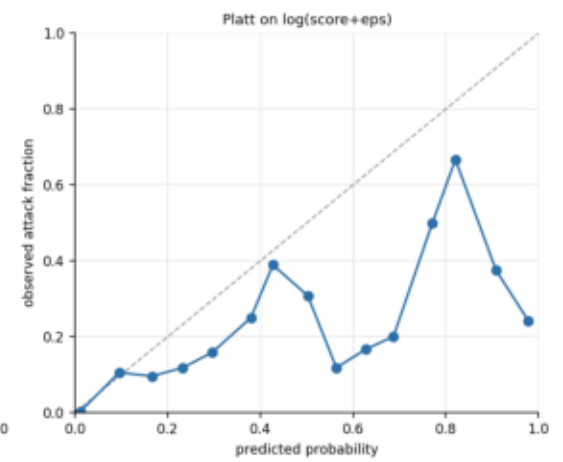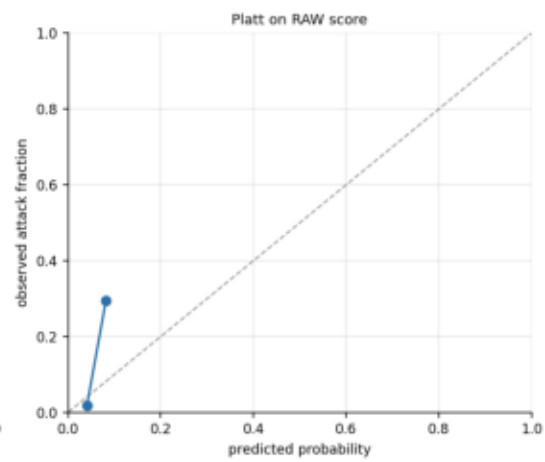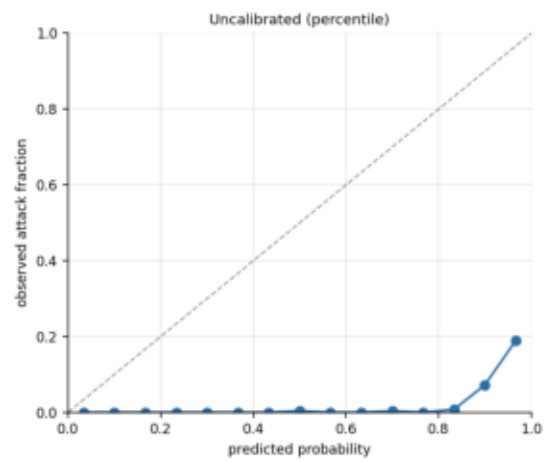




reliability_all_methods

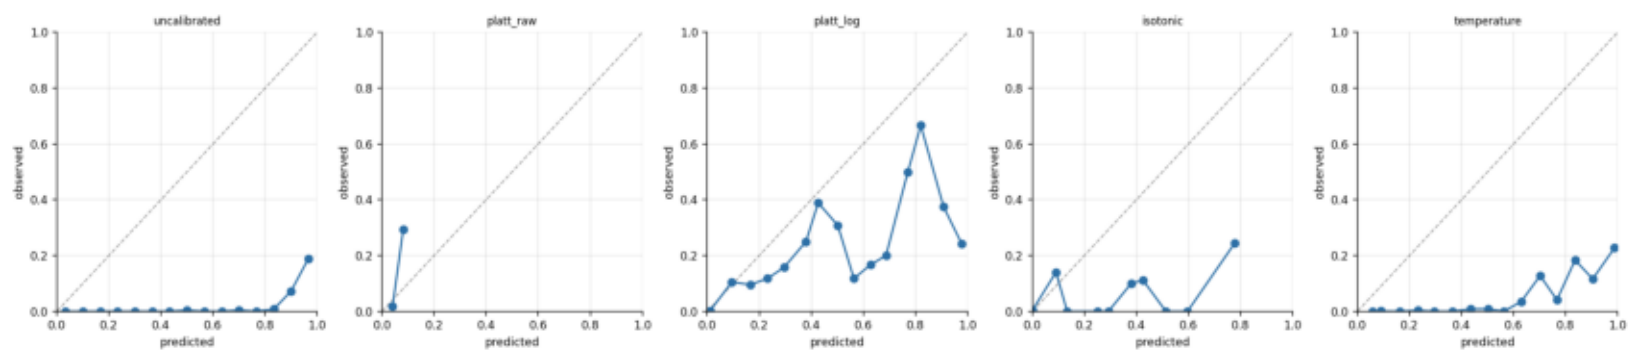

calibration_comparison_bars

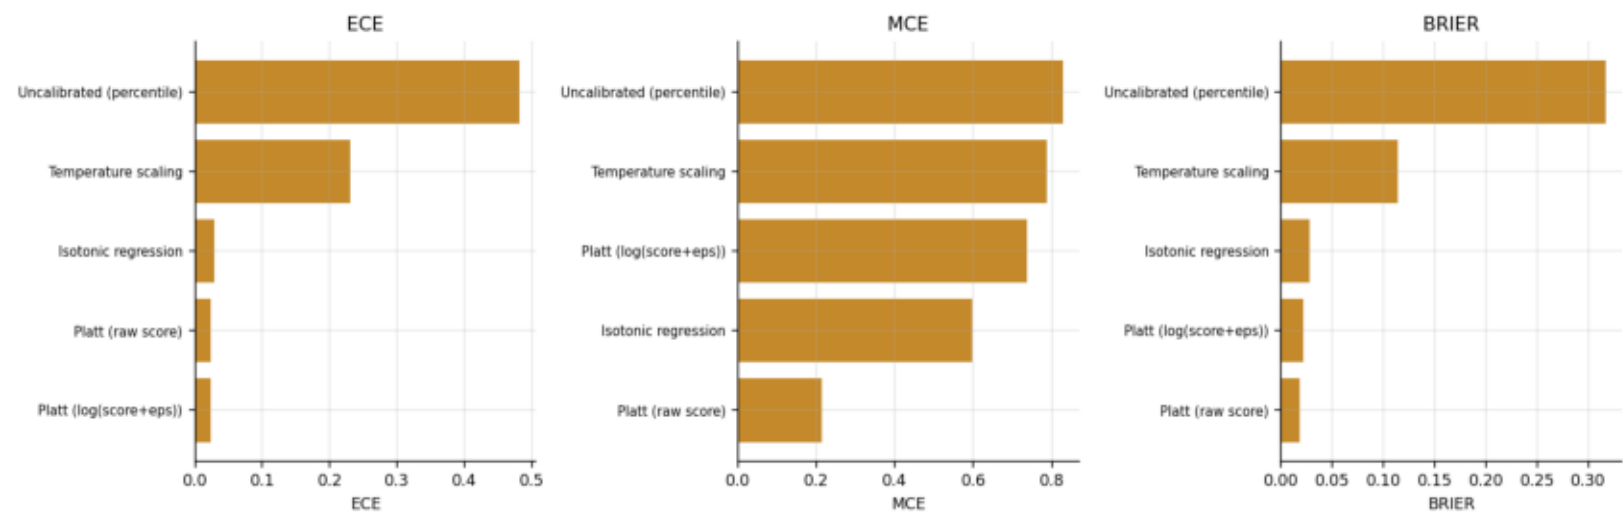


drift_calibration

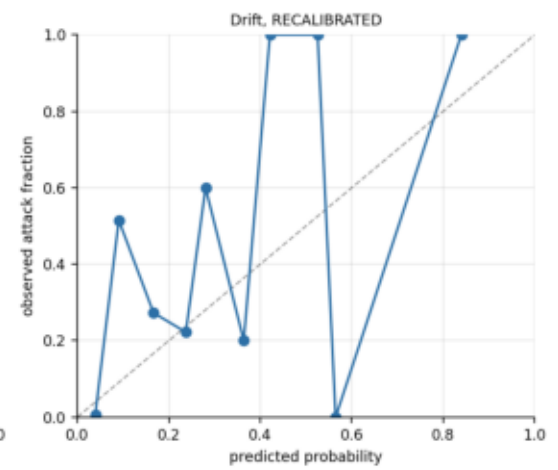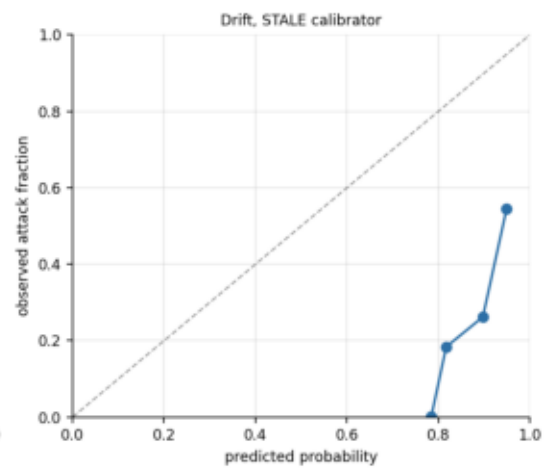
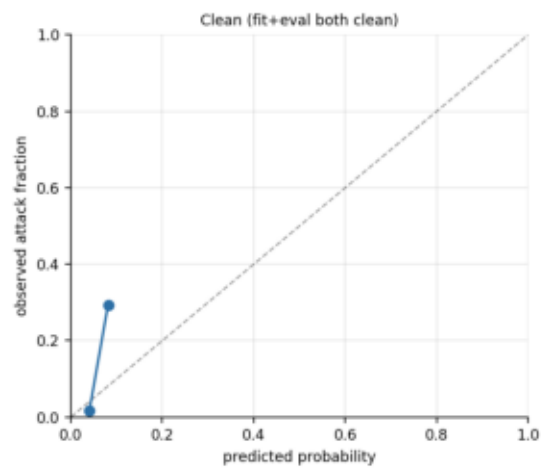


drift_fpr_recovery

FPR recovery via recalibration under drift

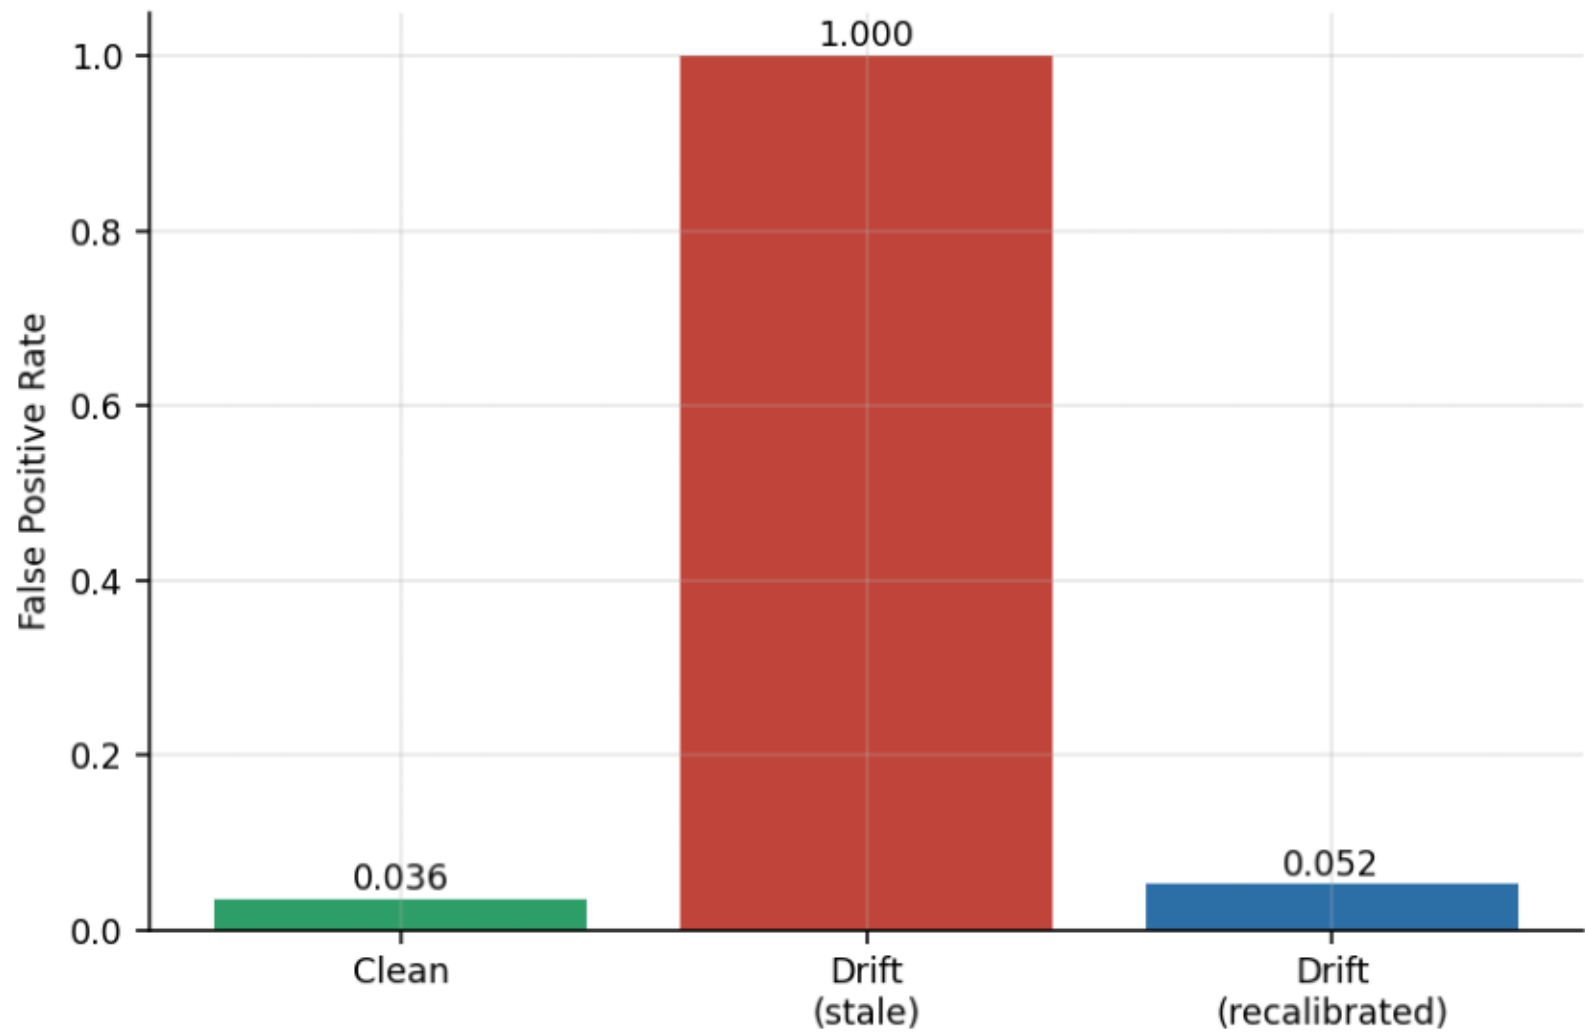

summary_dashboard

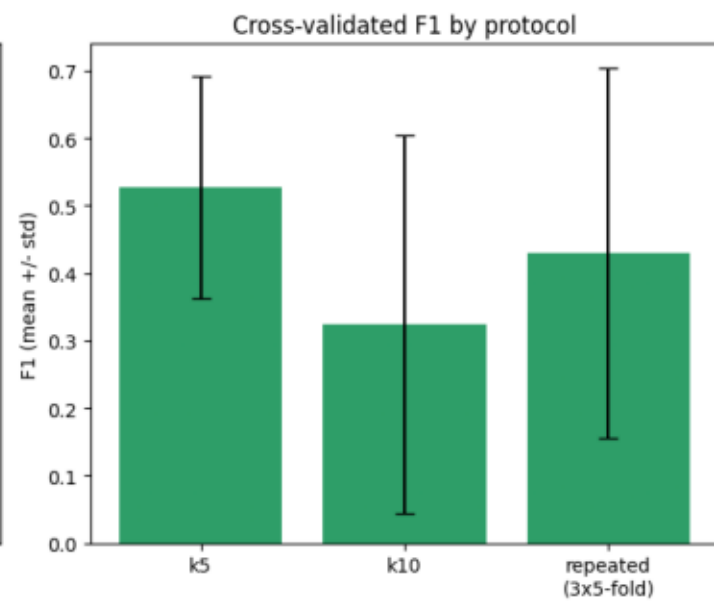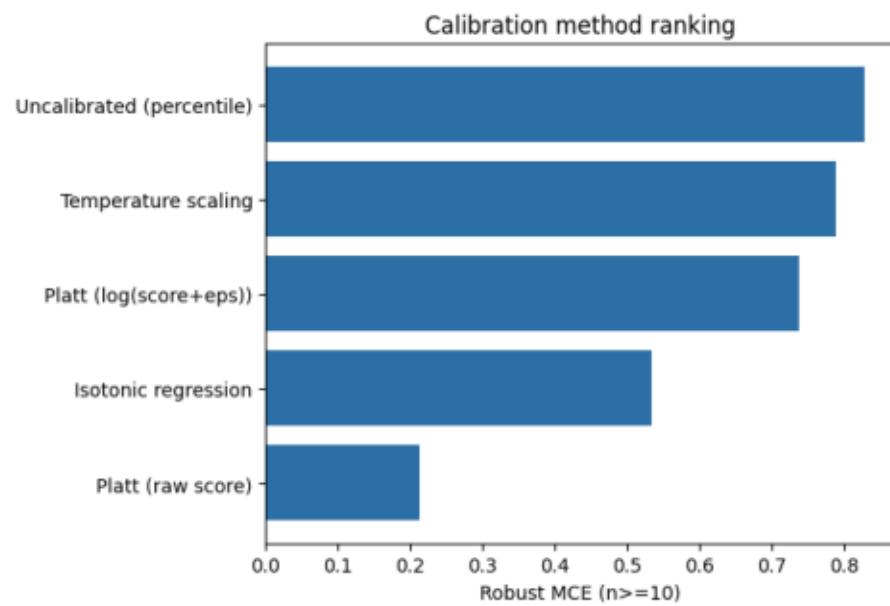

threshold_sensitivity

