


Phase 5b — SGCC Real-Data Validation

Consumer-level · leak-free · honest synthetic-vs-real comparison


benchmark

SGCC consumer-level benchmark

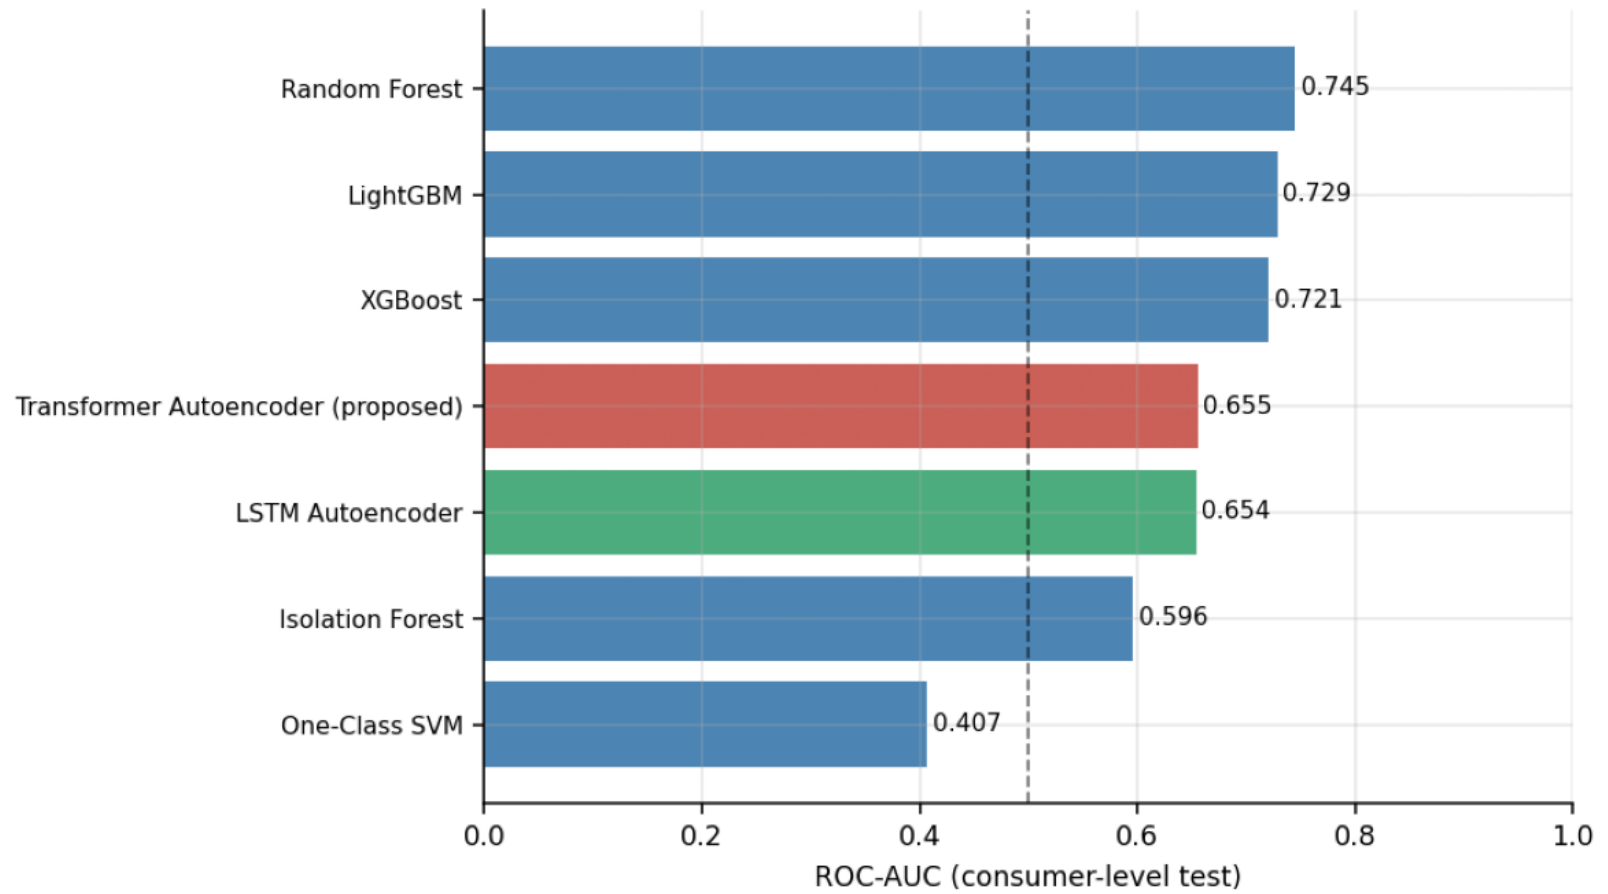


literature

SGCC: ours vs published

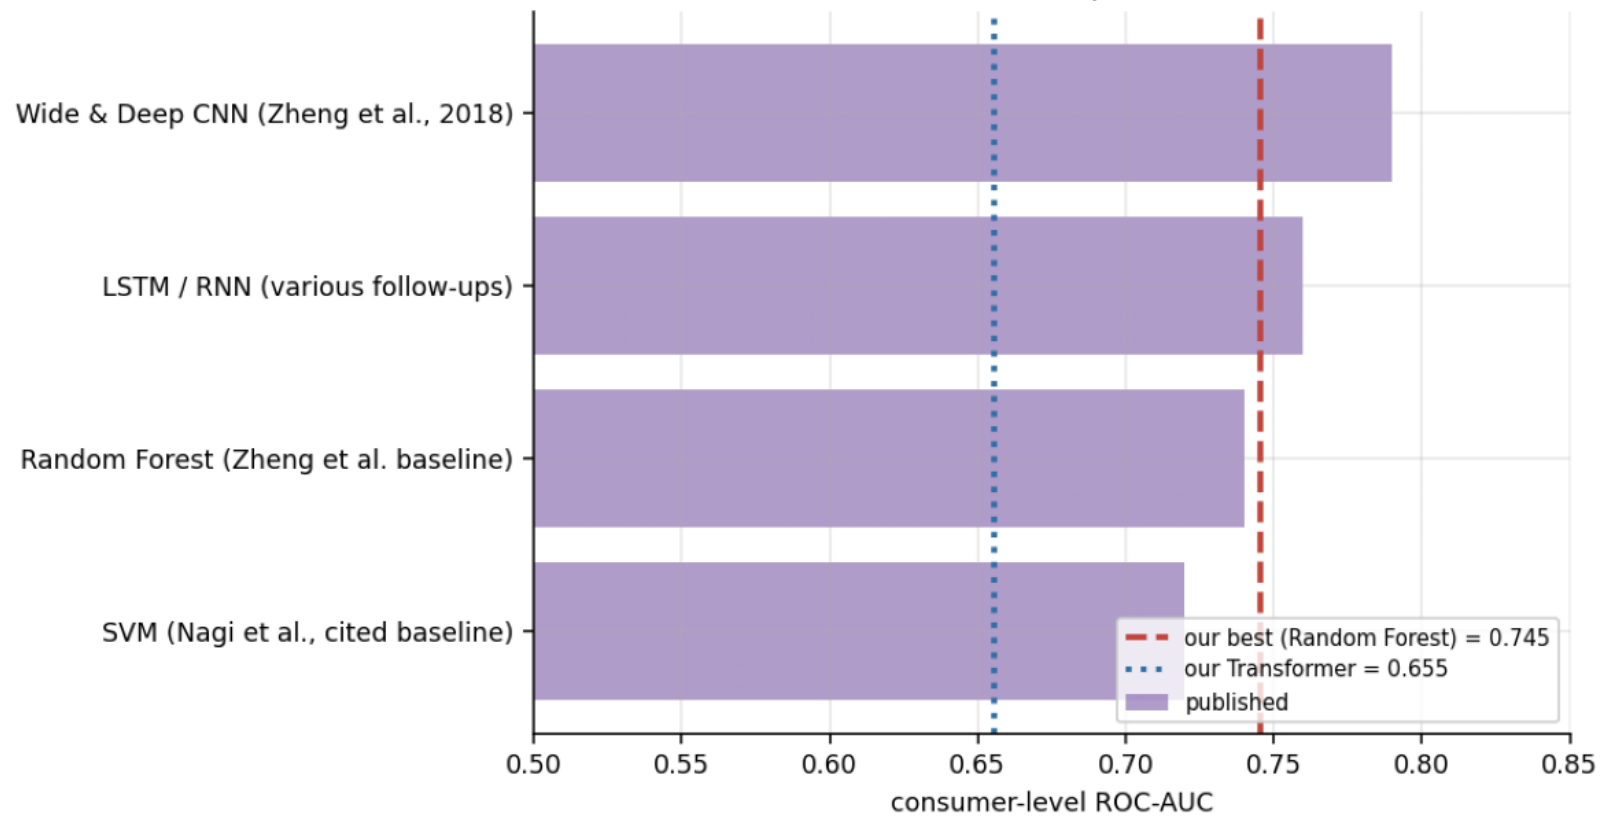

ablation

SGCC ablation — does attention help on real data?

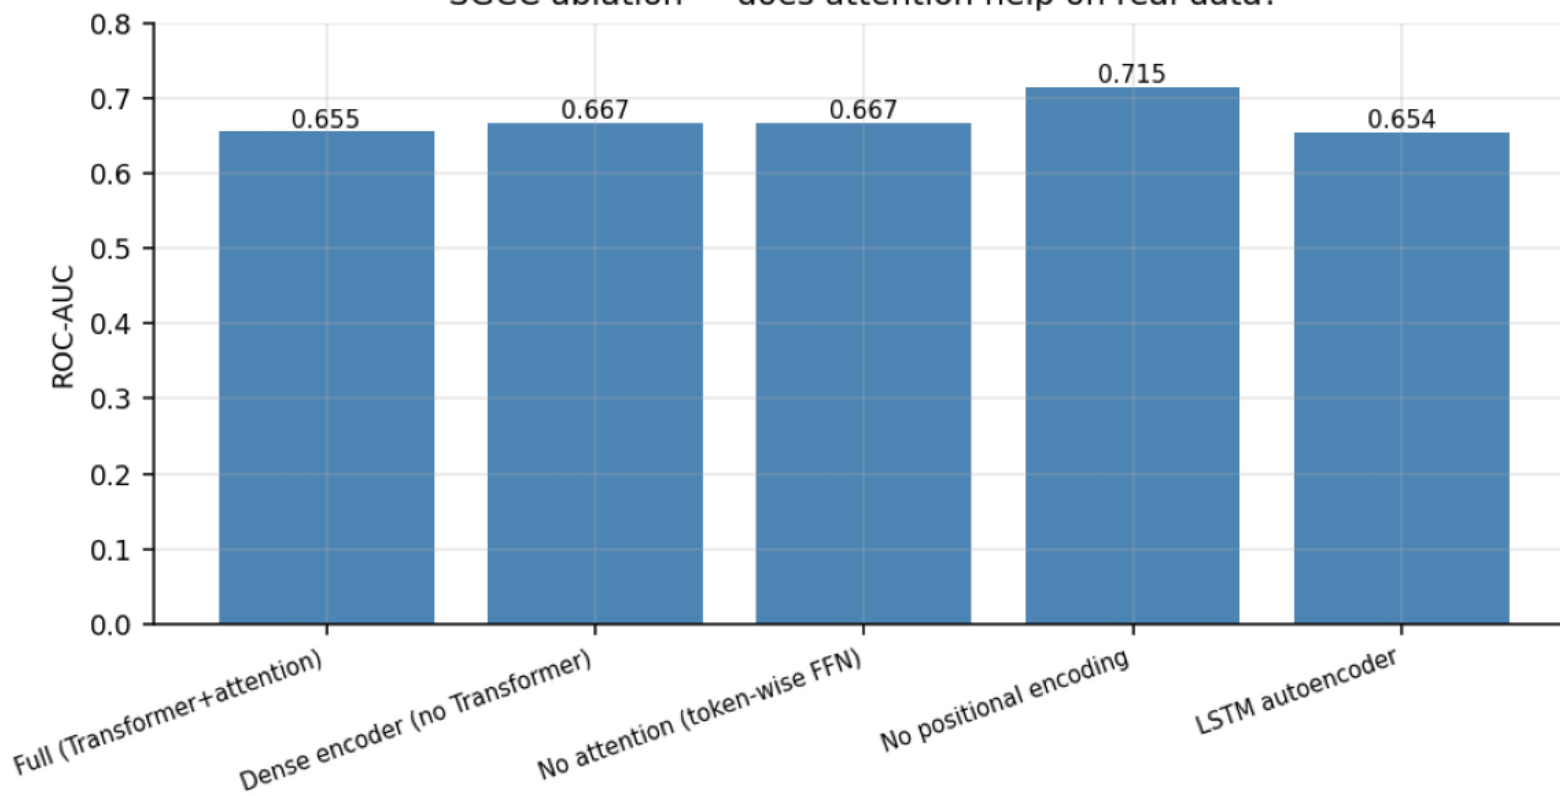

sgcc_calibration

SGCC calibration (Platt-on-raw)
ECE=0.0014 Brier=0.0769

