





5




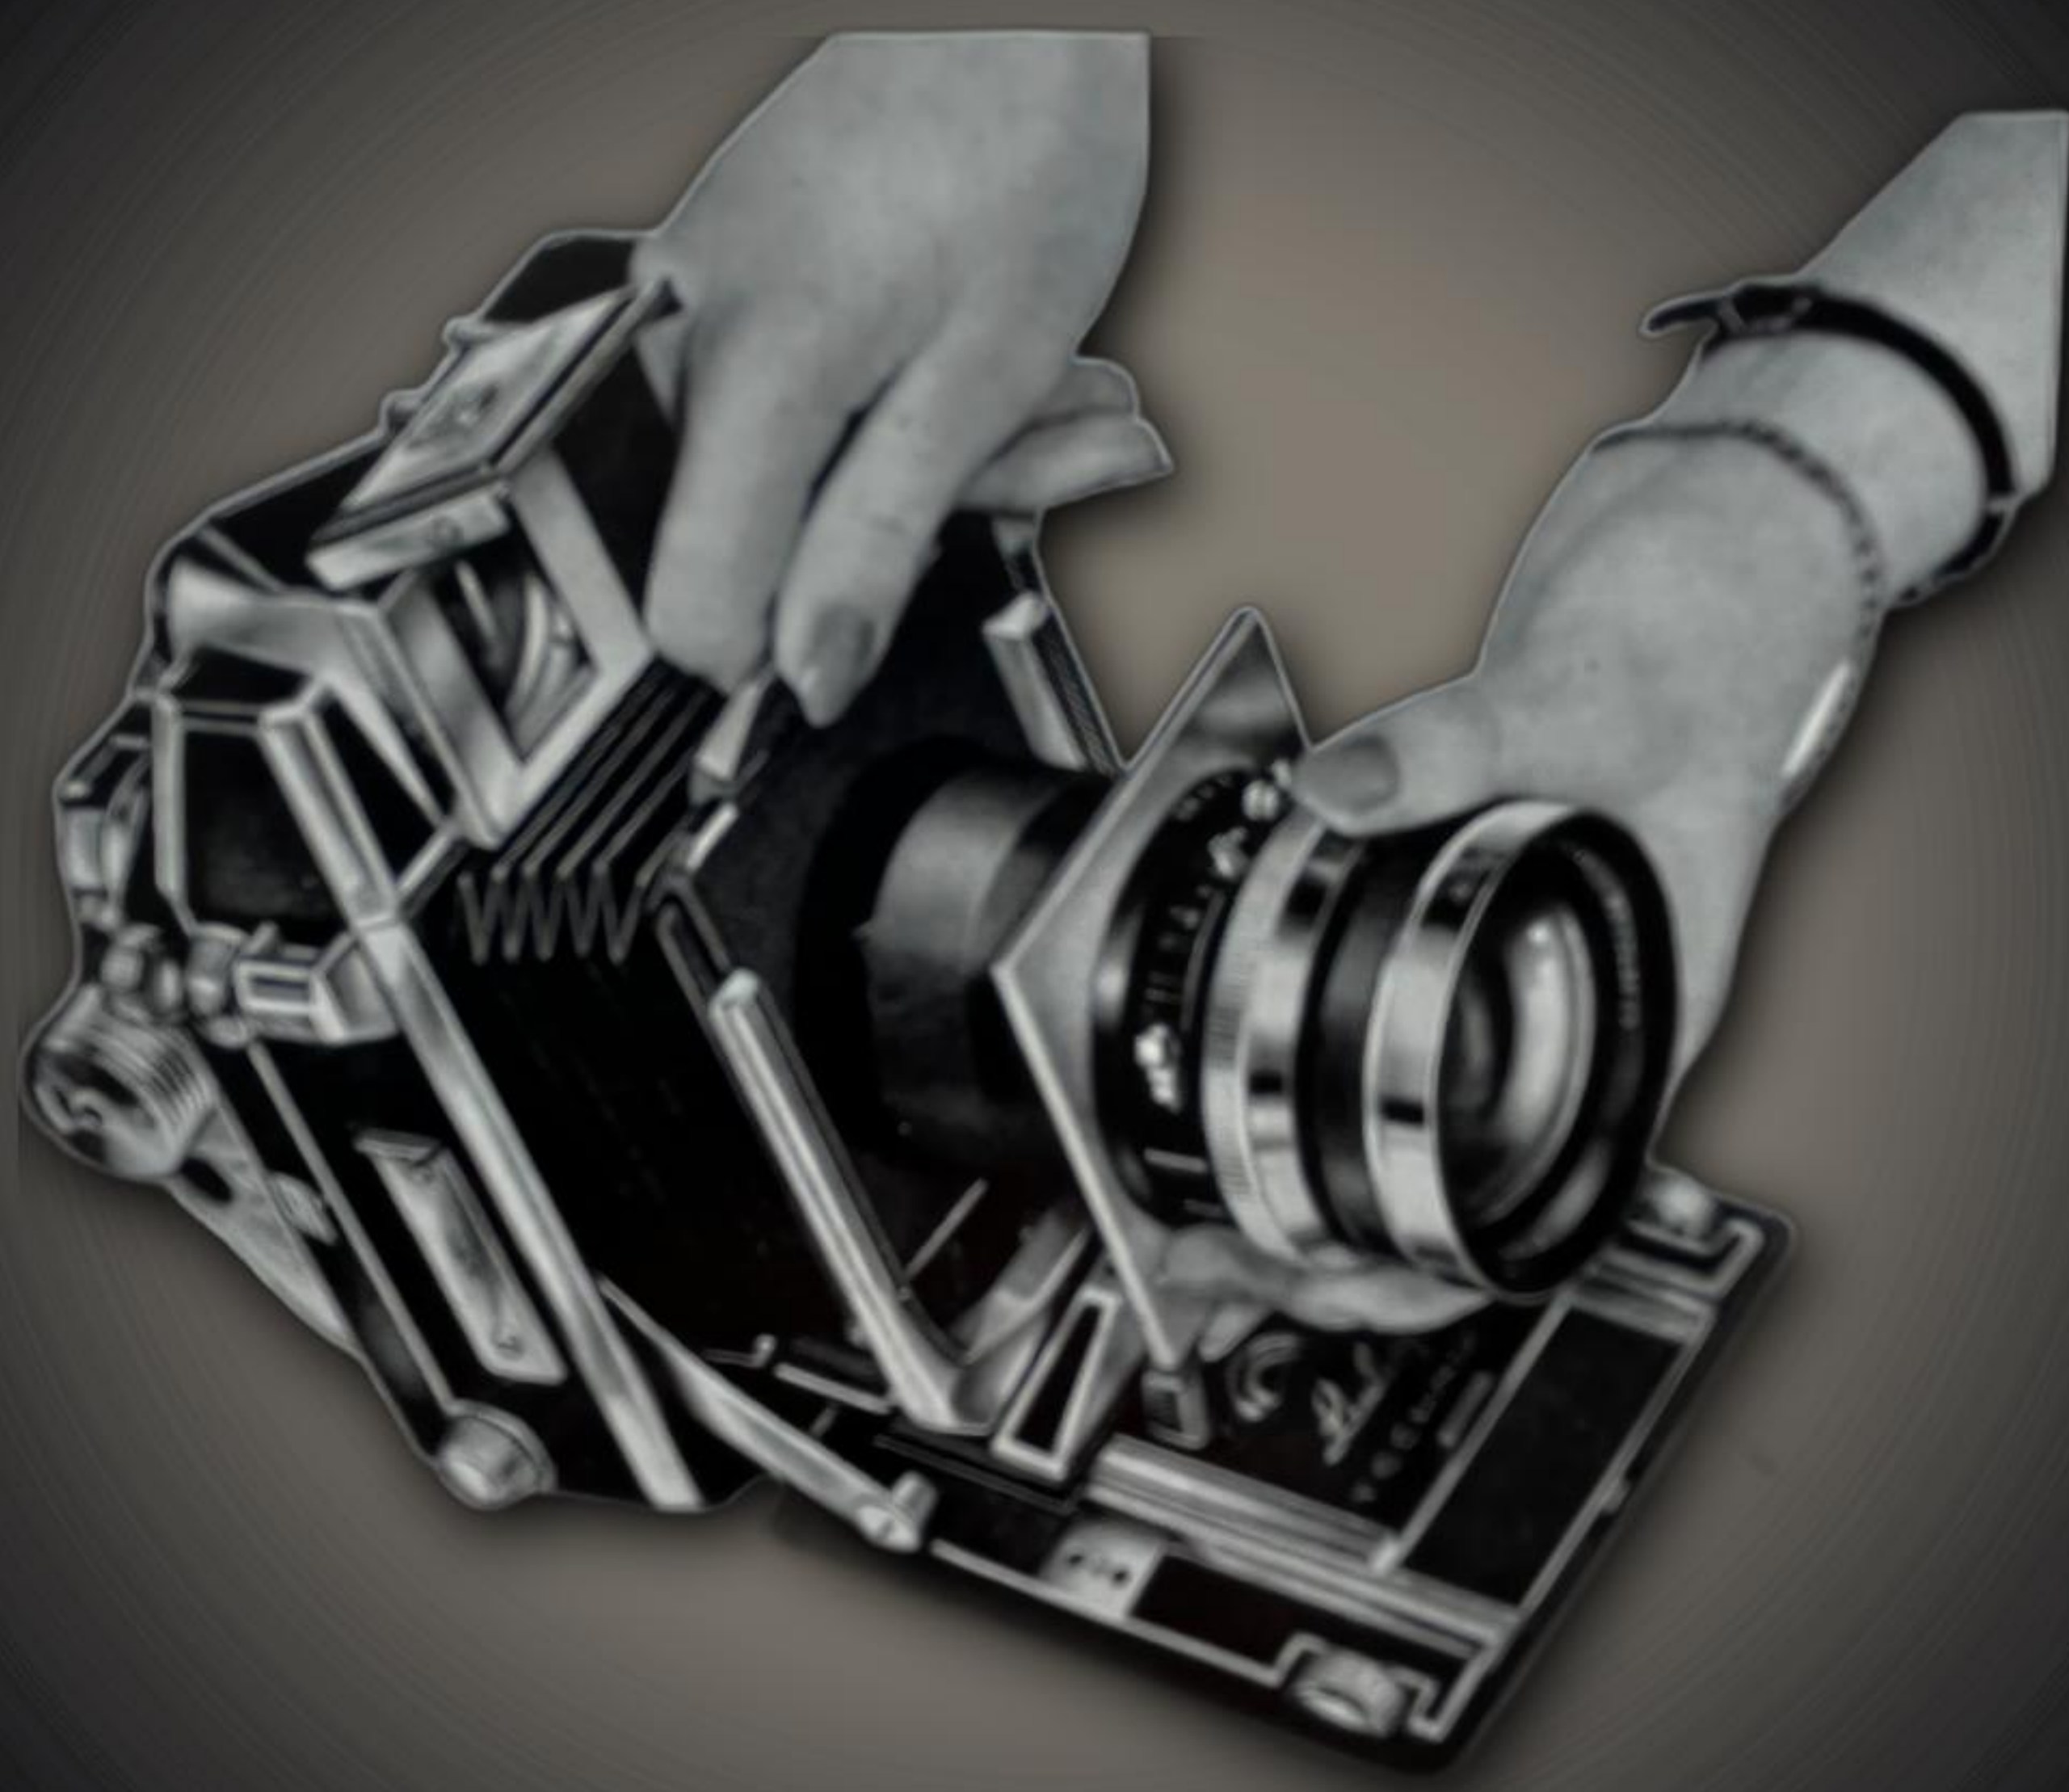

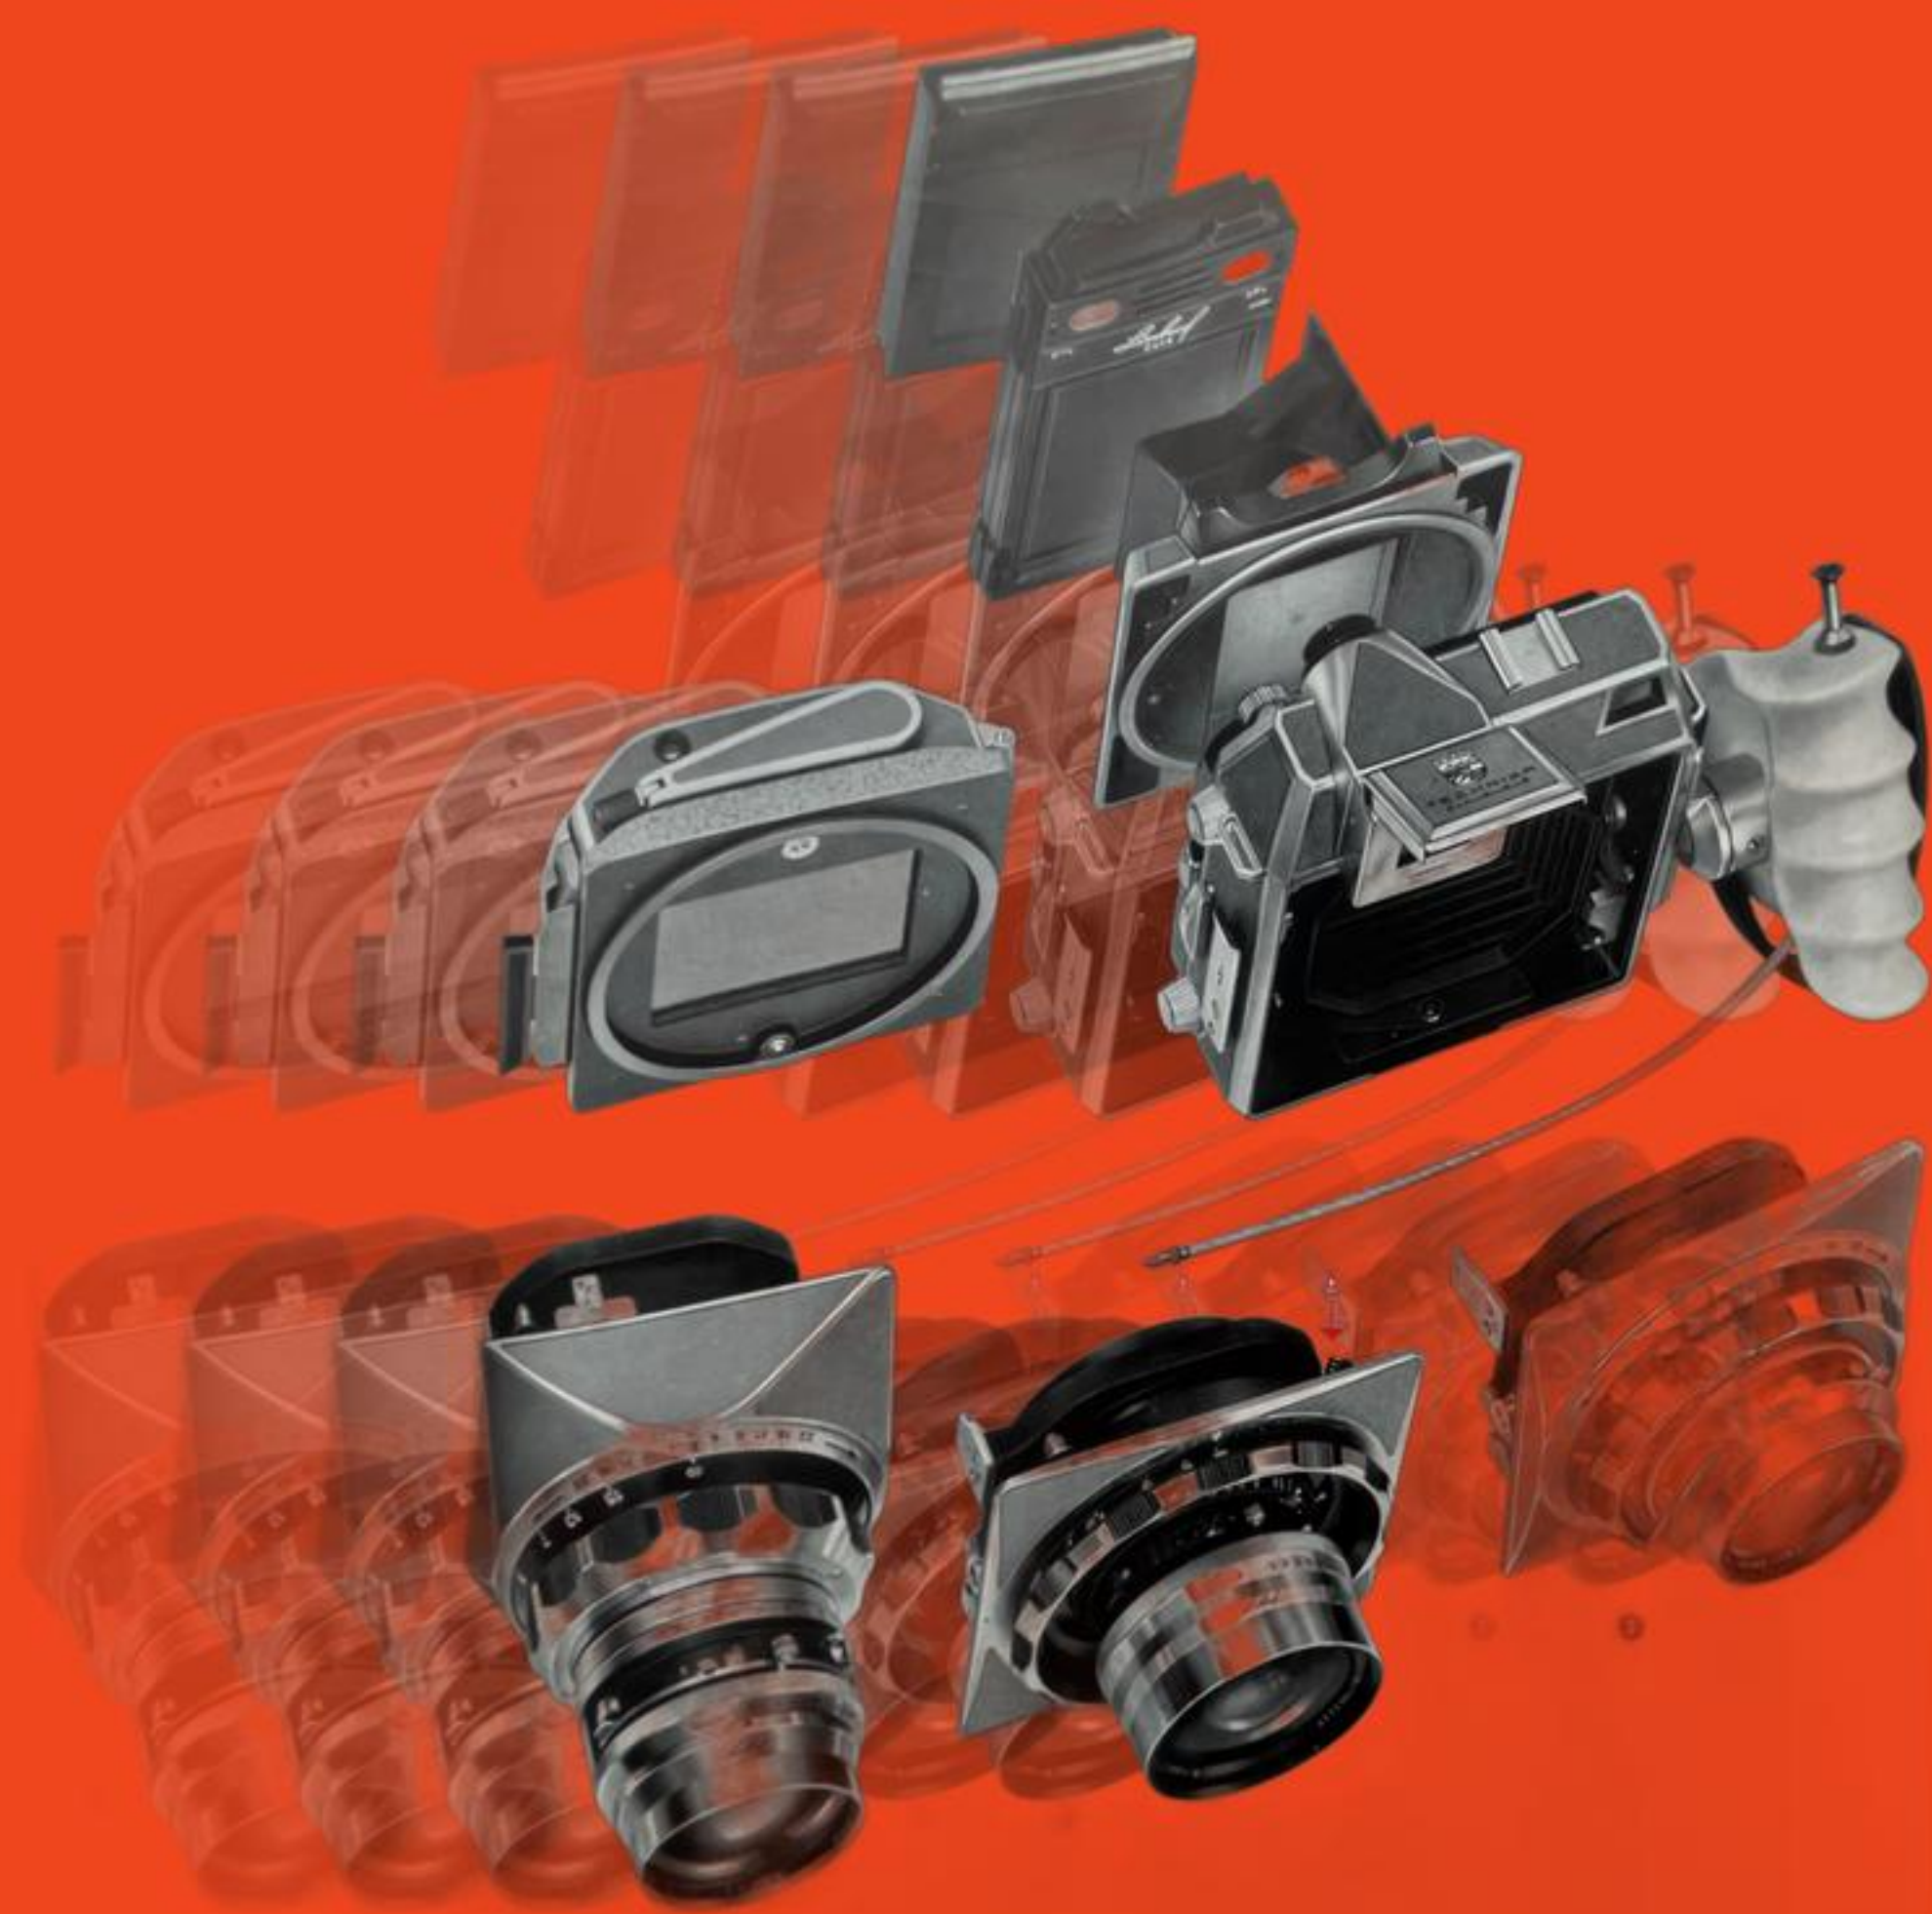



Contaflex of Zeiss Ikon, the first camera designed for color image. The Contaflex line.

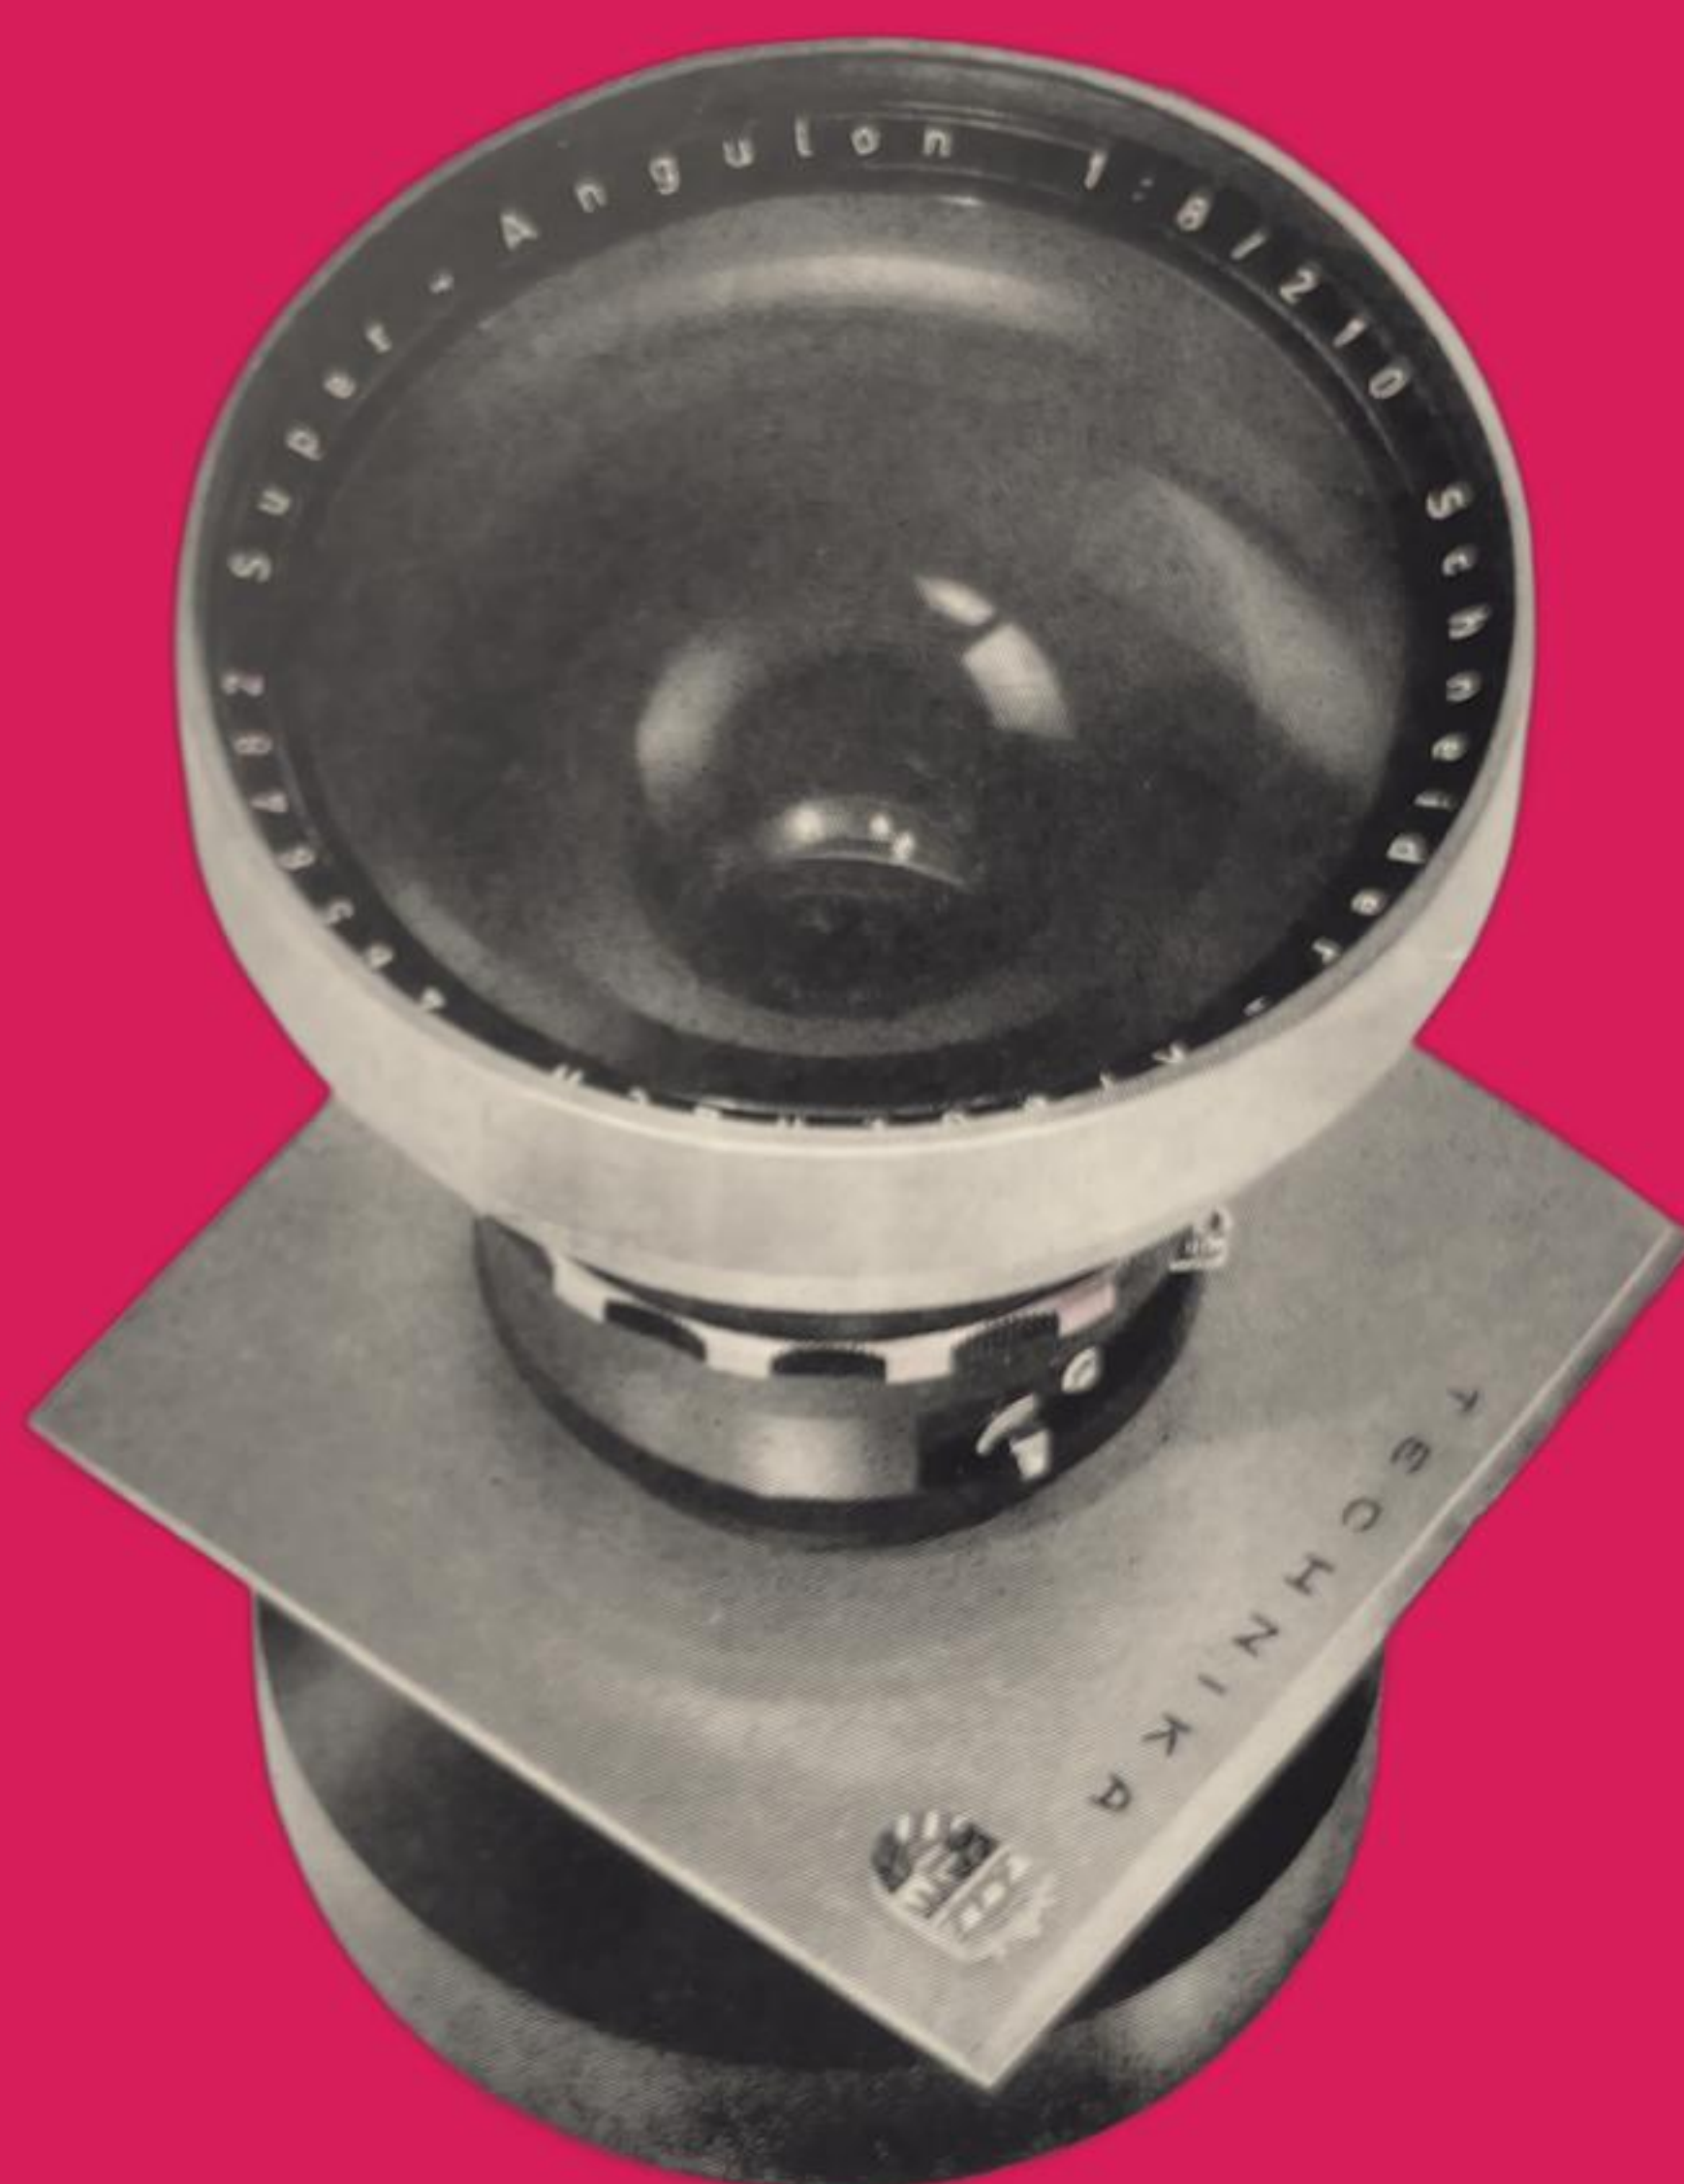











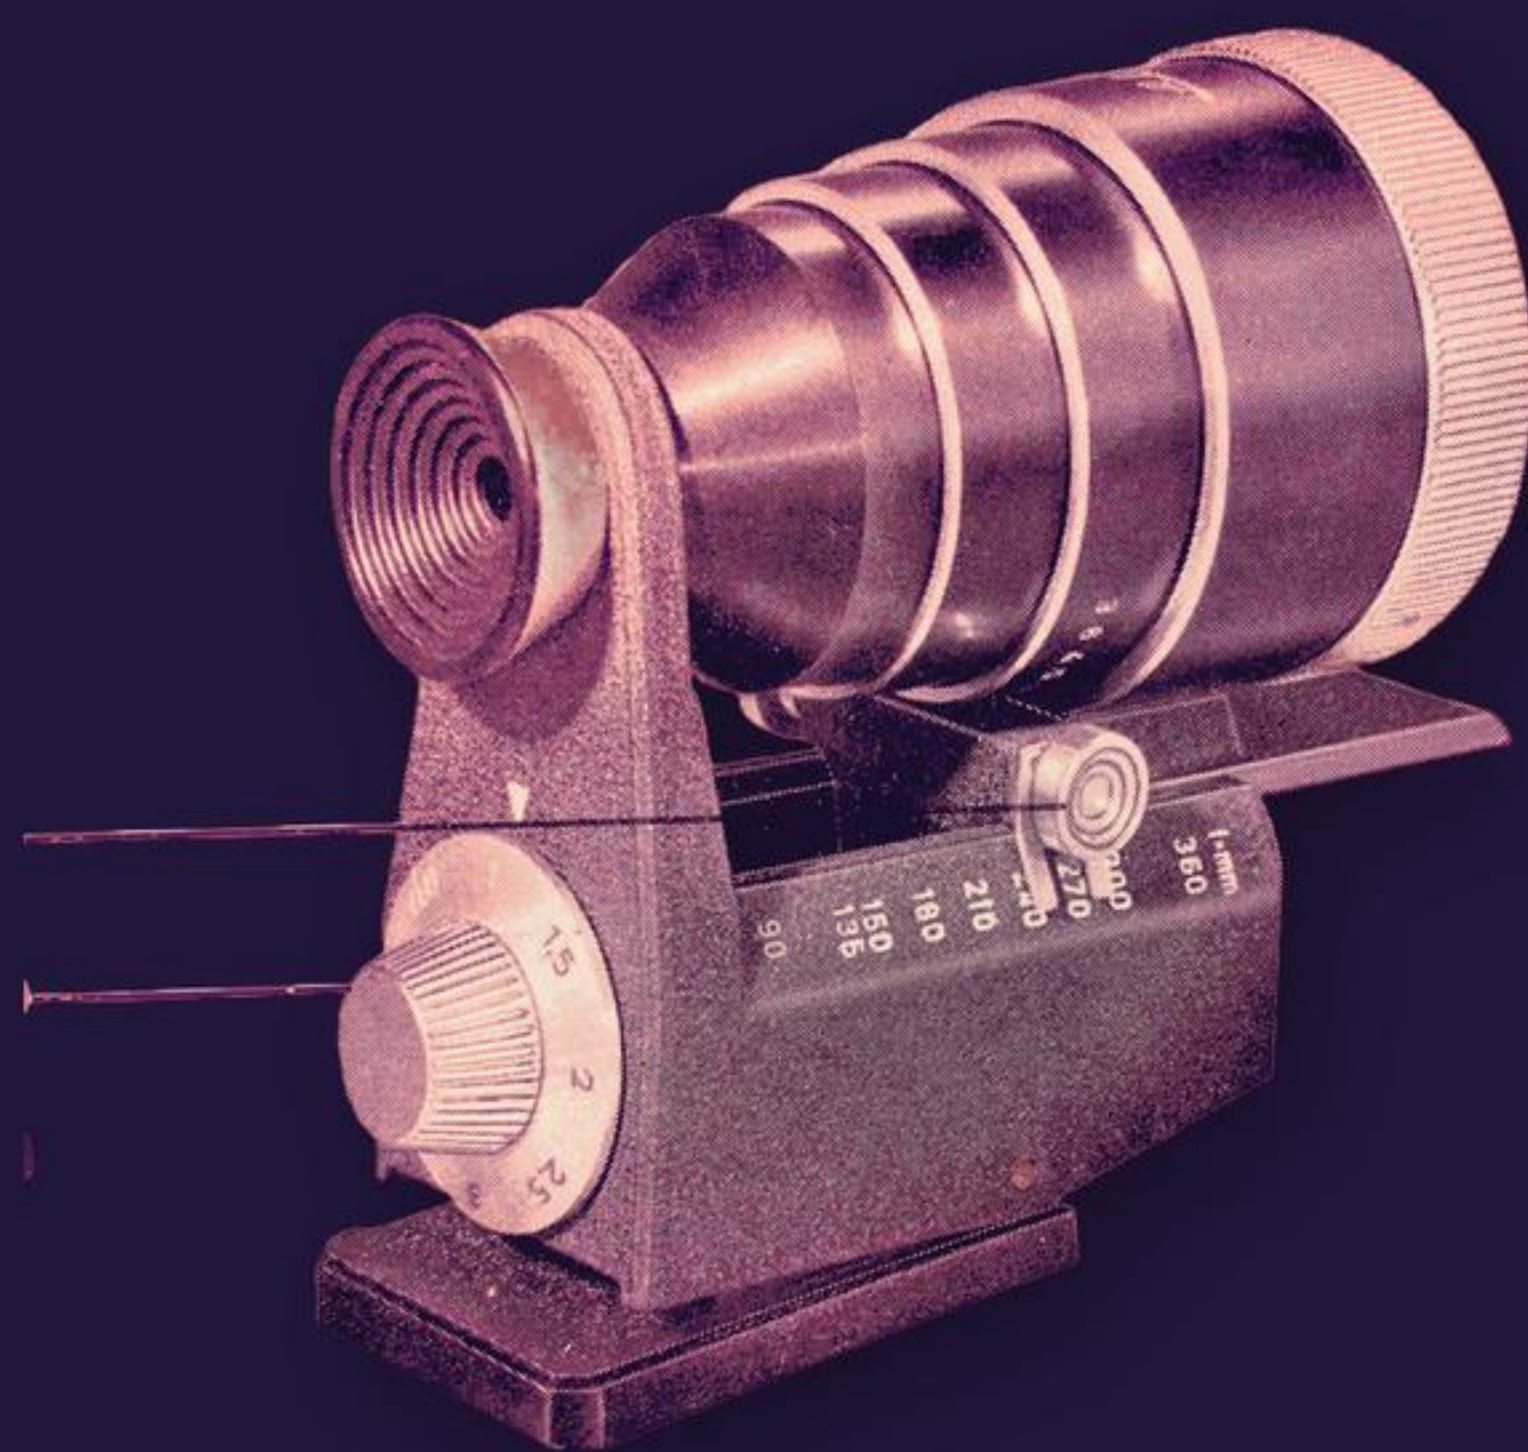


Fig. 47. (a) The microscope is set up for the parallel measurement of the angle of incidence of the light on the surface of the specimen. (b) The microscope is set up for the parallel measurement of the angle of reflection of the light on the surface of the specimen.

or to ② (Fig. 48) for the parallel measurement of the angle of reflection of the light on the surface of the specimen. After slipping the two locking screws on the scale until it audibly clicks, the

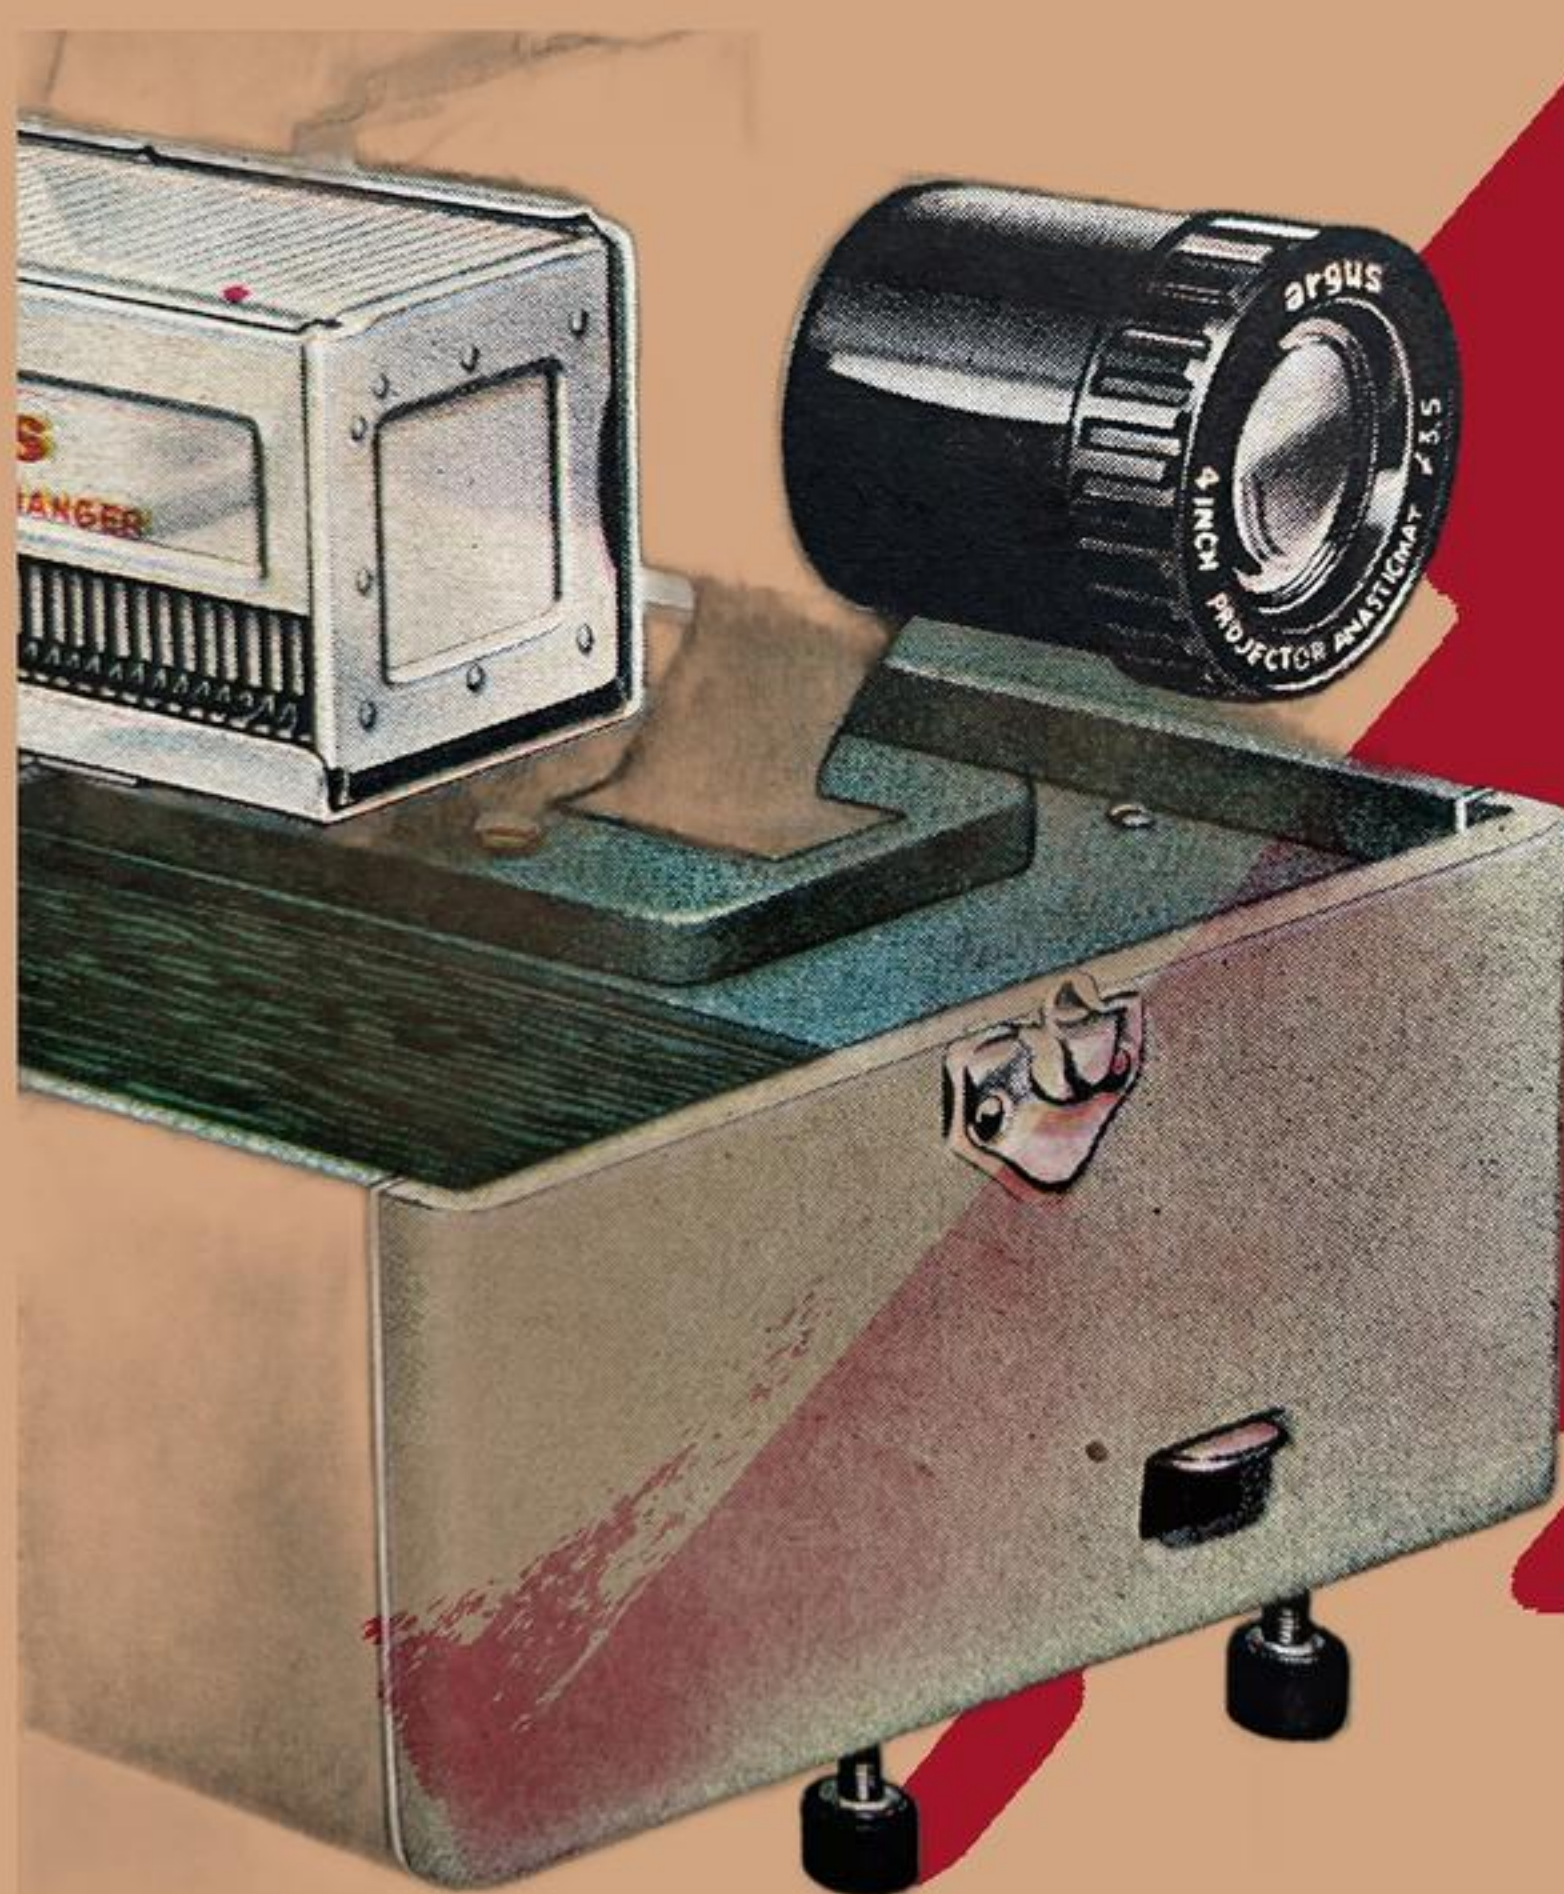

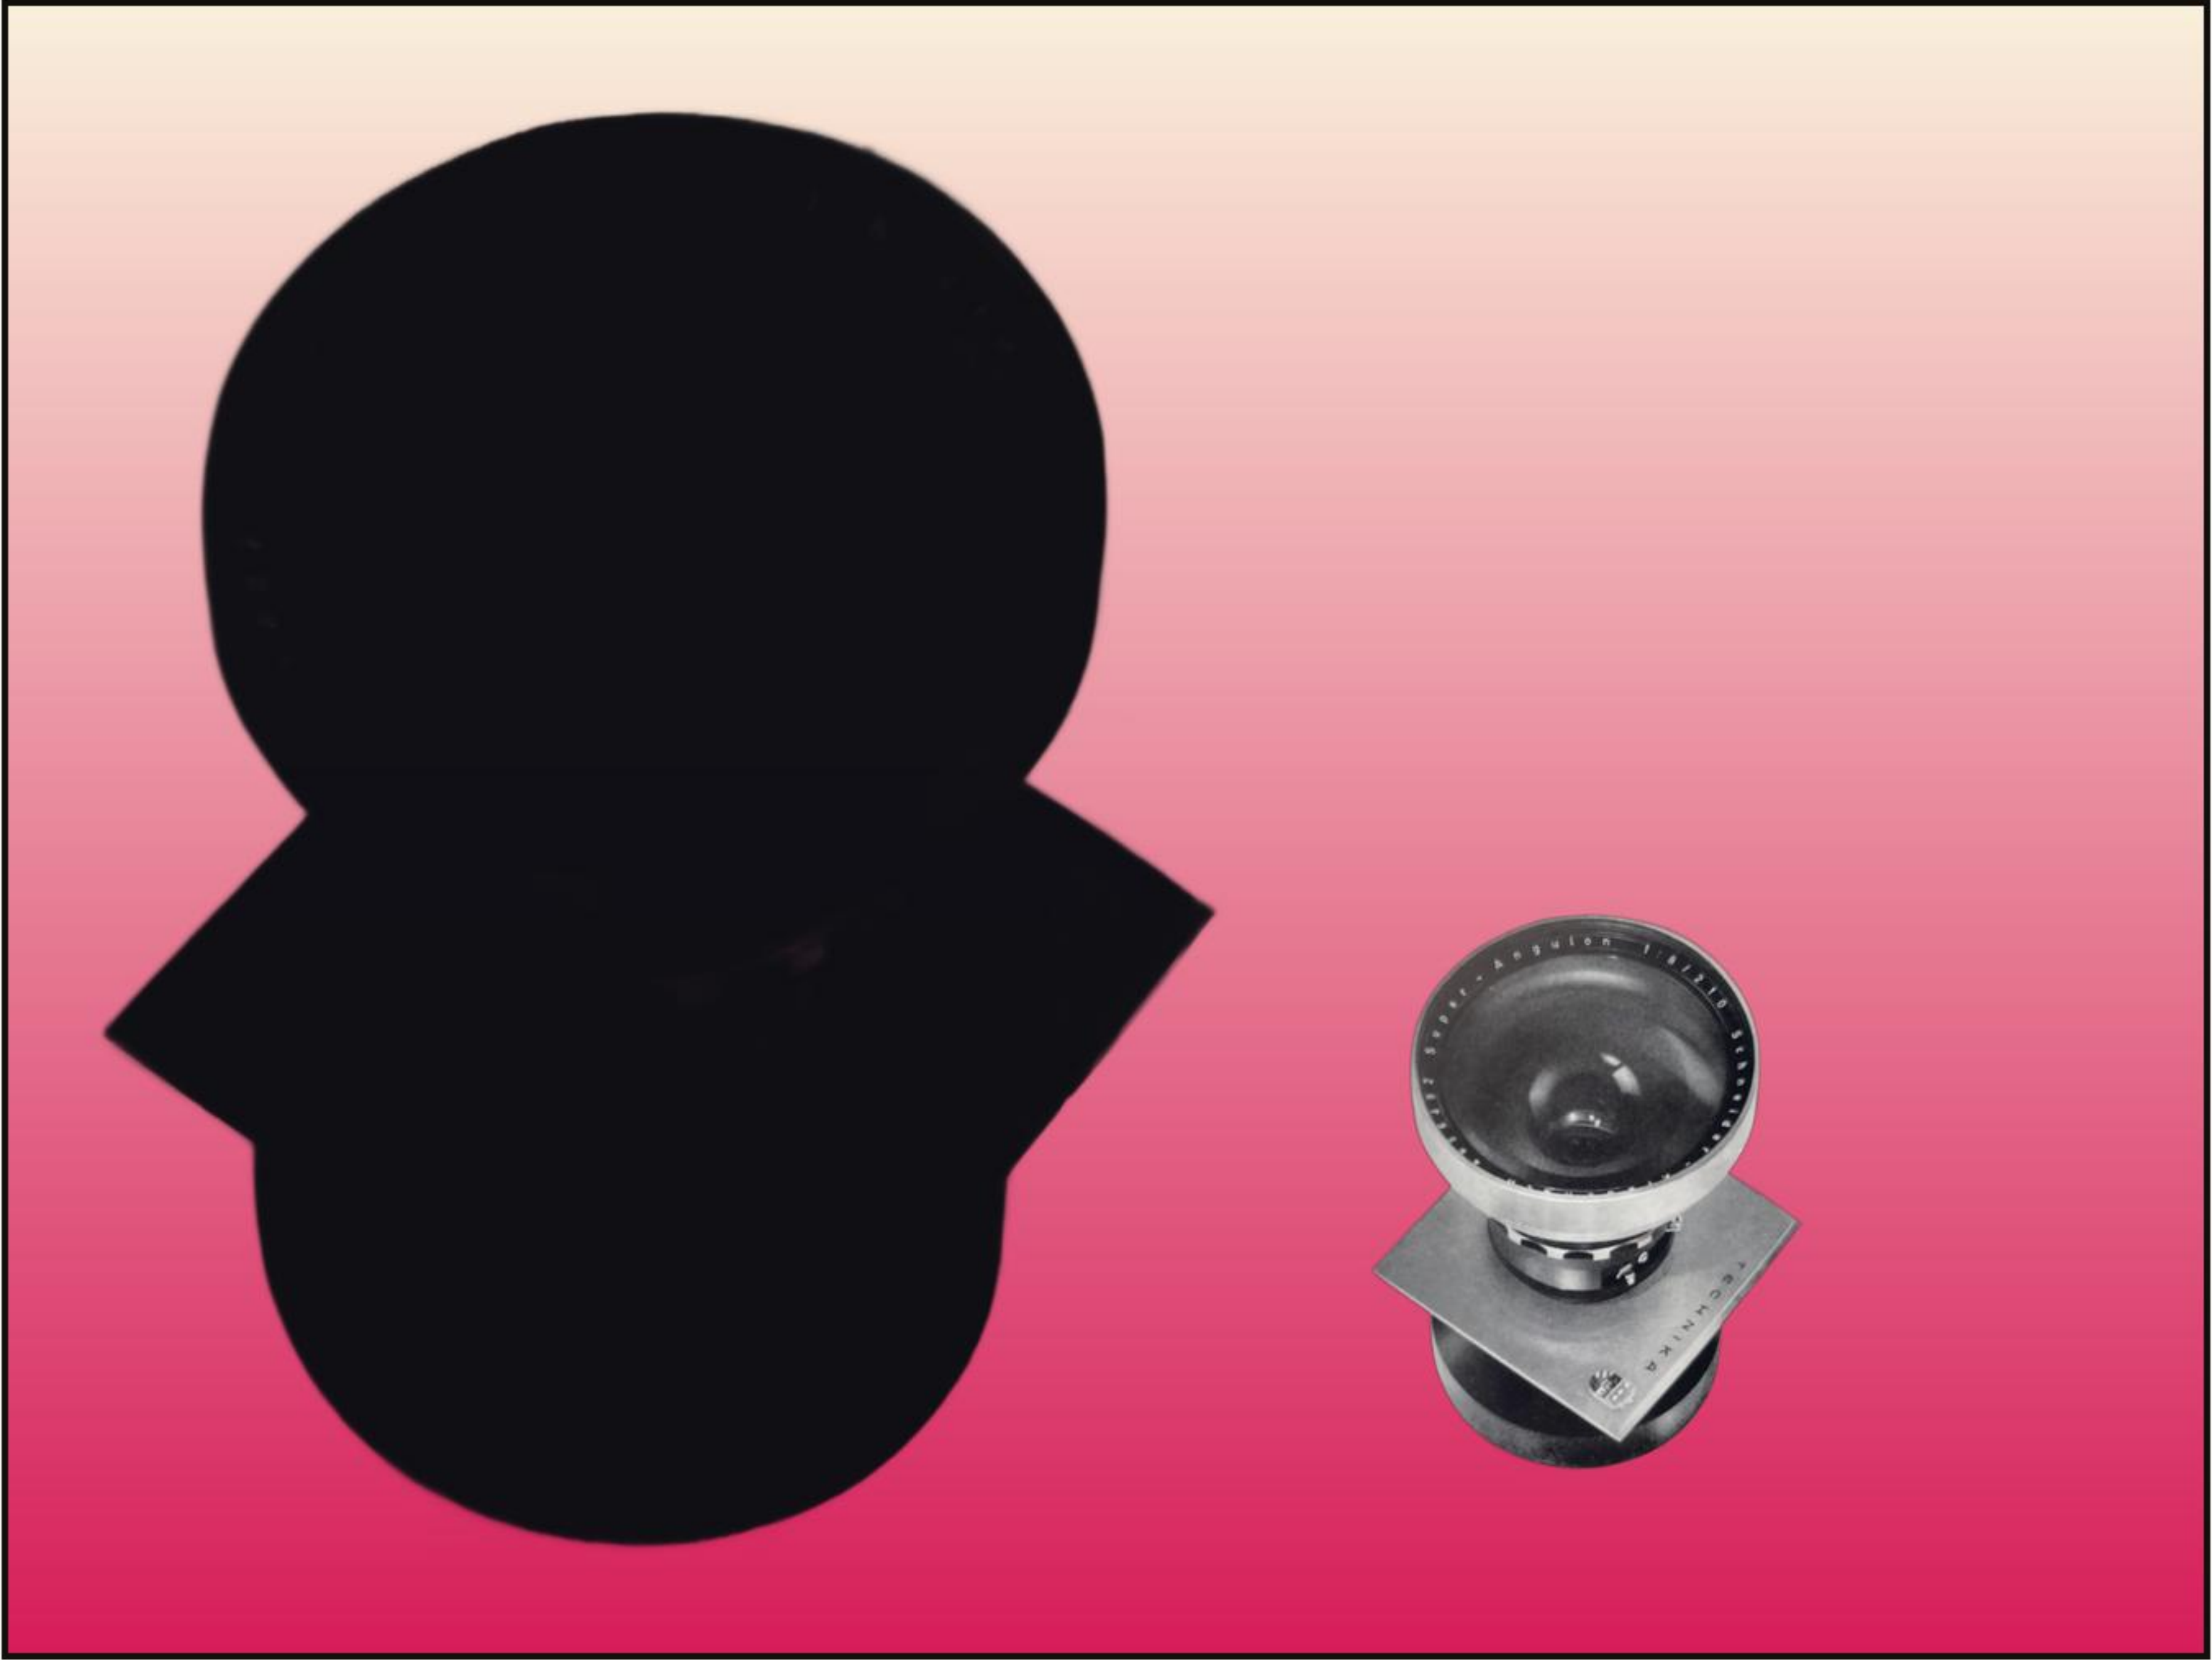

CAMERA OPTICS

Original and found photographs, segmented and collaged by Mark Ghuneim

ISSUE V

Edition of 100 + 10 AP

No. _____ / 100