
RehabPose session report: Shoulder flexion

Session synthetic-sample · user synthetic-demo · side R · sagittal view · synthetic · started 2026-01-15T10:00:00+00:00

Disclaimer. RehabPose is a research and portfolio prototype. It is not a medical device, has not been clinically validated, and must not be used to diagnose, treat, or replace advice from a qualified healthcare professional. Stop exercising if you feel pain. Thresholds are engineering defaults, not clinical prescriptions.

SYNTHETIC sample: generated skeletons, not a real person. These numbers are not a measurement.

Reps	6	Target	150°
Active time	46.7 s		
Mean peak	142.9°	Best peak	150.2°
Quality (correct reps)	0.33	Mean similarity	0.900

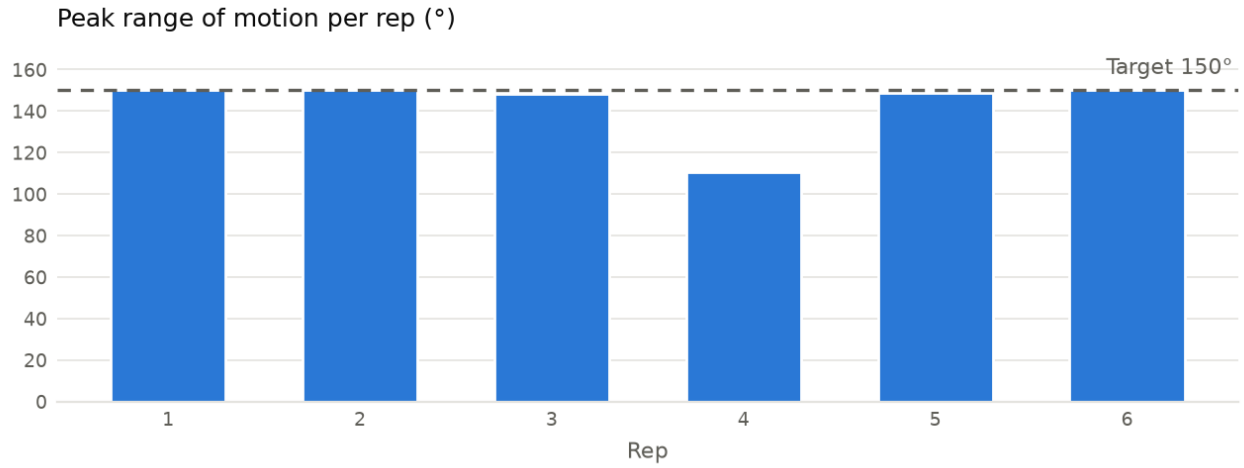


Repetitions

#	Peak°	Duration s	Peak vel /s	DTW similarity	Label	Flags
1	149.9	5.23	75	0.903	correct	–
2	150.0	5.20	74	0.899	compensated	TRUNK_LEAN
3	148.2	5.20	74	0.900	correct	–
4	110.6	4.80	55	0.894	incomplete_rom	INCOMPLETE_ROM
5	148.5	1.30	303	0.903	too_fast	TOO_FAST
6	150.2	5.23	79	0.903	compensated	ELBOW_BEND

DTW similarity compares each rep's shape with a synthetic reference curve, not a recorded movement.

Flags

Reps with each flag: ELBOW_BEND: 1, INCOMPLETE_ROM: 1, TOO_FAST: 1, TRUNK_LEAN: 1. Flag events: 5.

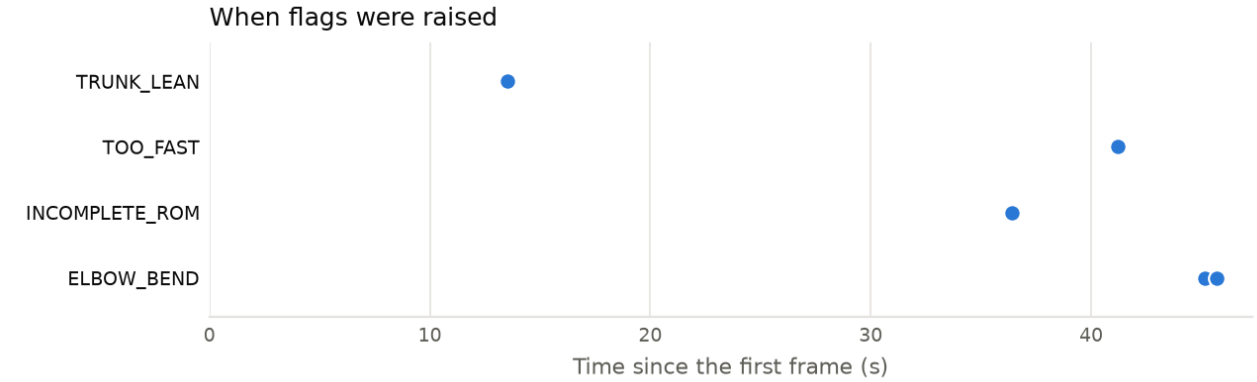

Model/version: synthetic-generator|rules · report v1 · generated 2026-11-01T17:26:01+00:00