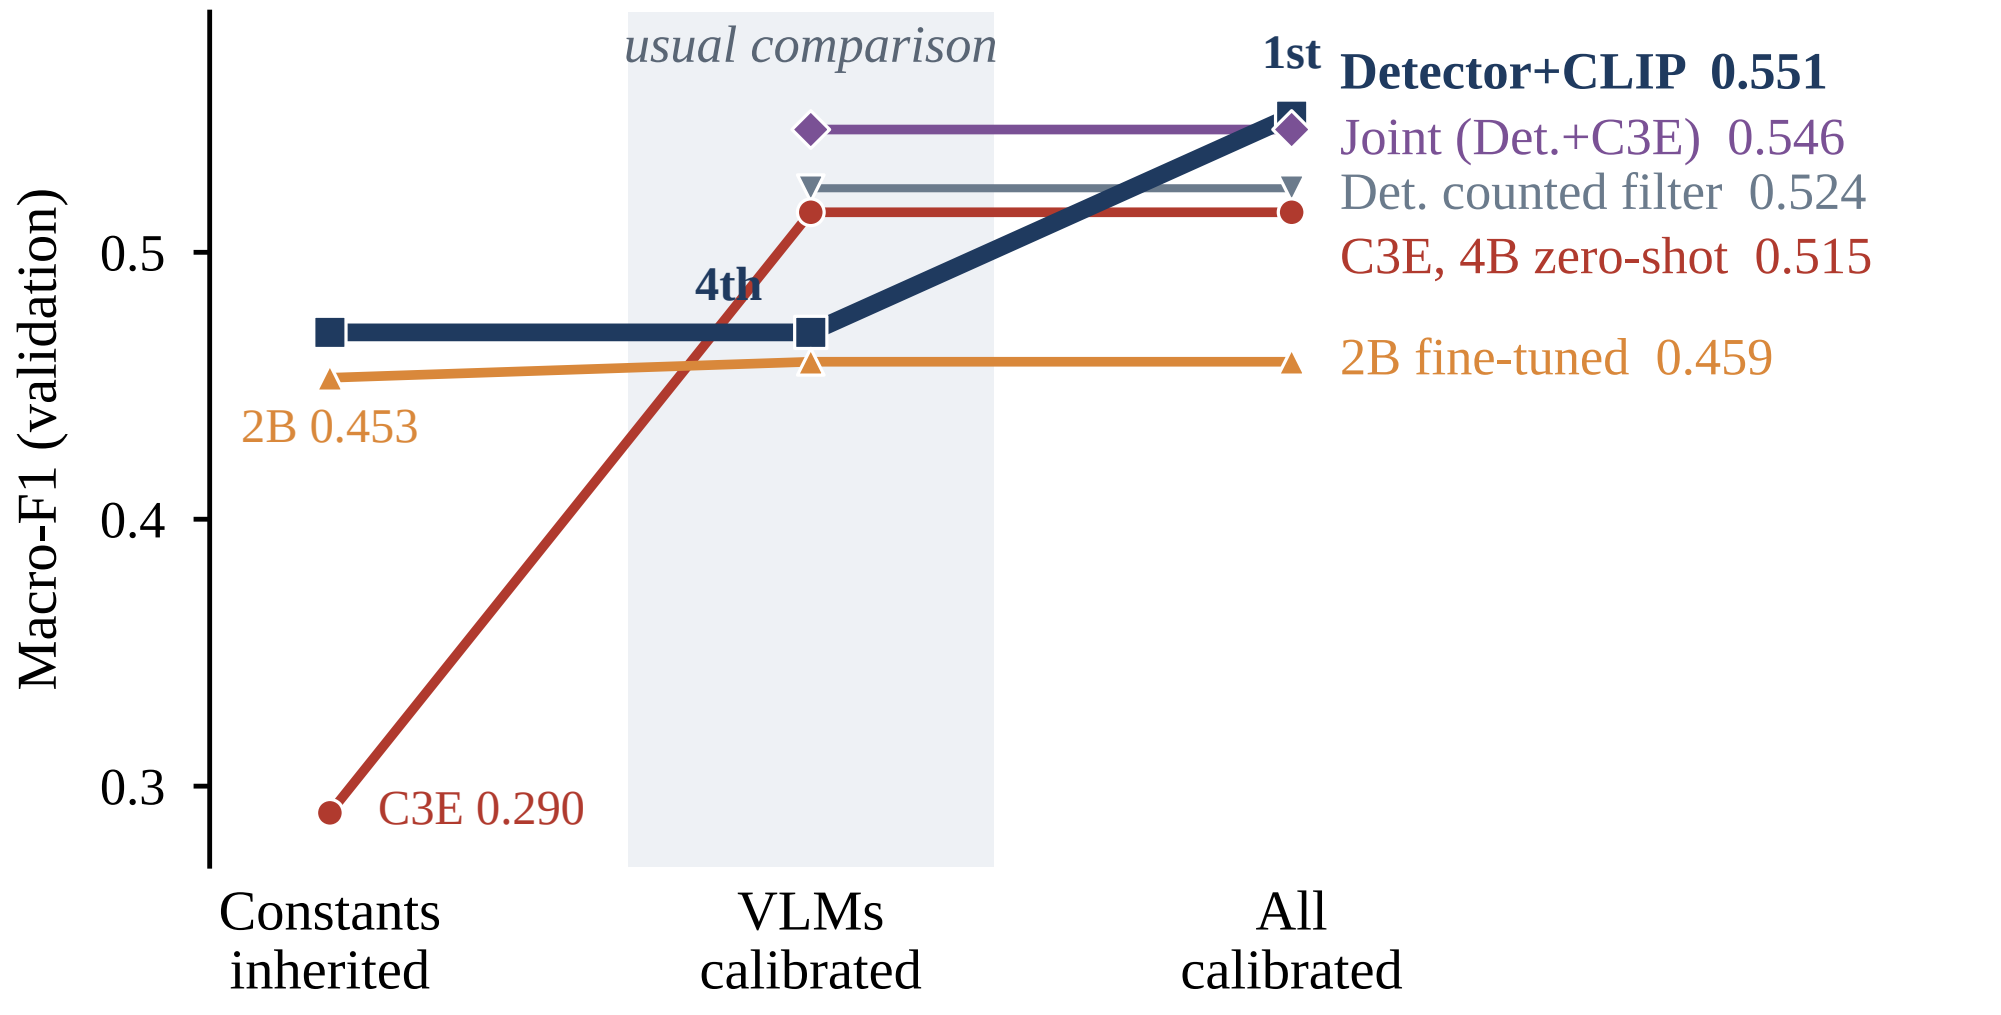
usual comparison
1st
Detector+CLIP 0.551
Joint (Det.+C3E) 0.546
Det. counted filter 0.524
C3E, 4B zero-shot 0.515
2B fine-tuned 0.459
4th
2B 0.453
C3E 0.290
Macro-F1 (validation)
0.5
0.4
0.3
Constants inherited
VLMs calibrated
All calibrated