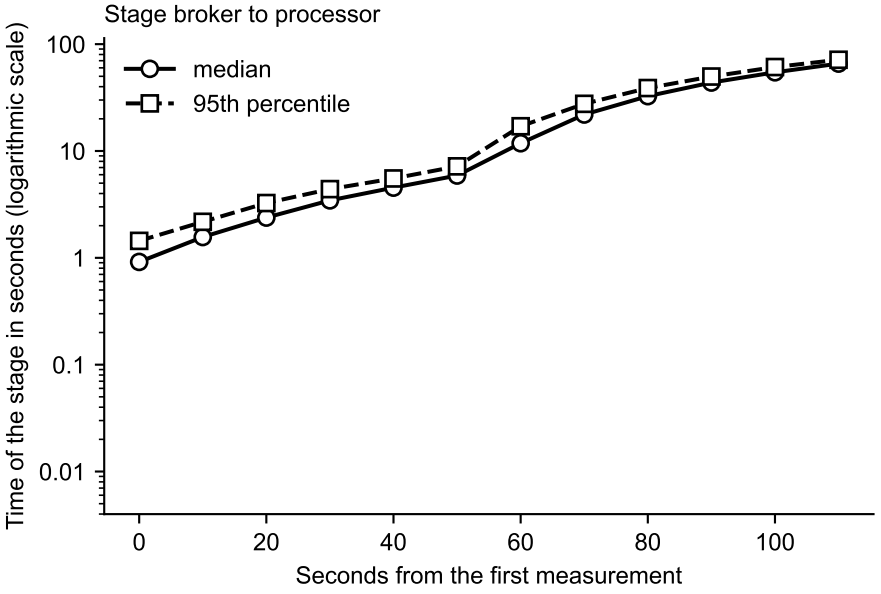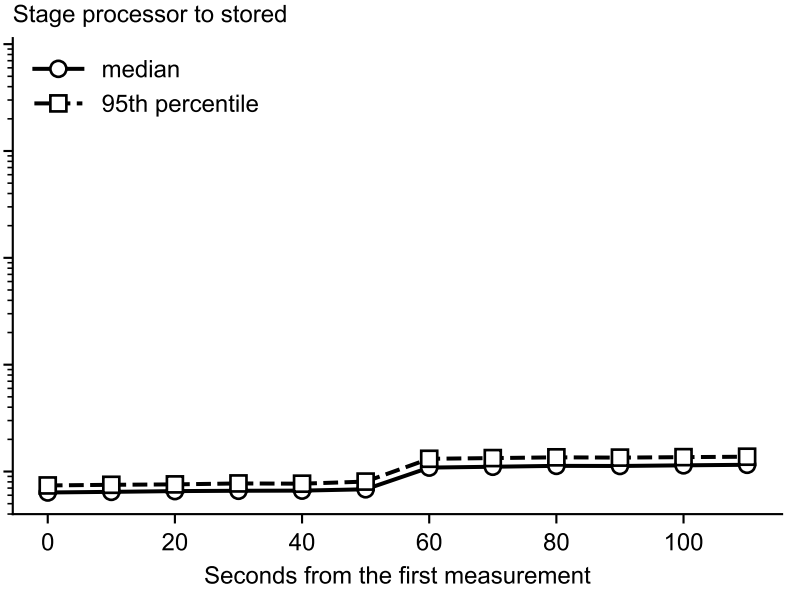Step of 50,000 readings per second, run 3, readings by the time of their measurement