

Name: NAME, FAKE NAME



ID:

Exam Date: 5/19/2022

CZMI

DOB: 5/19/1956

Exam Time: 8:12 AM

Gender: Female






Serial Number: 5000-4575

Technician: Operator, Cirrus


Signal Strength: 6/10

## Macula Thickness : Macular Cube 512x128




OD ● ○ OS

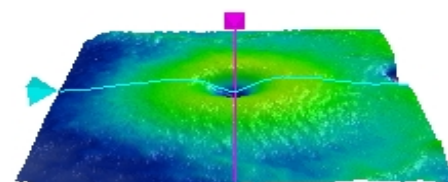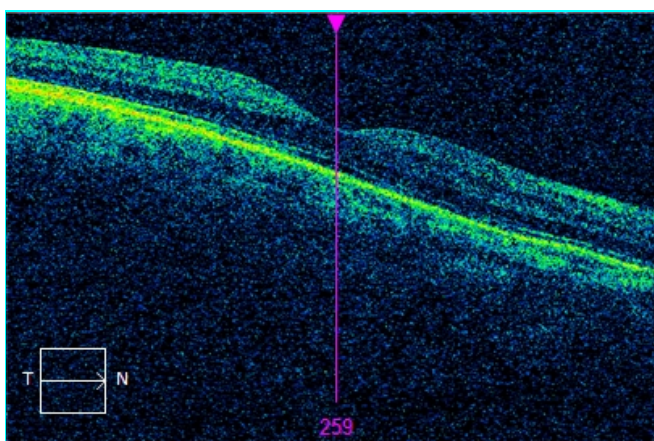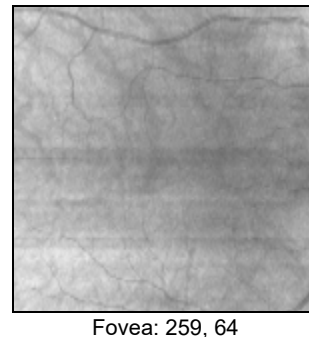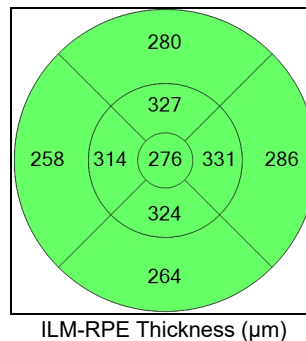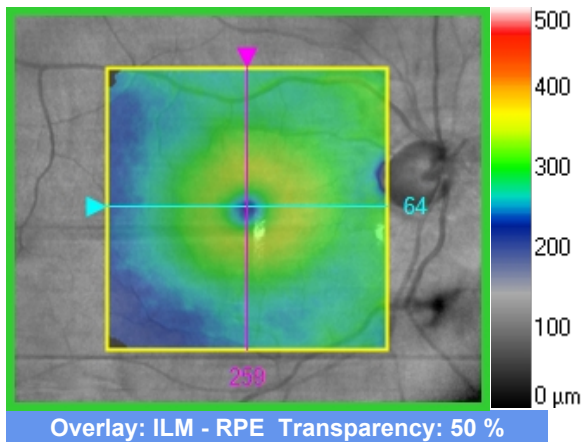

ILM - RPE

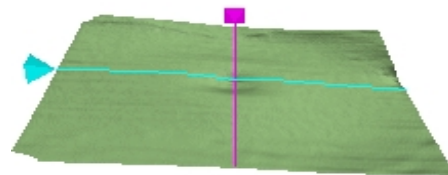

ILM

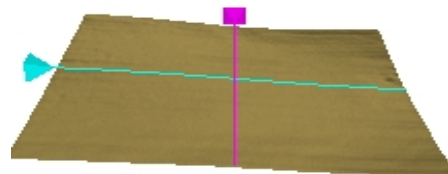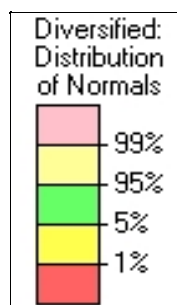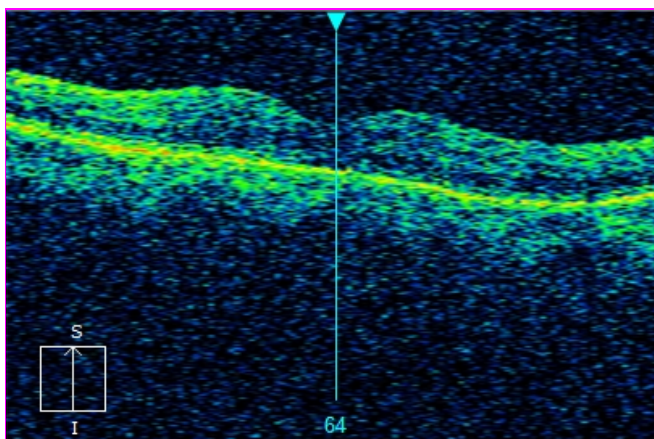

RPE

|           | Central Subfield Thickness (μm) | Cube Volume (mm <sup>3</sup> ) | Cube Average Thickness (μm) |
|-----------|---------------------------------|--------------------------------|-----------------------------|
| ILM - RPE | 276                             | 10.0                           | 277                         |

Comments

Doctor's Signature

SMHPC21418  
SW Ver: 11.5.1.47041  
Copyright 2019  
Carl Zeiss Meditec, Inc  
All Rights Reserved  
Page 1 of 1