




TTN H-NMR Validation Set - All 37 Functional Groups

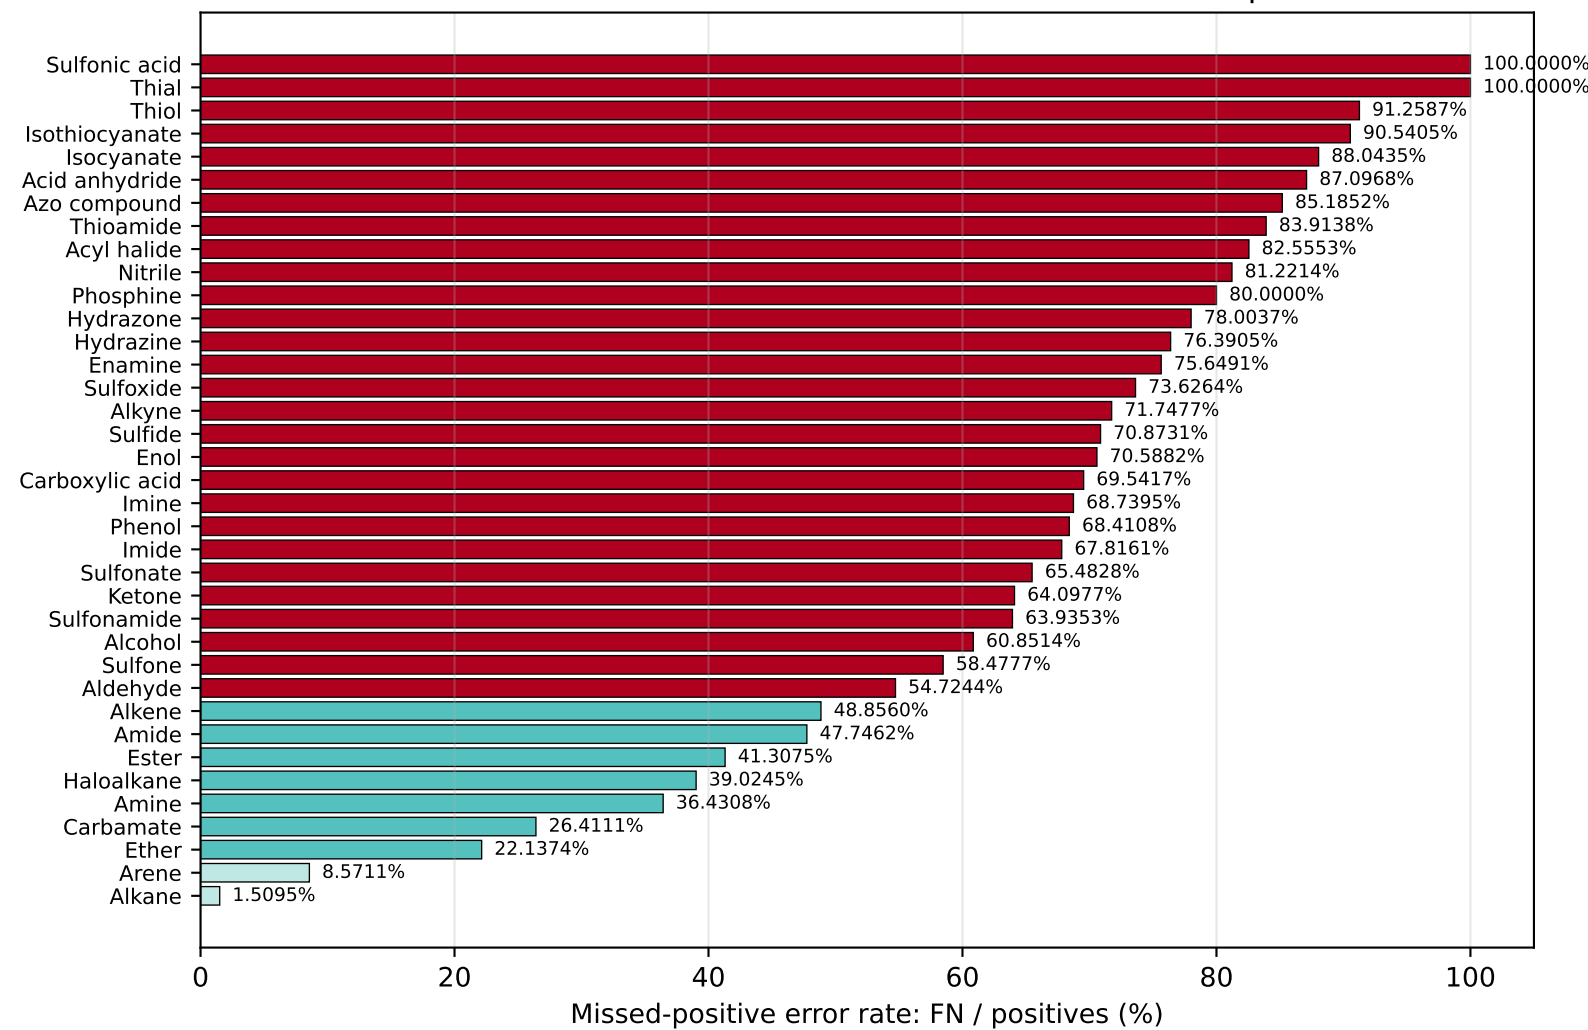

Error-Rate Distribution

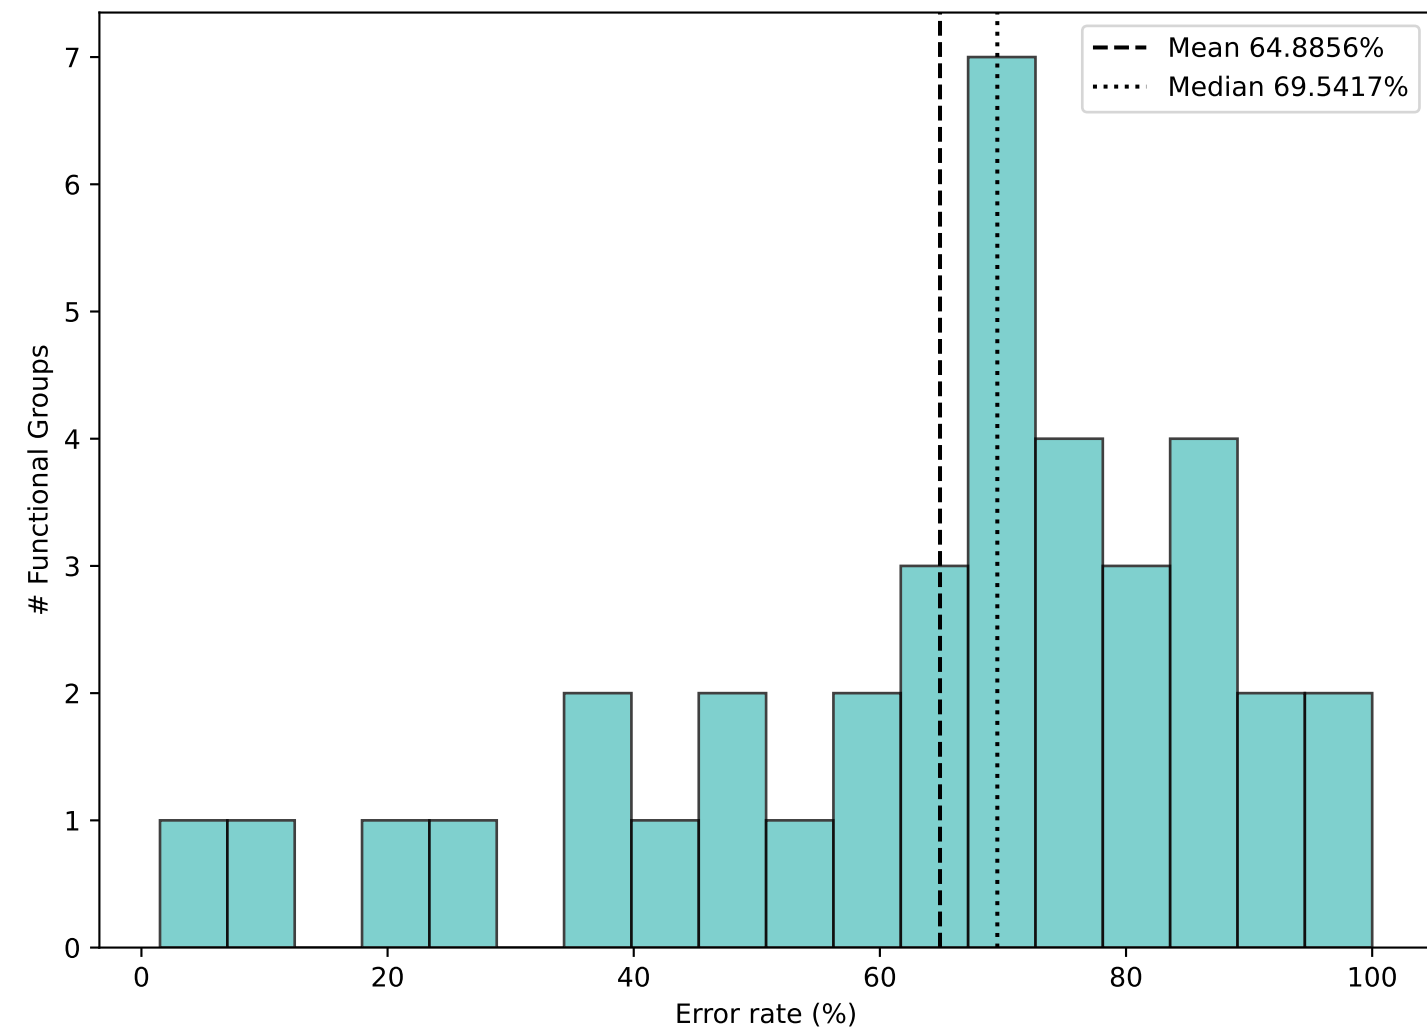

Top 10 Problem Groups

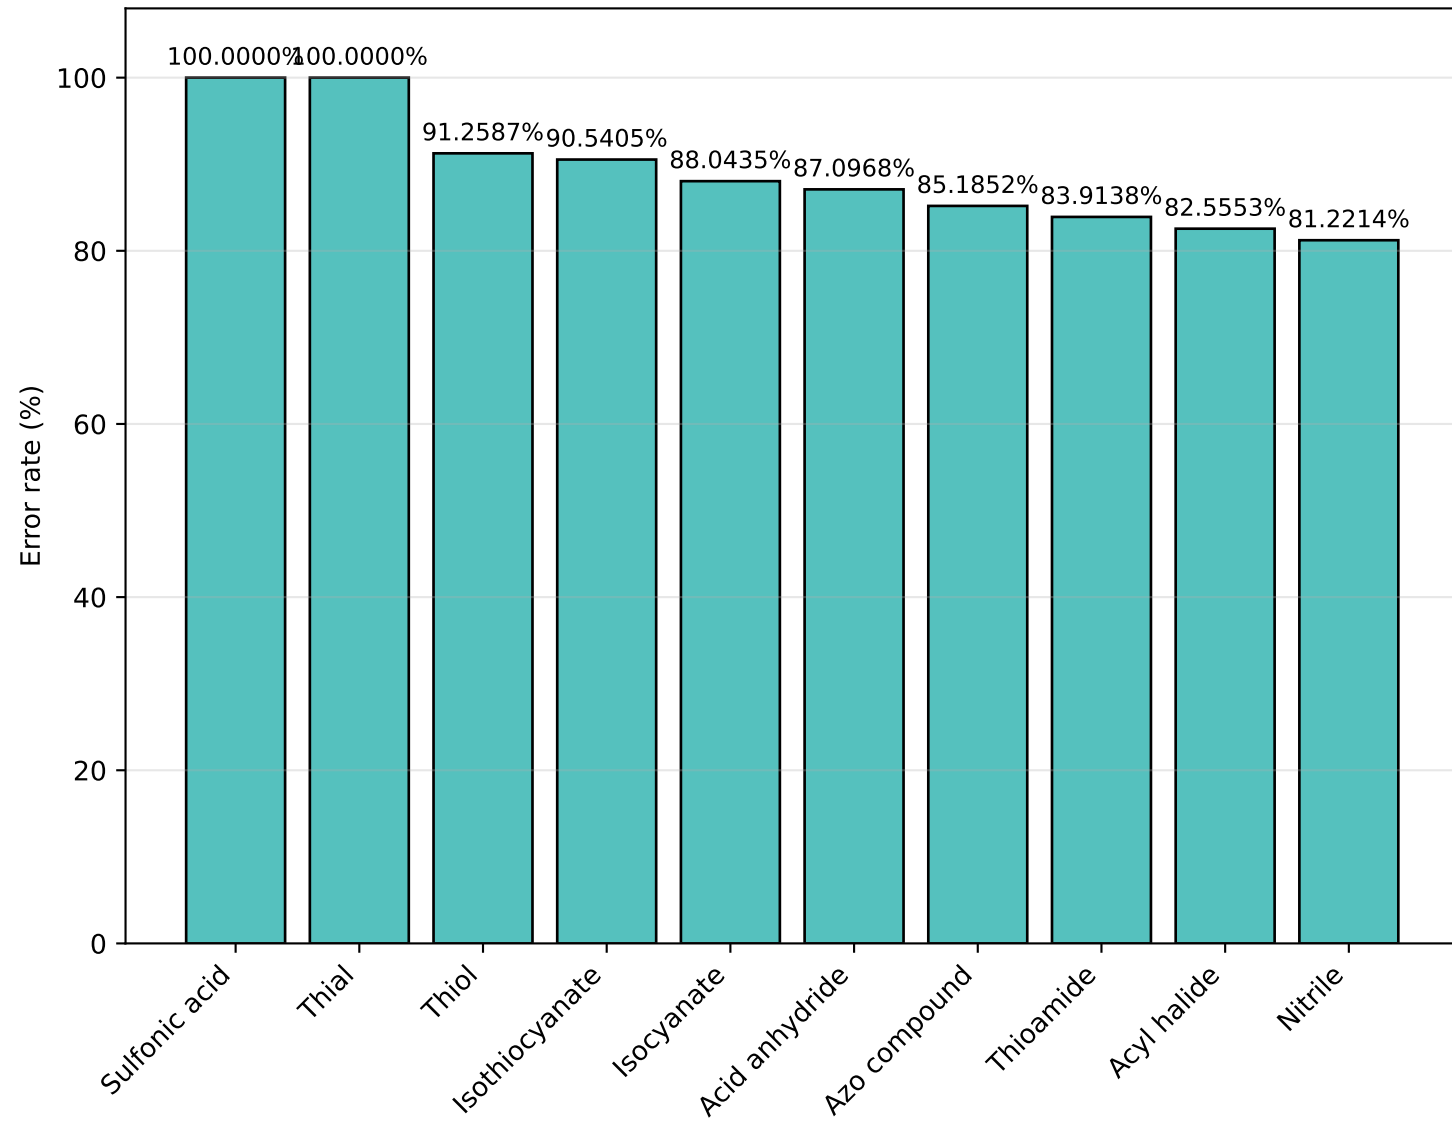

TTN H-NMR VALIDATION SET ERROR ANALYSIS

Global metrics:

F1 micro:	0.6850
F1 macro:	0.3172
Precision micro:	0.6734
Recall micro:	0.6969
Hamming accuracy:	0.9172

Error-rate statistics:

Mean:	64.8856%
Median:	69.5417%
Std:	23.7720%
Max:	100.0000% (Sulfonic acid)
Min:	1.5095% (Alkane)

Problem classes:

Severe (>50%):	28 groups
High (20-50%):	7 groups
Moderate (5-20%):	1 groups
Low (<=5%):	1 groups