




TTN IR Validation Set - All 37 Functional Groups

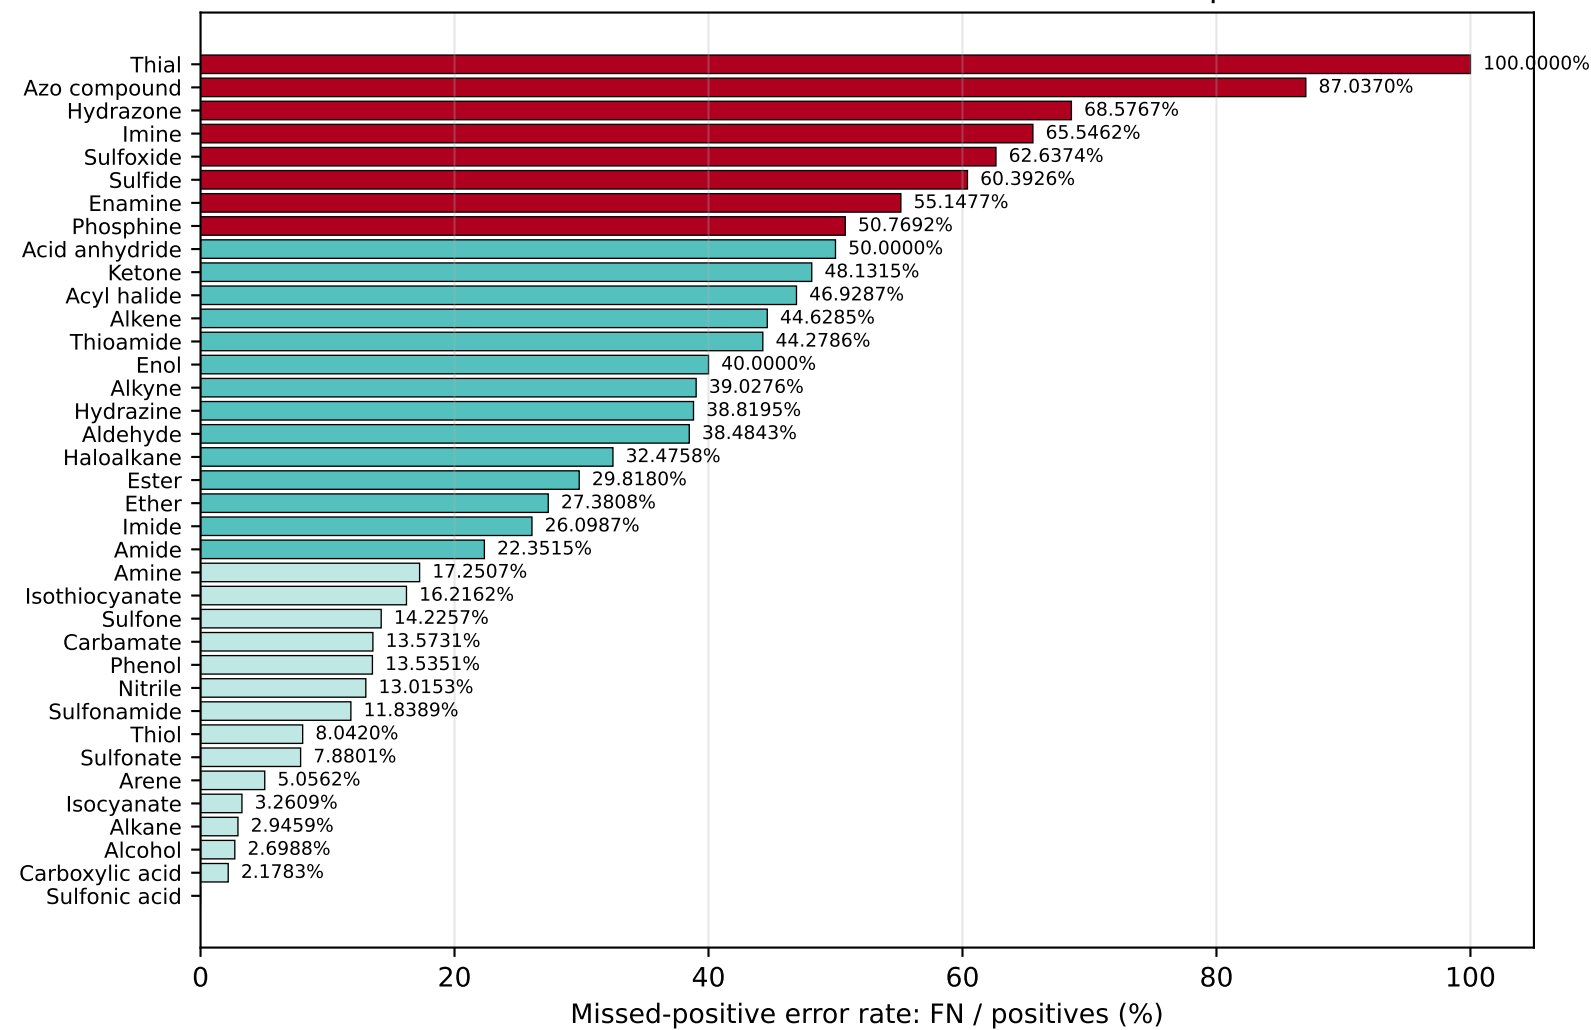

Error-Rate Distribution

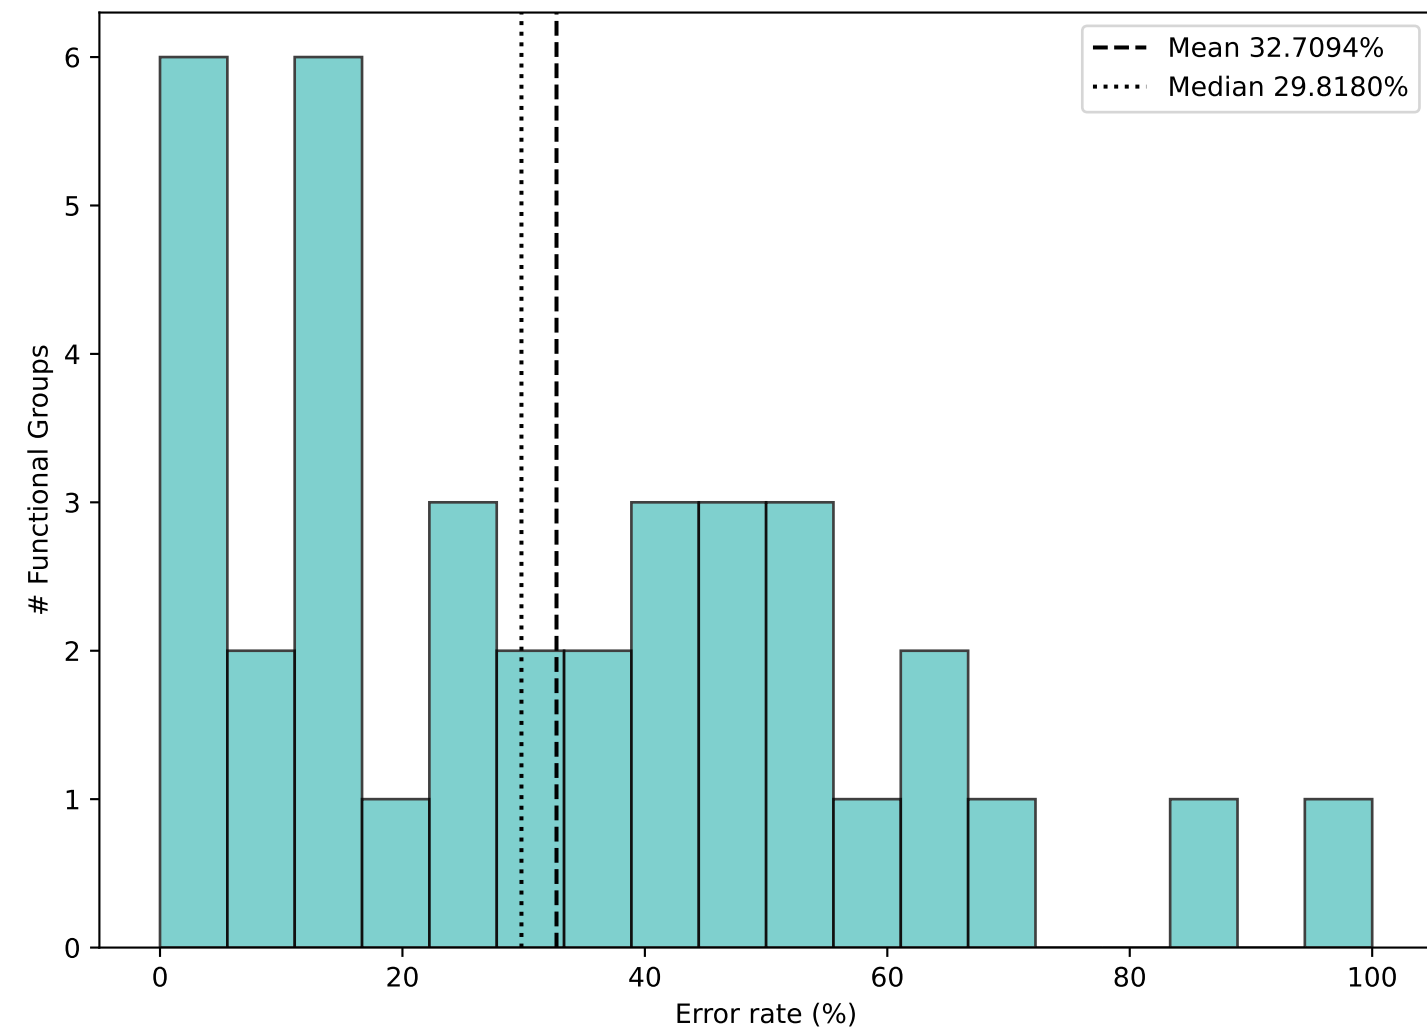

Top 10 Problem Groups

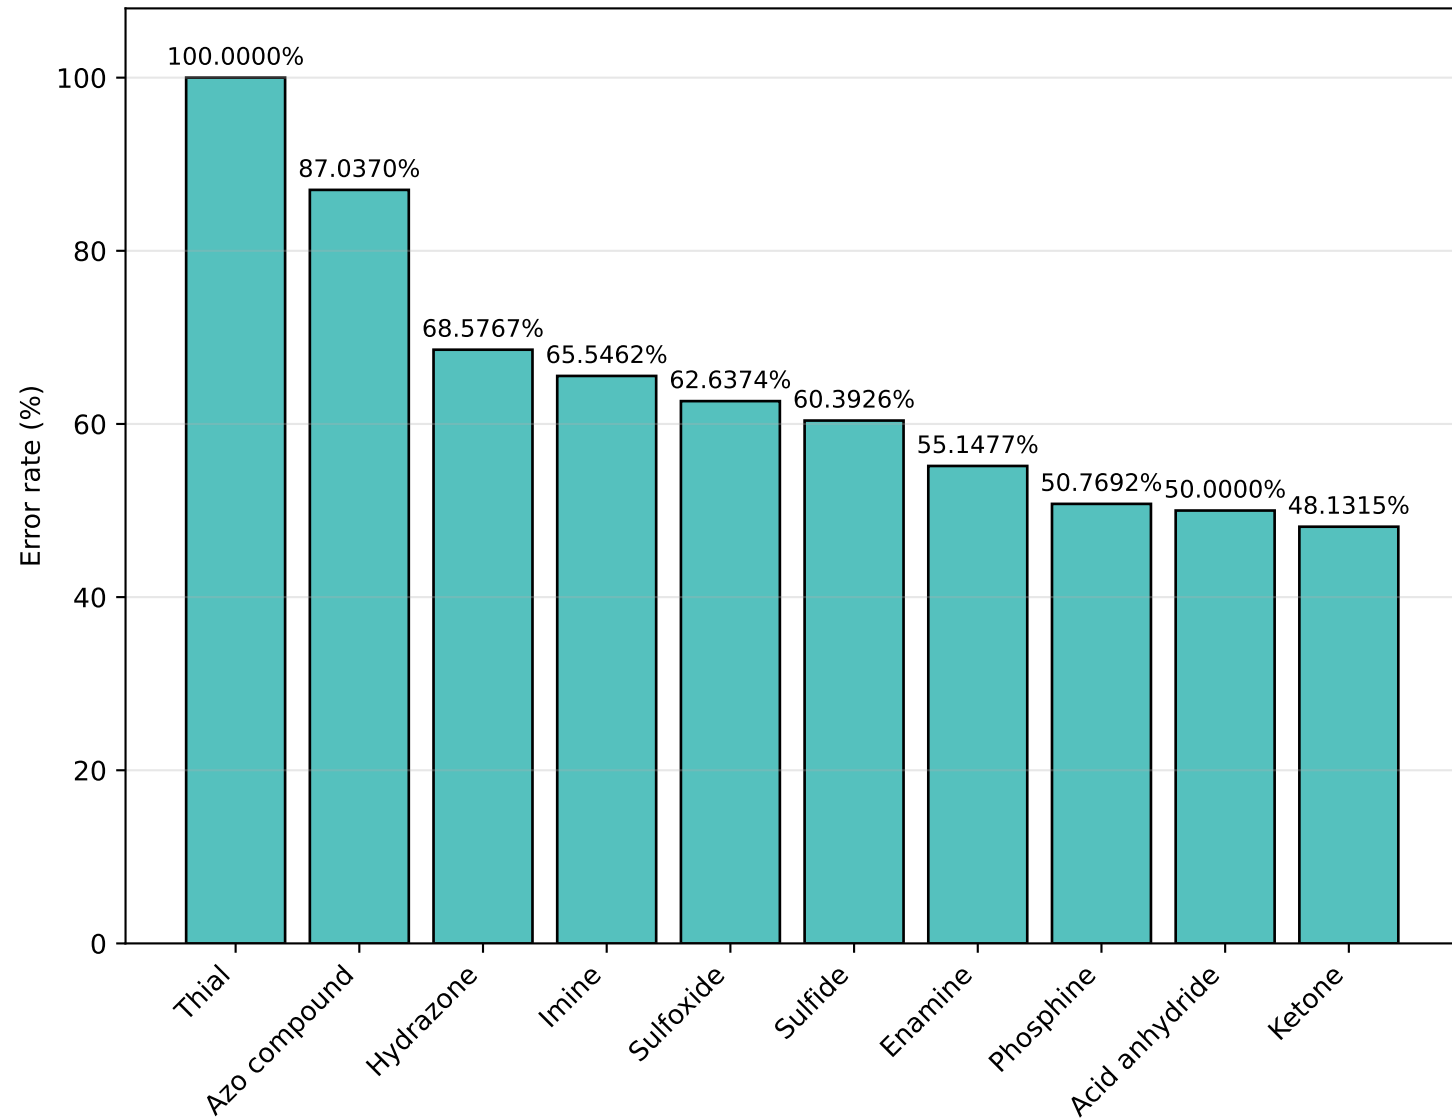

TTN IR VALIDATION SET ERROR ANALYSIS

Global metrics:

F1 micro:	0.8214
F1 macro:	0.5874
Precision micro:	0.8187
Recall micro:	0.8241
Hamming accuracy:	0.9537

Error-rate statistics:

Mean:	32.7094%
Median:	29.8180%
Std:	25.1428%
Max:	100.0000% (Thial)
Min:	0.0000% (Sulfonic acid)

Problem classes:

Severe (>50%):	8 groups
High (20-50%):	14 groups
Moderate (5-20%):	10 groups
Low (<=5%):	5 groups