




XGBoost IR Test Set - All 37 Functional Groups

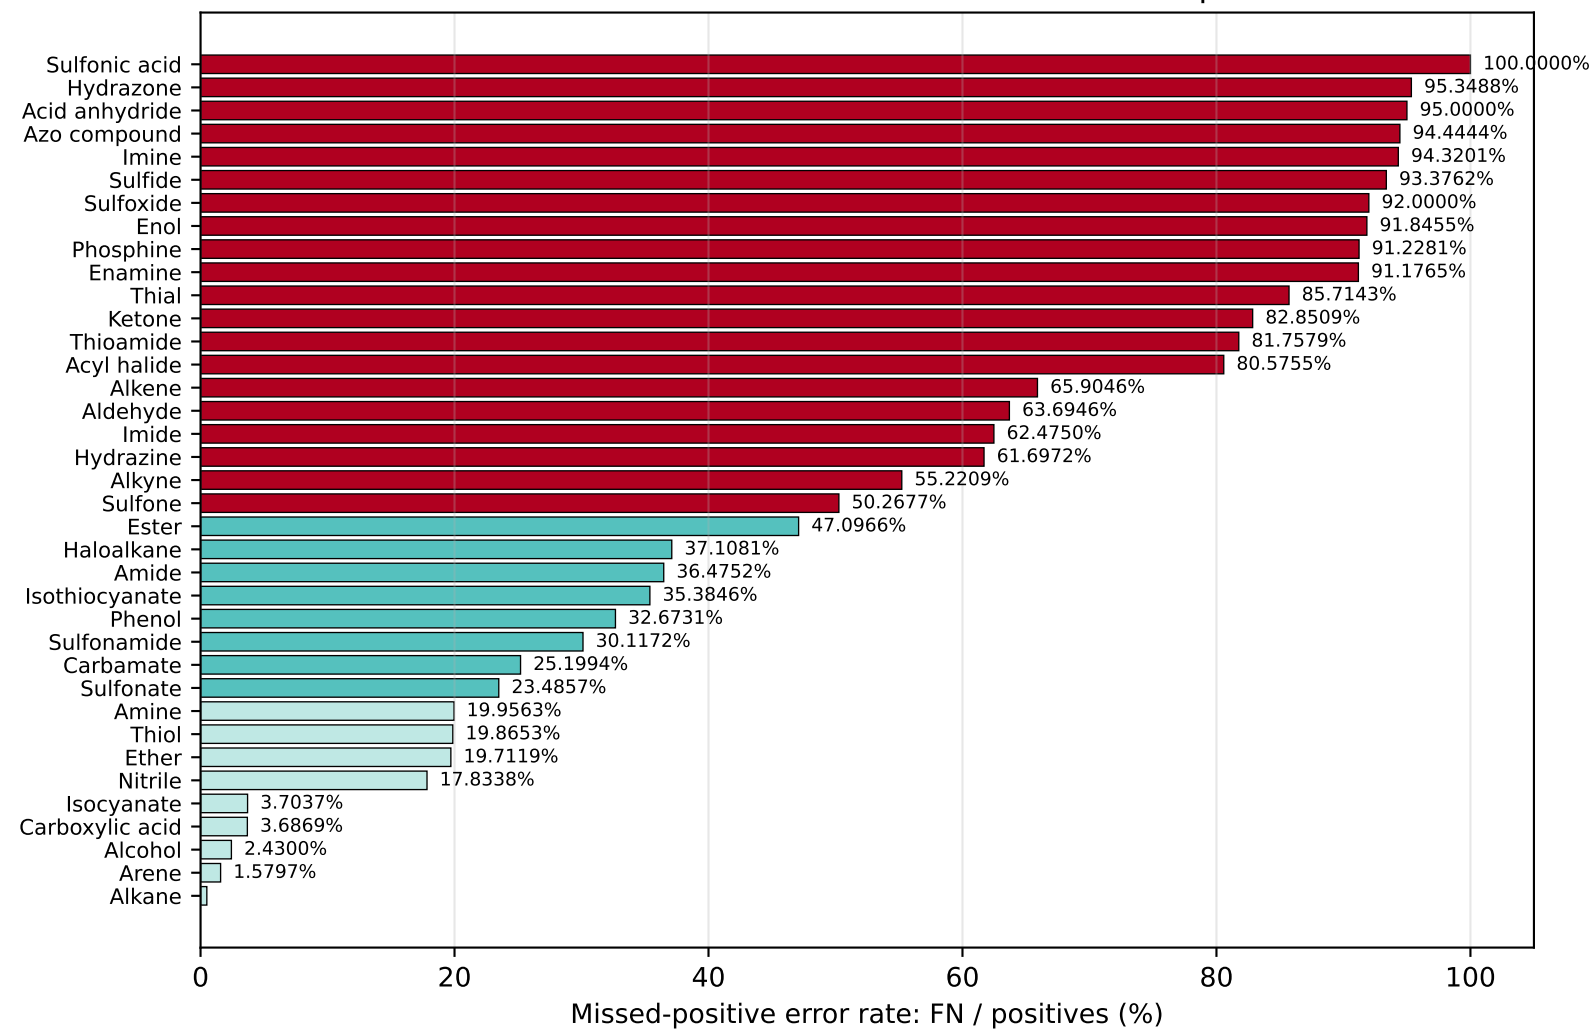

Error-Rate Distribution

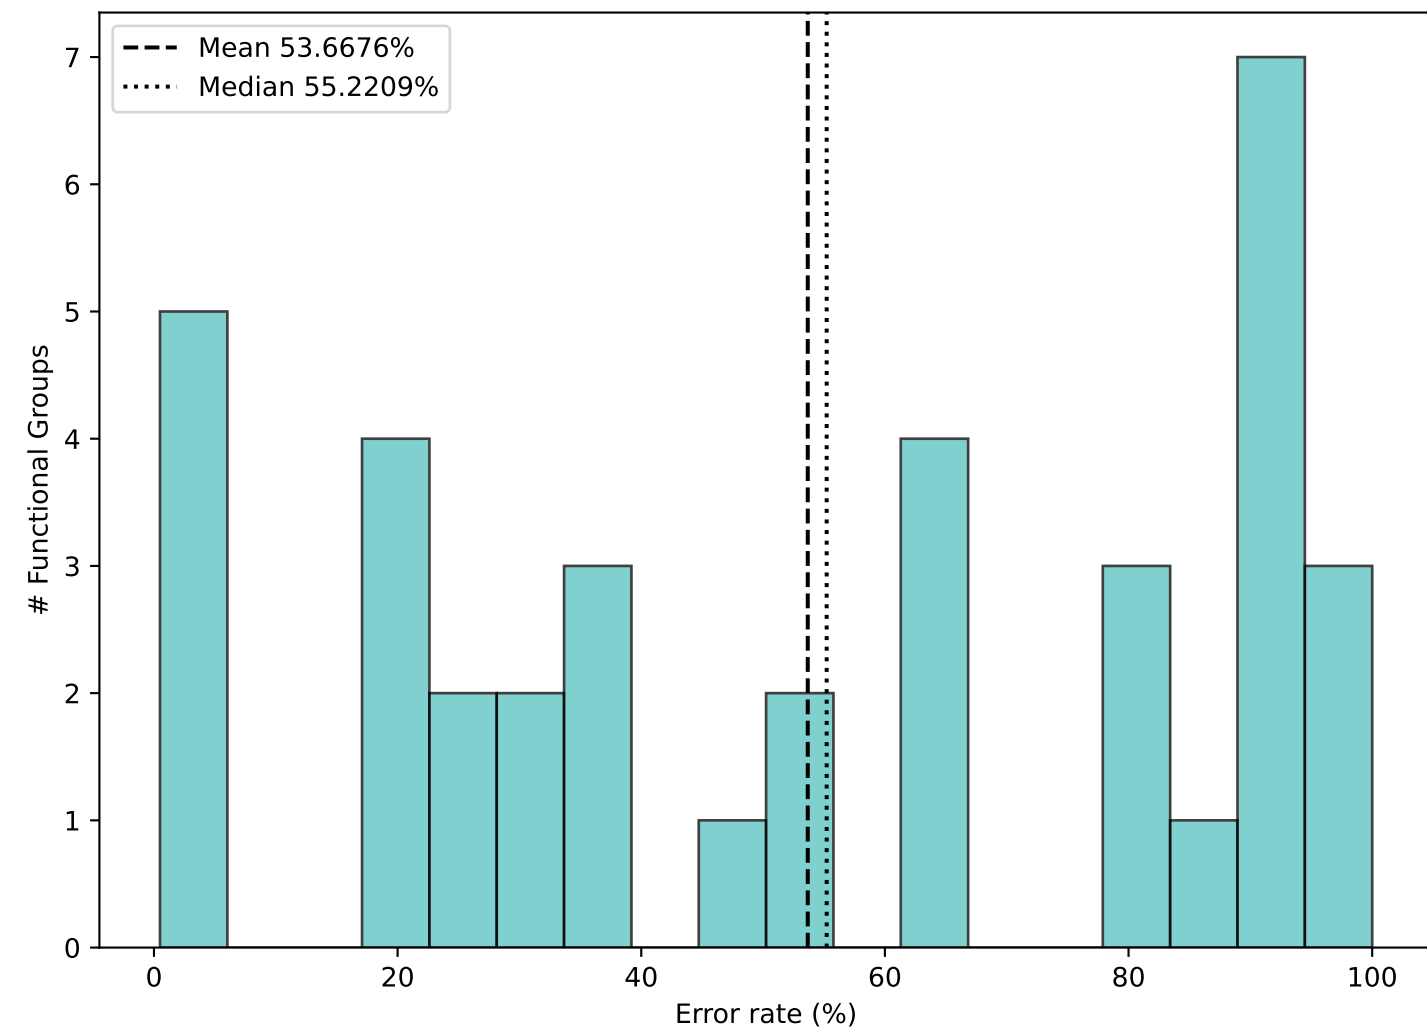

Top 10 Problem Groups

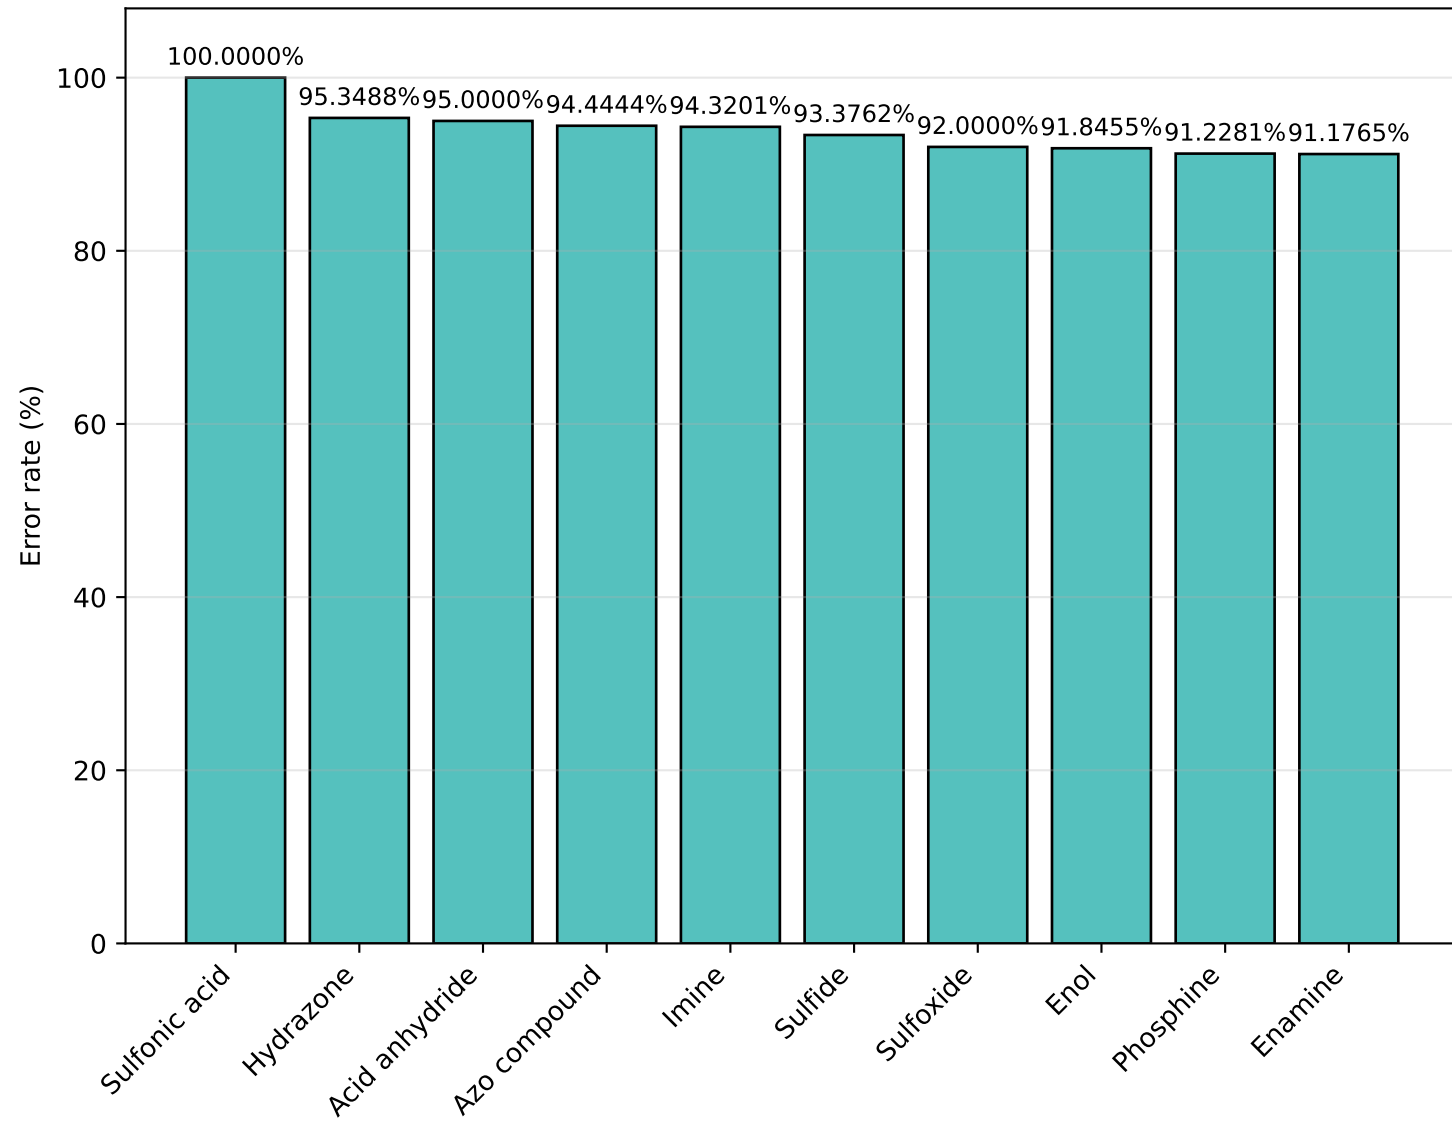

XGB00ST IR TEST SET ERROR ANALYSIS

Global metrics:

F1 micro:	0.8380
F1 macro:	0.5460
Precision micro:	0.8855
Recall micro:	0.7954
Hamming accuracy:	0.9603

Error-rate statistics:

Mean:	53.6676%
Median:	55.2209%
Std:	33.9802%
Max:	100.0000% (Sulfonic acid)
Min:	0.4959% (Alkane)

Problem classes:

Severe (>50%):	20 groups
High (20-50%):	8 groups
Moderate (5-20%):	4 groups
Low (<=5%):	5 groups