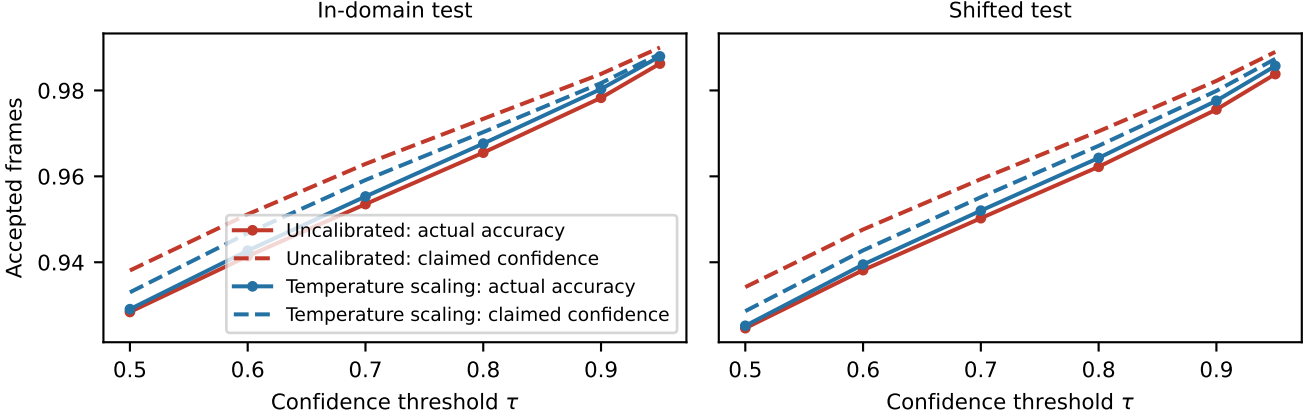
In-domain test
Shifted test
Accepted frames
0.98
0.96
0.94
0.5
0.6
0.7
0.8
0.9
Confidence threshold τ
Uncalibrated: actual accuracy
Uncalibrated: claimed confidence
Temperature scaling: actual accuracy
Temperature scaling: claimed confidence