




Phantom QA results for / fbirn_out/ses-64ch_func-bold_acq-cmrrme_task-tsnrxacpc.xml, slice 35

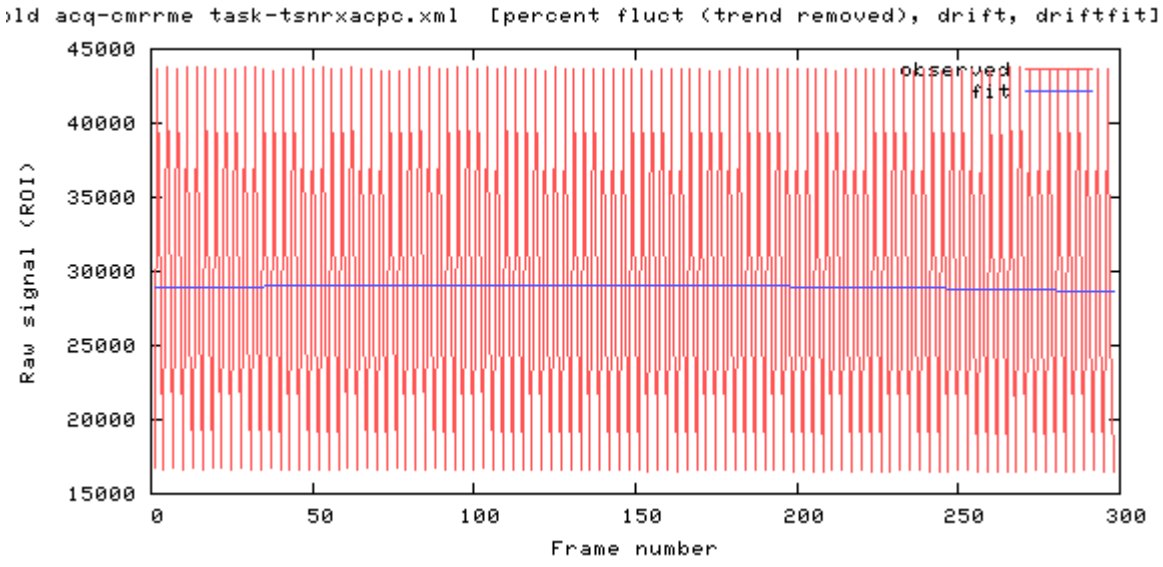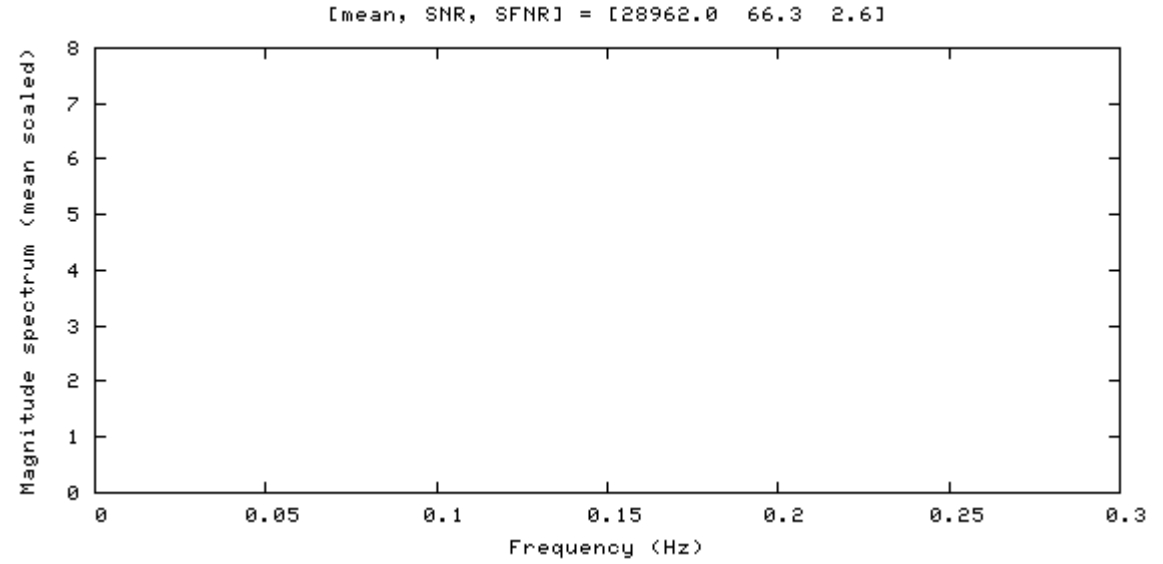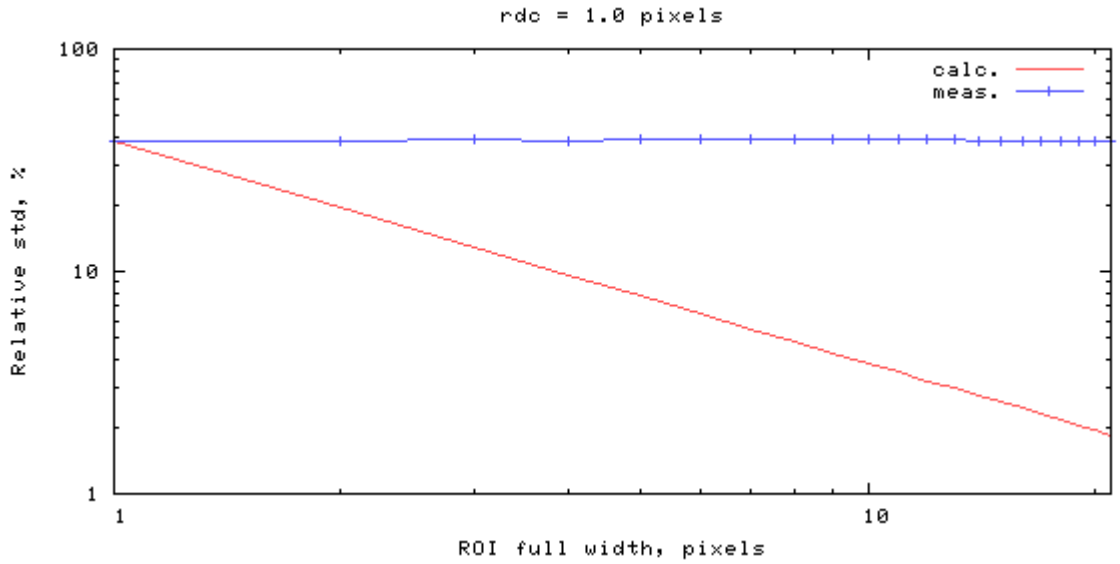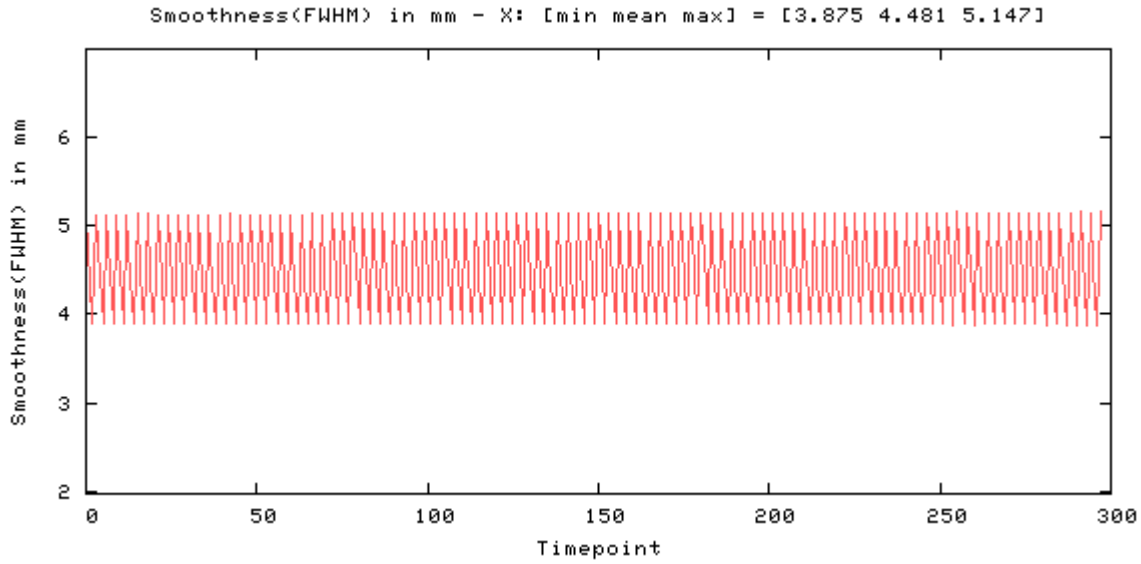


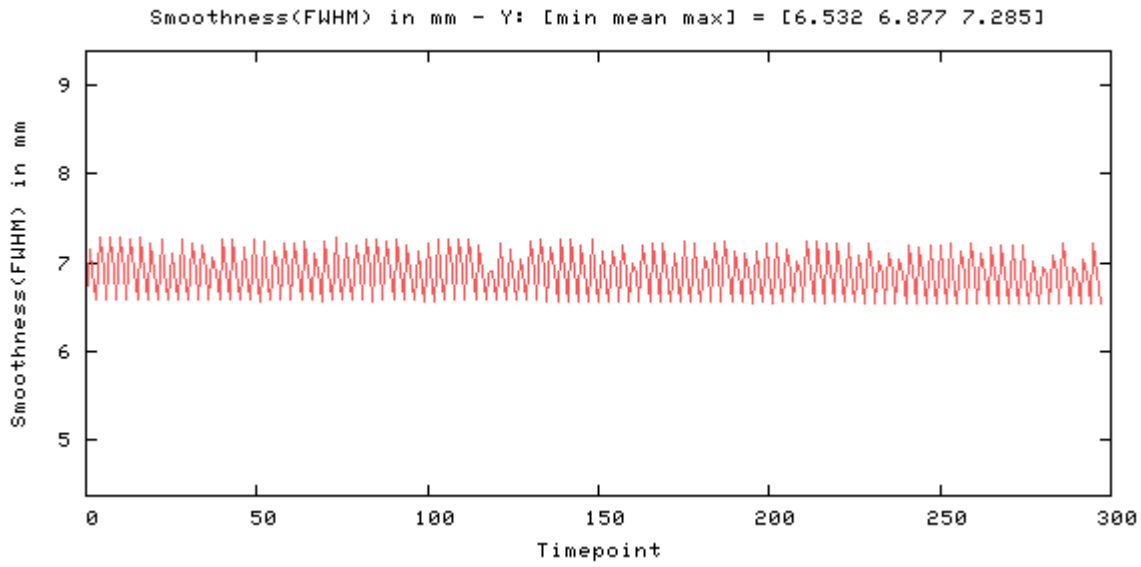




rdc = 1.0 pixels
calc.
meas.
Relative std, %
100
10
1
1
10
ROI full width, pixels



Smoothness(FWHM) in mm - X: [min mean max] = [3.875 4.481 5.147]
Smoothness(FWHM) in mm
6
5
4
3
2
0
50
100
150
200
250
300
Timepoint



Smoothness(FWHM) in mm - Y: [min mean max] = [6.532 6.877 7.285]
Smoothness(FWHM) in mm
9
8
7
6
5
0
50
100
150
200
250
300
Timepoint

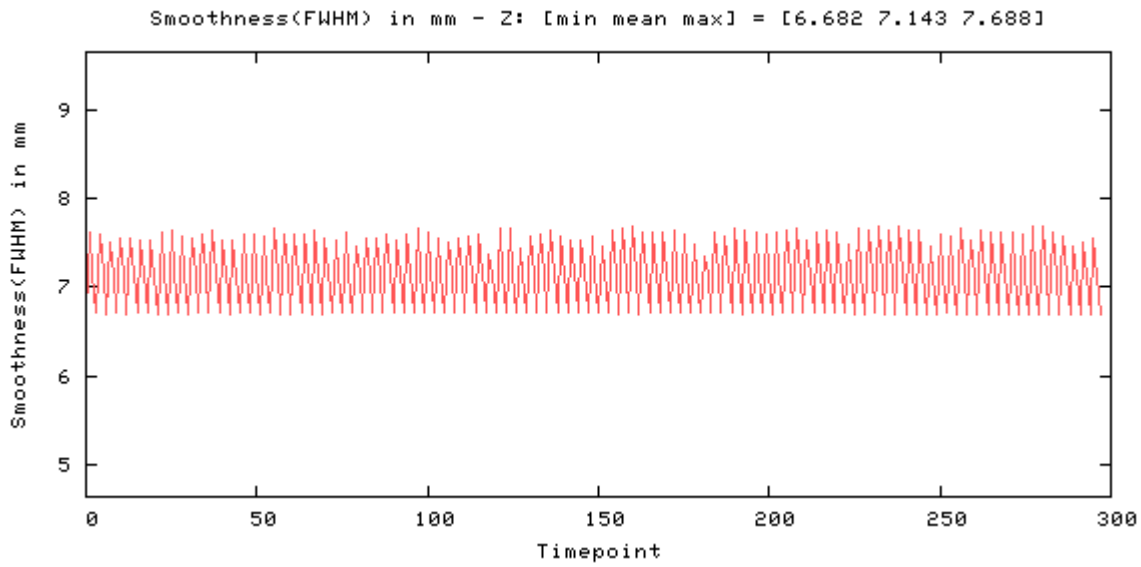
Smoothness(FWHM) in mm - Z: [min mean max] = [6.682 7.143 7.688]
Smoothness(FWHM) in mm
9
8
7
6
5
0
50
100
150
200
250
300
Timepoint

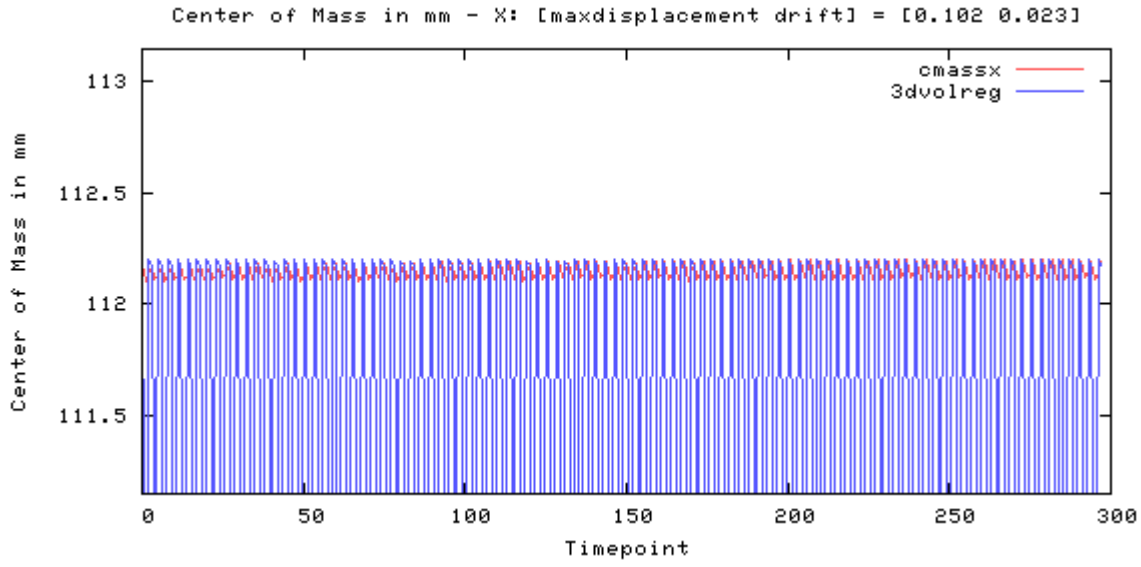
Center of Mass in mm - X: [maxdisplacement drift] = [0.102 0.023]
Center of Mass in mm
cmassx
3dvolreg
113
112.5
112
111.5
0
50
100
150
200
250
300
Timepoint

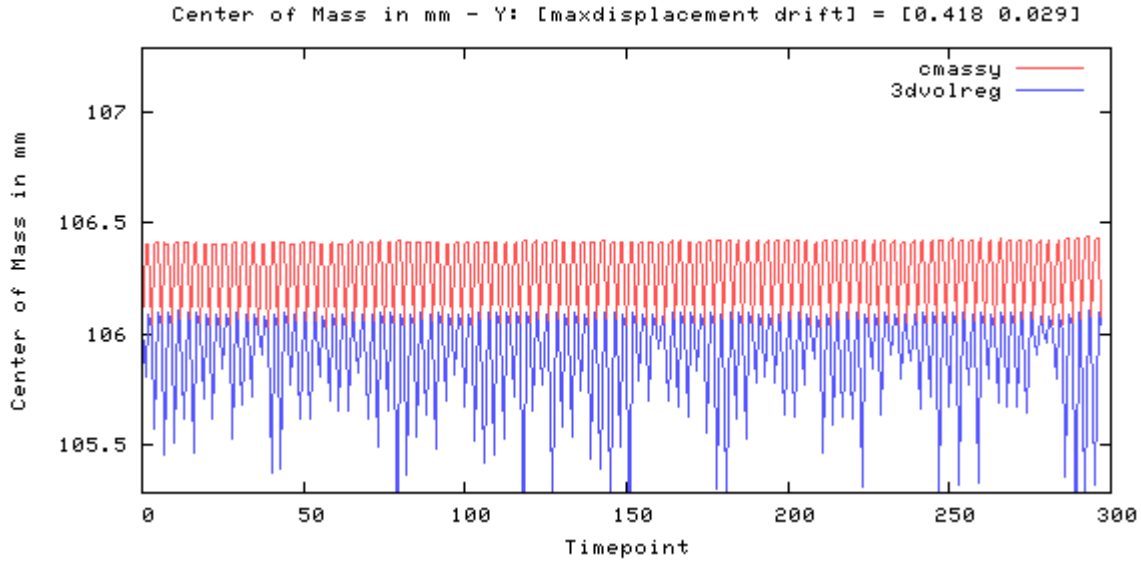
Center of Mass in mm - Y: [maxdisplacement drift] = [0.418 0.029]
Center of Mass in mm
cmassy
3dvolreg
107
106.5
106
105.5
0
50
100
150
200
250
300
Timepoint

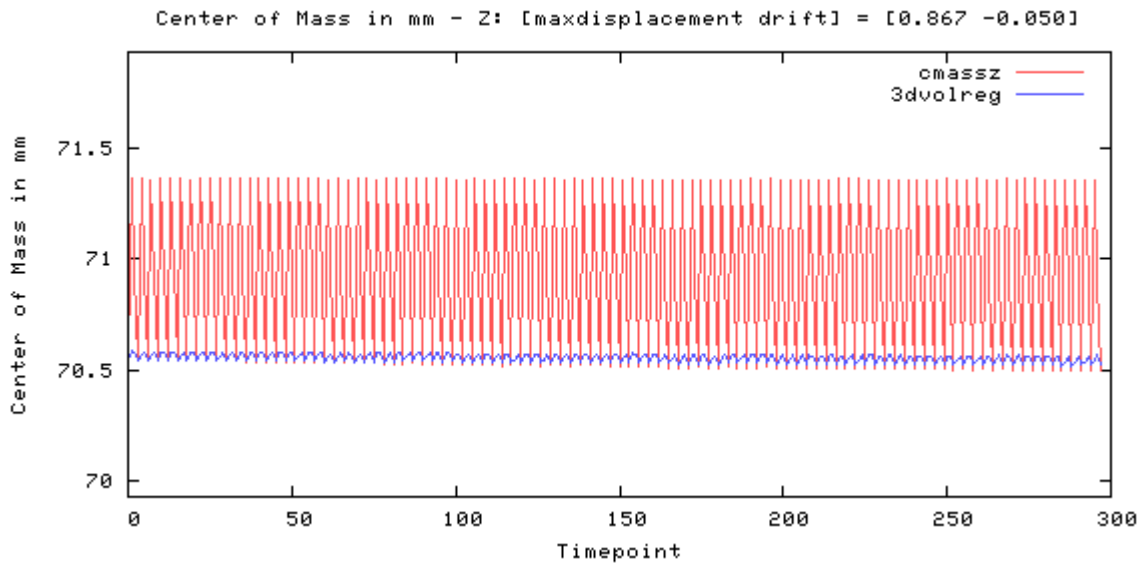

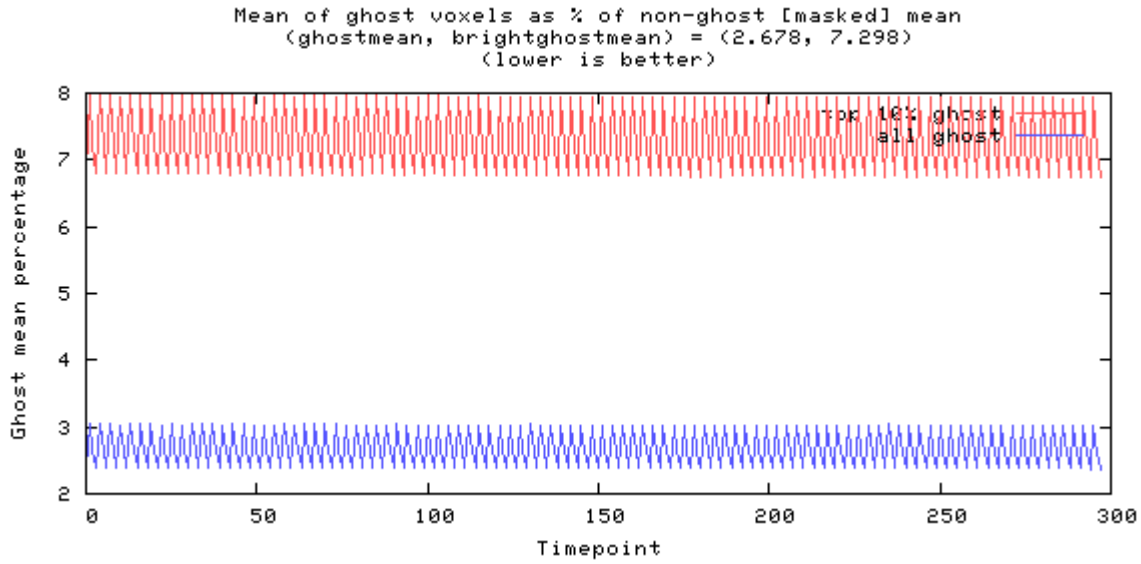


Odd-even difference image

-43420	6396




image min: -43420, image max: 6396

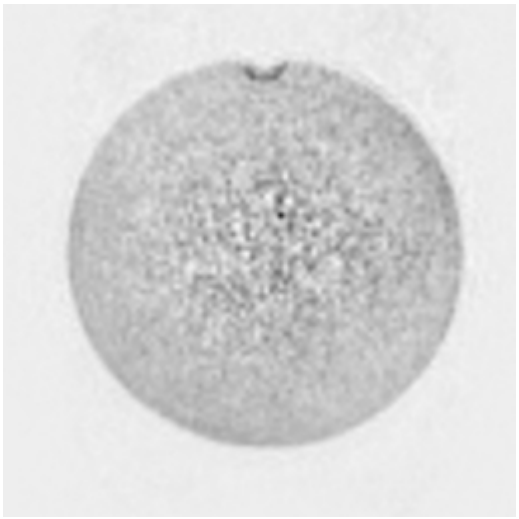

Mean image

0 39064.6


image min: 0, image max: 39383.2

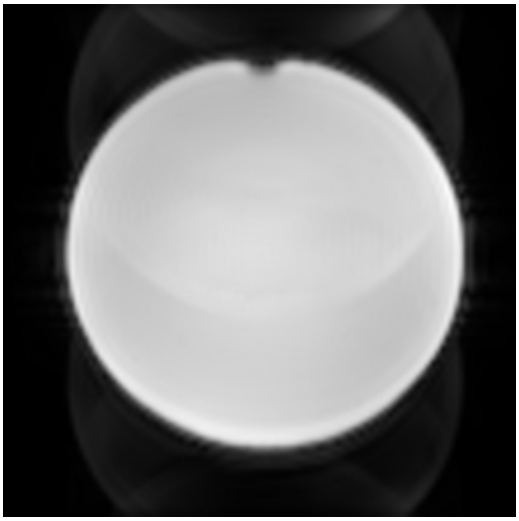

Standard Deviation image

0 17617.7


image min: 0, image max: 17617.7

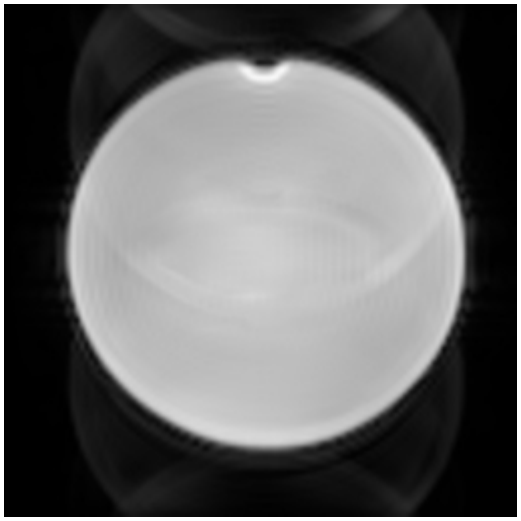

SFNR image



image min: 0, image max: 9.2934

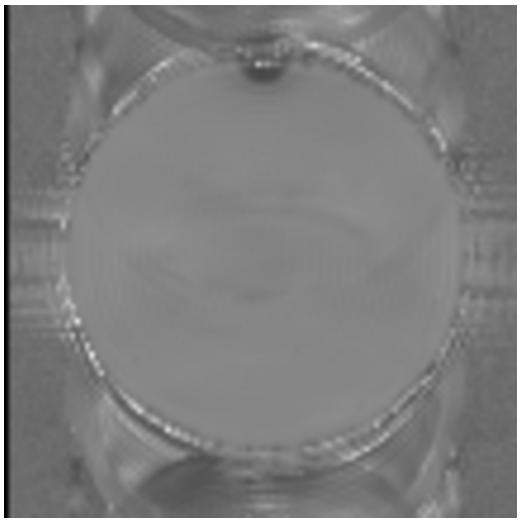

Acquisition parameters

dimensions	108x108x72x300
spacing	2.03704mmx2.03704mmx2mmx0ms
gap	0mmx0mmx0mmx0ms
scanner	AWP213018
psdname	
examnumber	d10c7553-a968-4e
studyid	Stability_20261012
seriesnumber	13
runnumber	1
magneticfield	3

description	ses-64ch_func-bold_acq-cmrrme_task-tsnrxacpc
scandate	2026-10-12
scantime	11:31:43
tr	1720
te	13.4 37.84 62.28 13.4 37.84 62.28 13.4 37.84 62.28

operator	
flipangle	70
prescribedslicespacing	2
frequencydirection	1
receivecoilname	HeadNeck_64_CS
transmitcoilname	Body
institution	THE UNIVERSITY OF PENNSYLVANIA
examdescription	ACTIVE KIRWAN
scanner	AWP213018
scannermanufacturer	Siemens Healthineers
scannermodelname	MAGNETOM Cima.X
protocolname	ses-64ch_func-bold_acq-cmrrme_task-tsnrxacpc
institutionaddress	Grays Ferry Ave. BLDG 250 STE 140 3401,Philadelphia,69 - KEYSTONE,US,19146
institutionaldepartmentname	MindCORE Neuroimaging Suite 140
acquisitiondatetime	20261012113126.585000
frametype	ORIGINAL
pixelpresentation	MONOCHROME
volumetricproperties	DISTORTED
volumebasedcalculationtechnique	NONE
complexiimagecomponent	MAGNITUDE
acquisitioncontrast	UNKNOWN
mracquisitiontype	2D
numaverages	1
spacingbetweenslices	2
echotrainlength	40
percentsampling	100
percentphasefieldofview	100
scannerserialnumber	213018
softwareversions	syngo MR XA61
inplanephaseencodingdirection	COLUMN
variableflipangleflag	N
contentqualification	RESEARCH
acquisitionduration	204.60500000000002
resonantnucleus	1H
applicablesafetystandardagency	IEC
acquisitionnumber	1
instancenumber	1
numtemporalpositions	100
imagecomments	

	Not for diagnostic use, Unaliased MB4/ PE4/LB SENSE1
samplesperpixel	1
photometricinterpretation	MONOCHROME2
numberofframes	72
rows	108
columns	108
bitsallocated	16
bitsstored	16
highbit	15
lossyimagecompression	00