




Phantom QA results for / fbirn_out/ses-64ch_func-bold_acq-siemensstd_task-tsnr.xml, slice 17

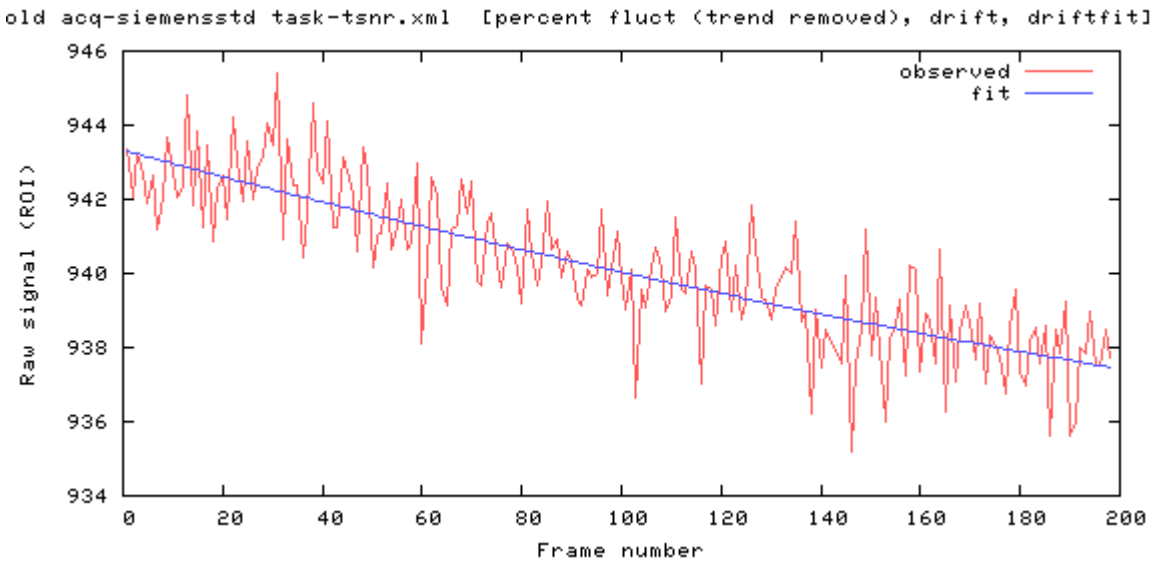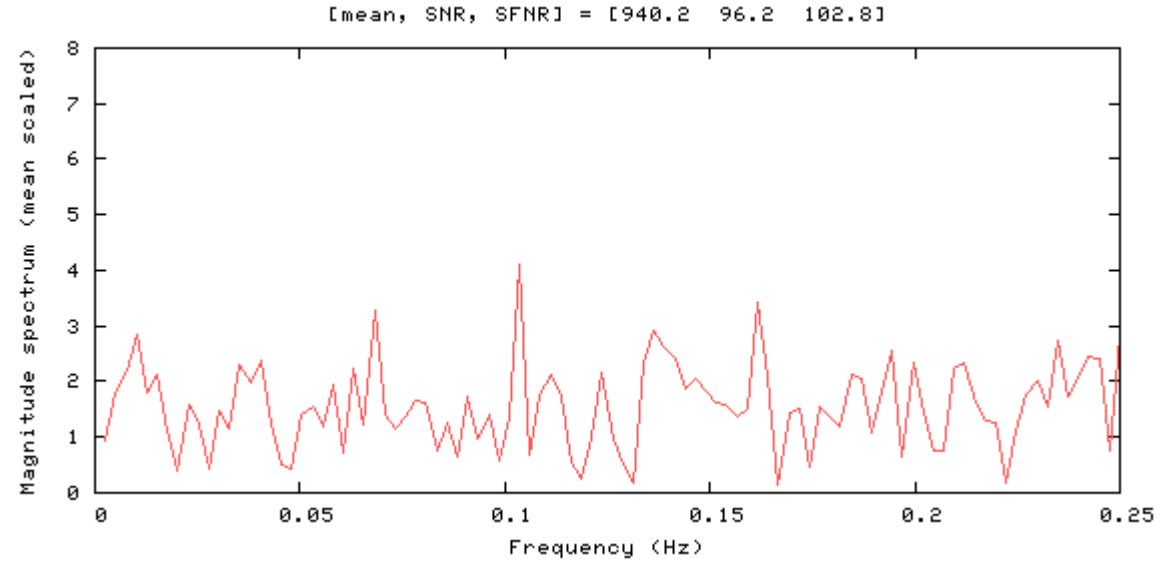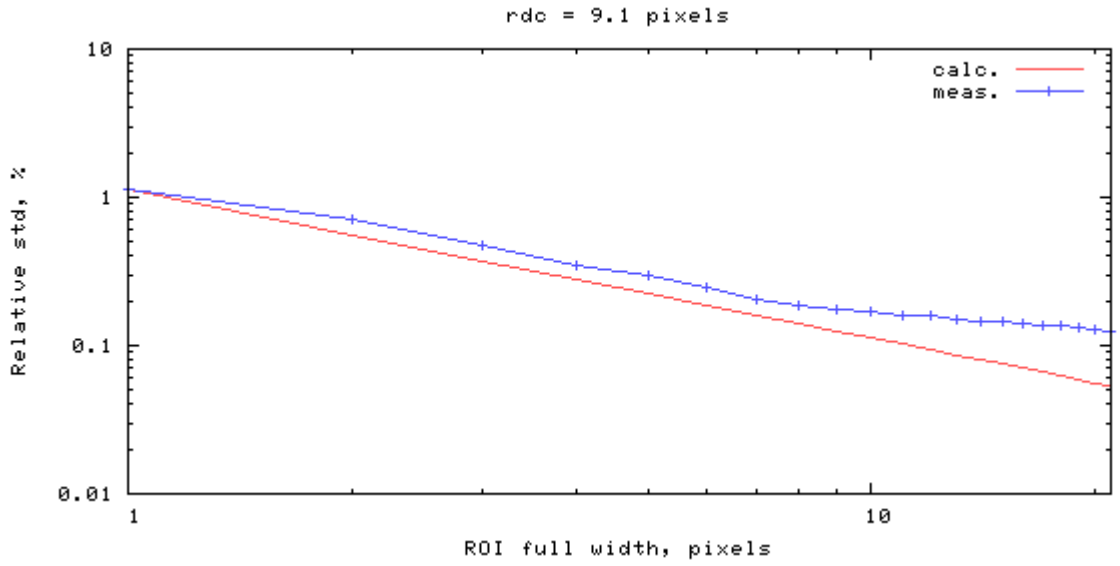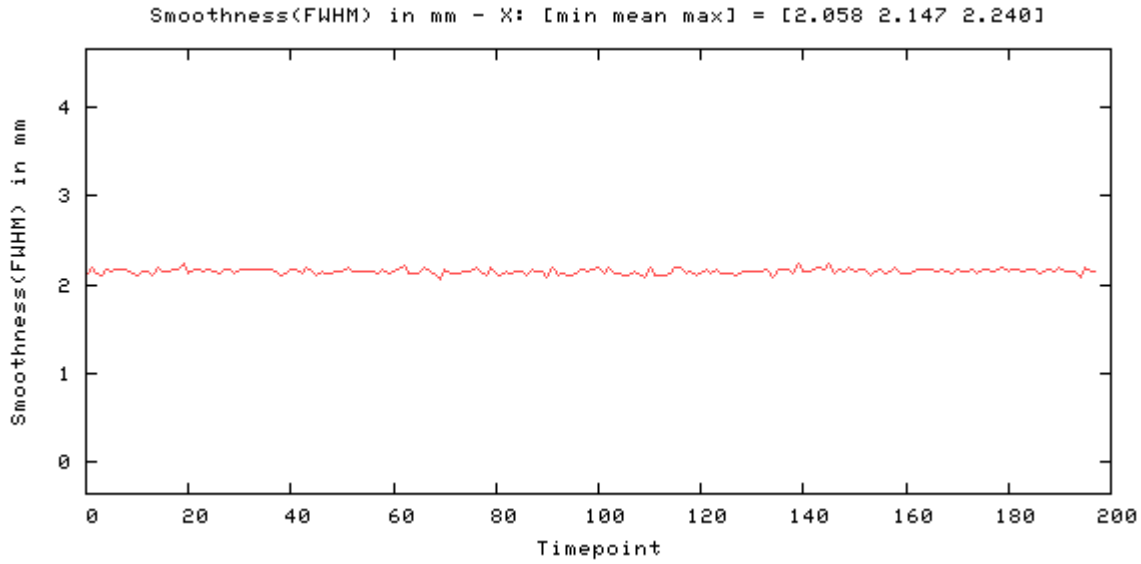


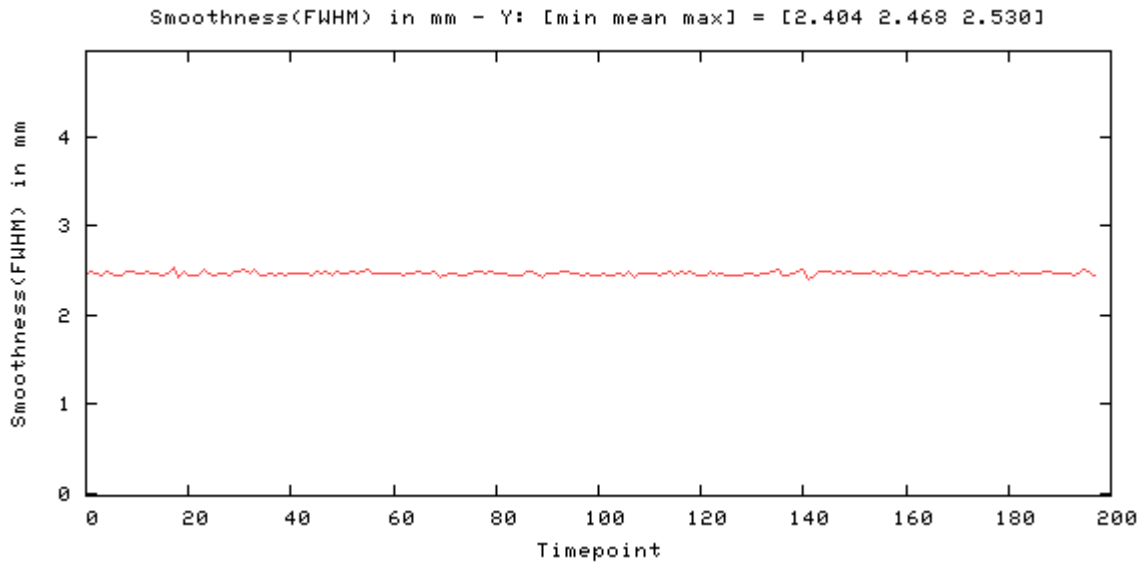




rdc = 9.1 pixels
calc.
meas.
Relative std, %
10
1
0.1
0.01
1
10
ROI full width, pixels



Smoothness(FWHM) in mm - X: [min mean max] = [2.058 2.147 2.240]
Smoothness(FWHM) in mm
4
3
2
1
0
0
20
40
60
80
100
120
140
160
180
200
Timepoint



Smoothness(FWHM) in mm - Y: [min mean max] = [2.404 2.468 2.530]
Smoothness(FWHM) in mm
4
3
2
1
0
0
20
40
60
80
100
120
140
160
180
200
Timepoint

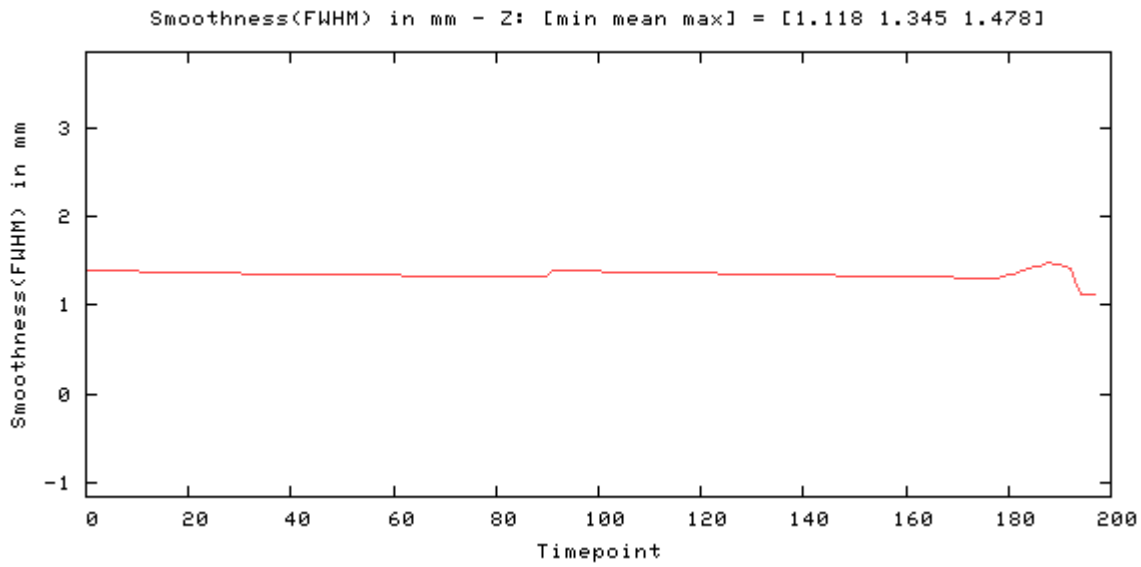
Smoothness(FWHM) in mm - Z: [min mean max] = [1.118 1.345 1.478]
Smoothness(FWHM) in mm
3
2
1
0
-1
0
20
40
60
80
100
120
140
160
180
200
Timepoint

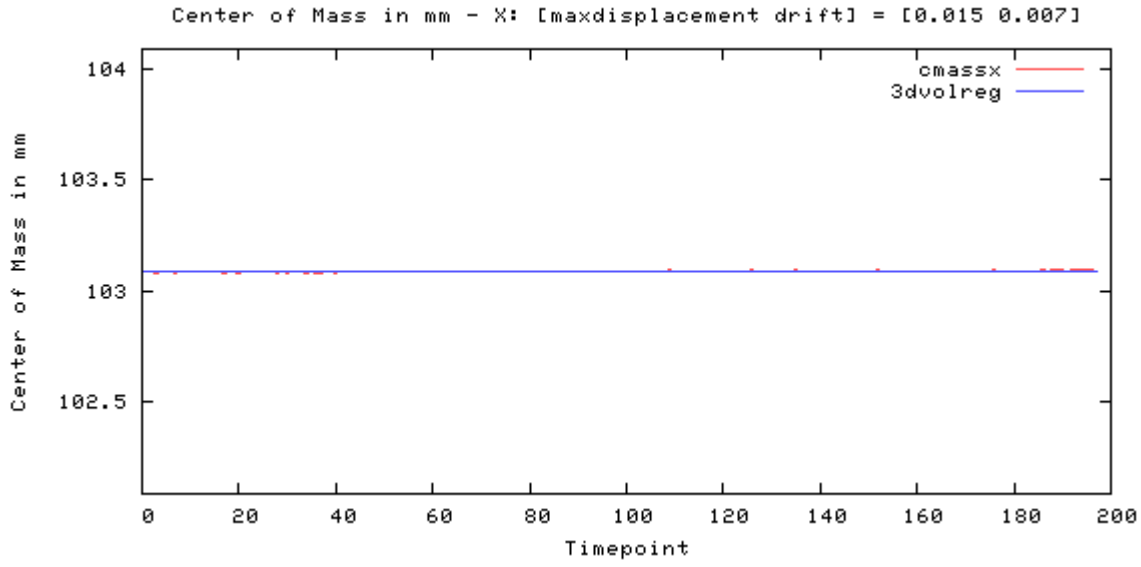
Center of Mass in mm - X: [maxdisplacement drift] = [0.015 0.007]
Center of Mass in mm
104
103.5
103
102.5
cmassx
3dvolreg
0
20
40
60
80
100
120
140
160
180
200
Timepoint

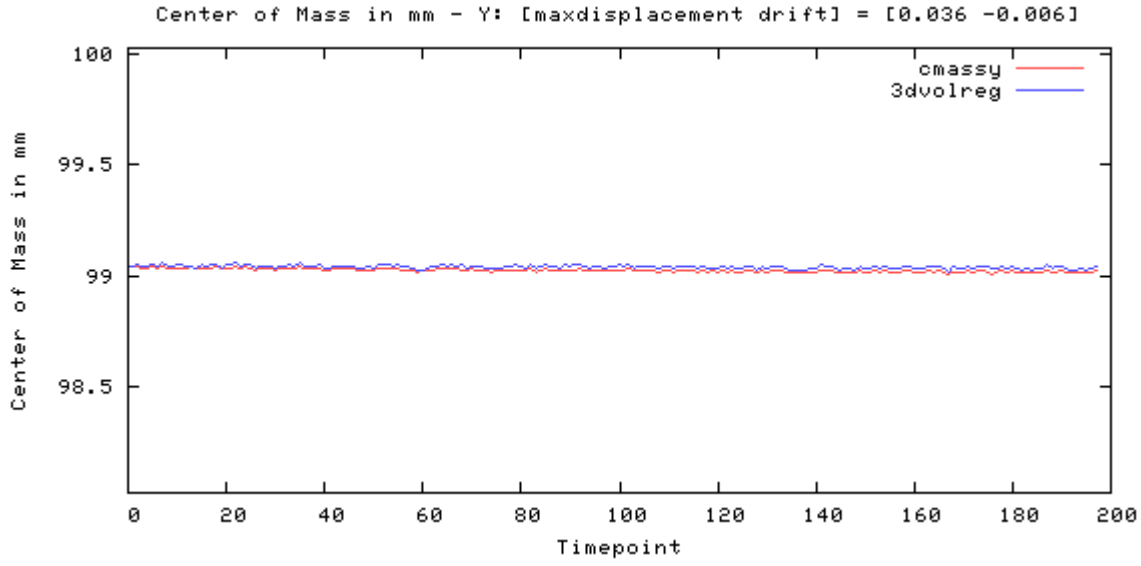
Center of Mass in mm - Y: [maxdisplacement drift] = [0.036 -0.006]
Center of Mass in mm
100
99.5
99
98.5
cmassy
3dvolreg
0
20
40
60
80
100
120
140
160
180
200
Timepoint

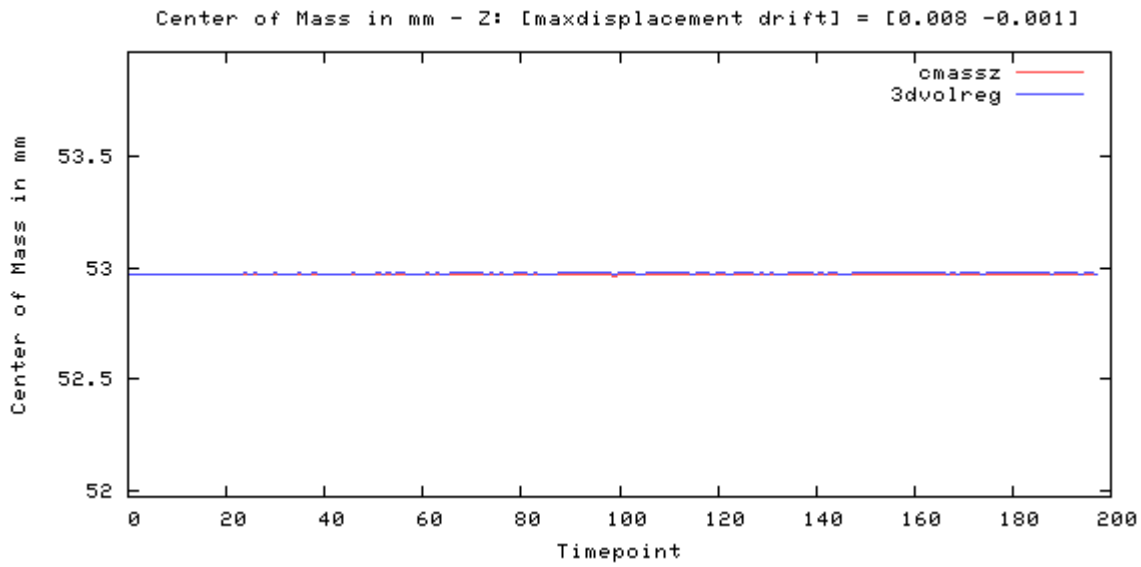


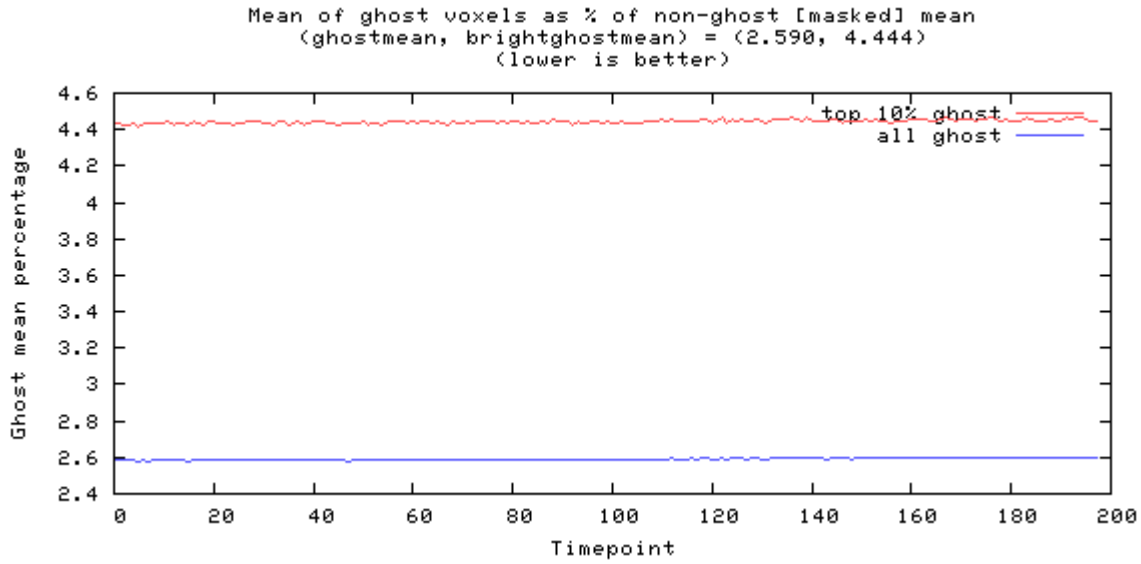

Odd-even difference image



image min: -412, image max: 454

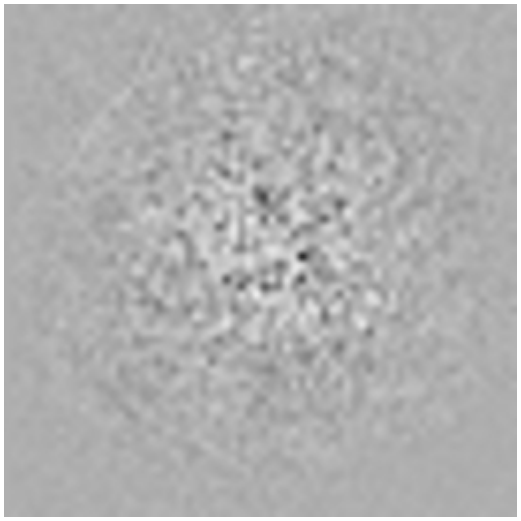

Mean image

0 1326.38


image min: 0, image max: 1326.38



Standard Deviation image

0 12.5071


image min: 0, image max: 12.7156

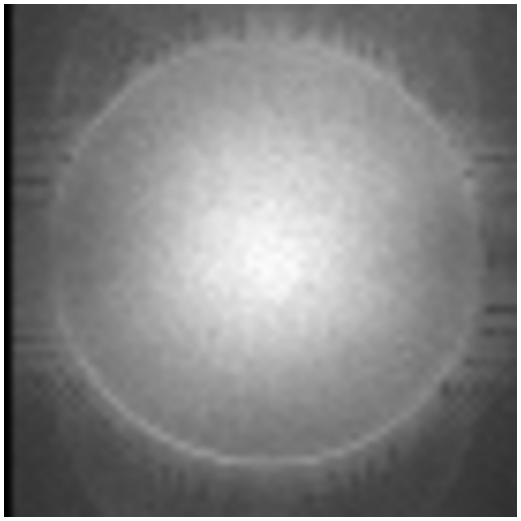

SFNR image



image min: 0, image max: 530.013

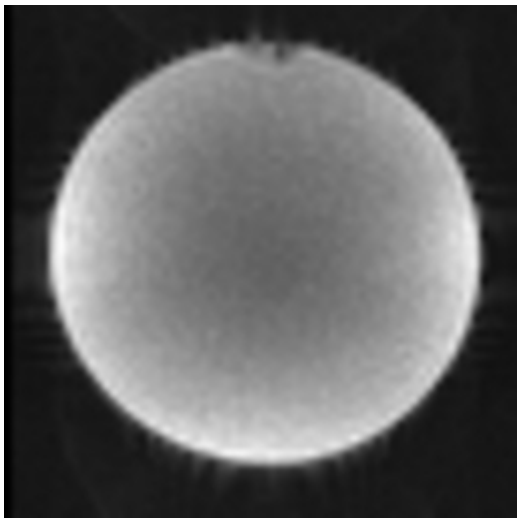

Acquisition parameters

dimensions	68x68x36x200
spacing	3mmx3mmx3mmx2000ms
gap	0mmx0mmx0mmx0ms
scanner	AWP213018
psdname	
examnumber	dc08a757-1251-4f
studyid	Stability_20261109
seriesnumber	4
runnumber	1
magneticfield	3

description	ses-64ch_func-bold_acq-siemensstd_task-tsnr
scandate	2026-11-09
scantime	11:09:03
tr	2000
te	30
operator	
flipangle	79
prescribedslicespacing	3
frequencydirection	1
receivecoilname	HeadNeck_64_CS
transmitcoilname	Body
institution	THE UNIVERSITY OF PENNSYLVANIA
examdescription	ACTIVE KIRWAN
scanner	AWP213018
scannermanufacturer	Siemens Healthineers
scannermodelname	MAGNETOM Cima.X
protocolname	ses-64ch_func-bold_acq-siemensstd_task-tsnr
institutionaddress	Grays Ferry Ave. BLDG 250 STE 140 3401,Philadelphia,69 - KEYSTONE,US,19146
institutionaldepartmentname	MindCORE Neuroimaging Suite 140
acquisitiondatetime	20261109110901.557500
frametype	ORIGINAL
pixelpresentation	MONOCHROME
volumetricproperties	DISTORTED
volumebasedcalculationtechnique	NONE
complexiimagecomponent	MAGNITUDE
acquisitioncontrast	UNKNOWN
mracquisitiontype	2D
numaverages	1
spacingbetweenslices	3
echotrainlength	33
percentsampling	100
percentphasefieldofview	100
scannerserialnumber	213018
softwareversions	syngo MR XA61
inplanephaseencodingdirection	COLUMN
variableflipangleflag	N
contentqualification	PRODUCT
acquisitionduration	407.92500000000001

resonantnucleus	1H
applicablesafetystandardagency	IEC
acquisitionnumber	1
instancenumber	1
numtemporalpositions	200
samplesperpixel	1
photometricinterpretation	MONOCHROME2
numberofframes	36
rows	68
columns	68
bitsallocated	16
bitsstored	12
highbit	11
lossyimagecompression	00