



Phantom QA results for / fbirn_out/ses-64ch_func-bold_acq-cmrrstd_task-tsnrxacpc.xml, slice 34

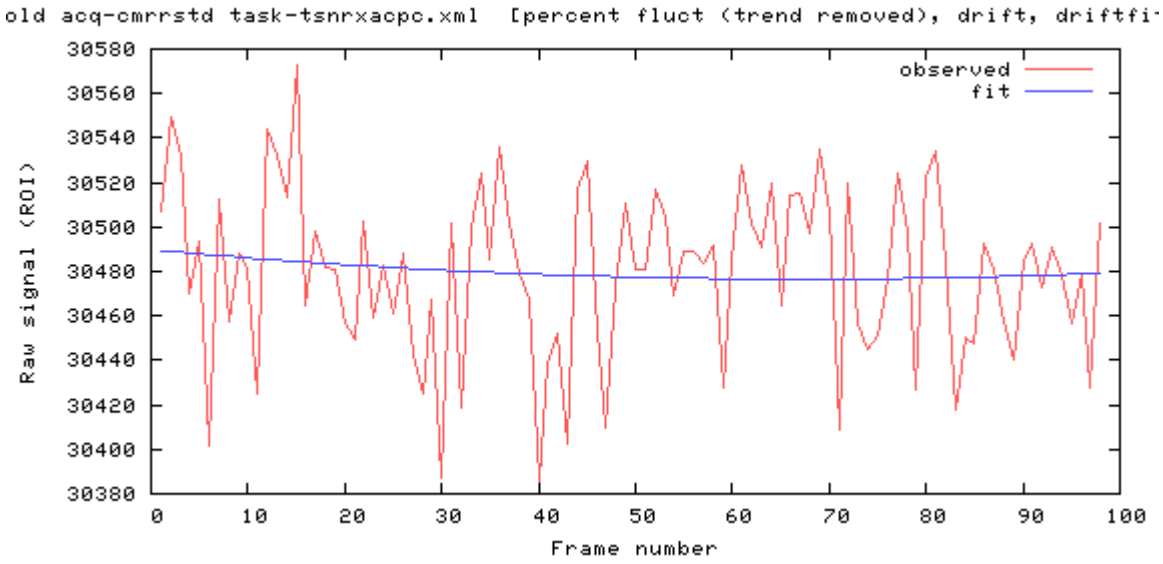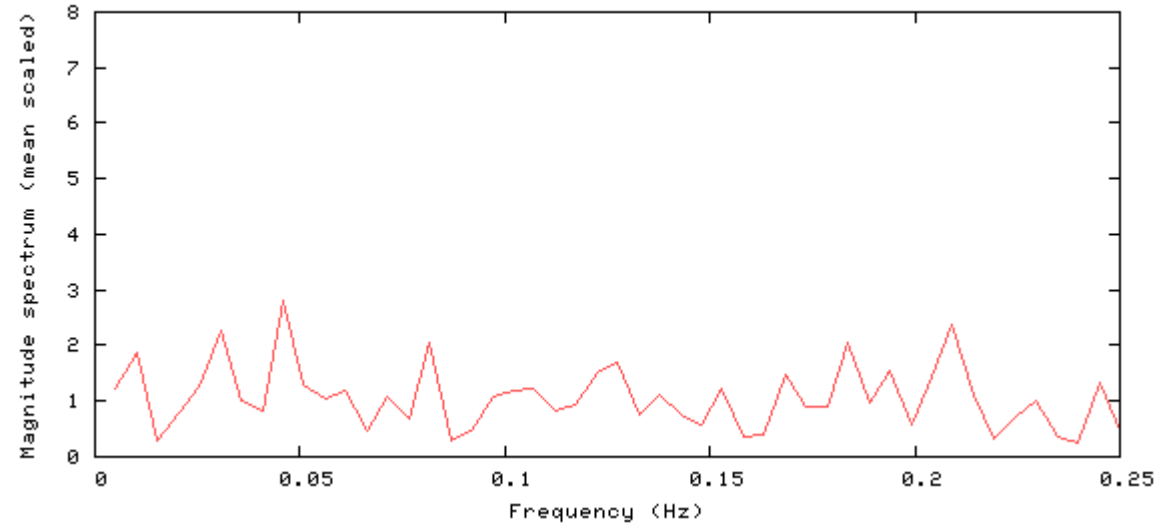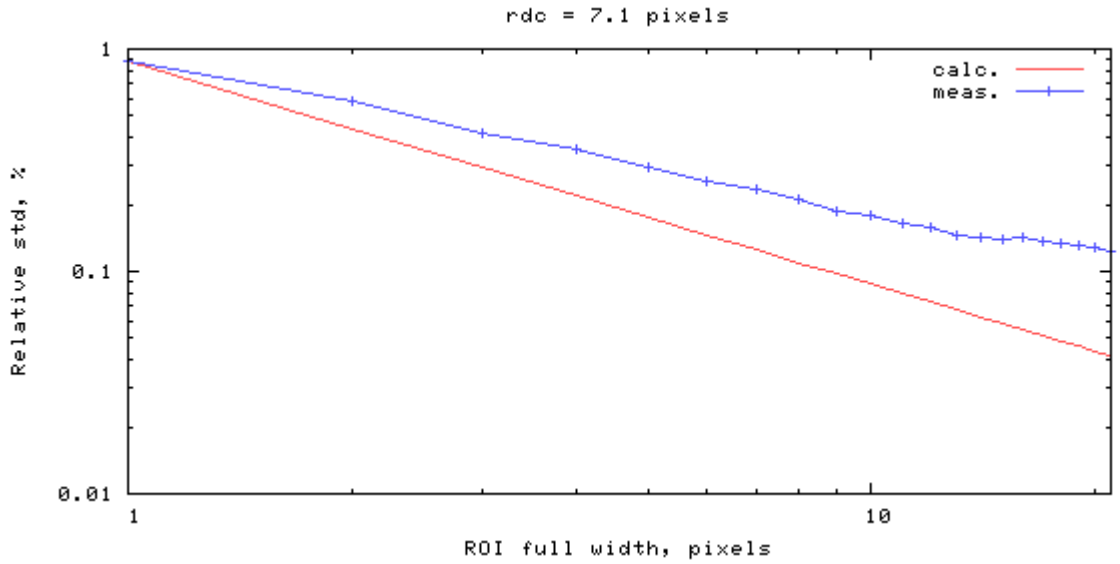



[mean, SNR, SFNR] = [30479.8 118.8 120.5]

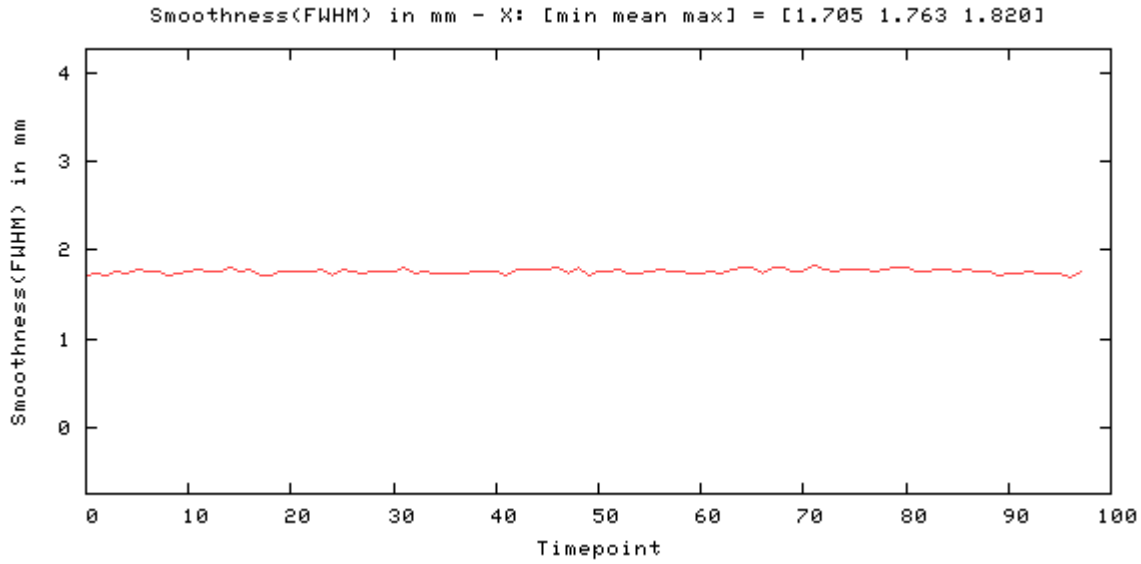




rdc = 7.1 pixels
calc.
meas.
Relative std, %
1
0.1
0.01
1
10
ROI full width, pixels



Smoothness(FWHM) in mm - X: [min mean max] = [1.705 1.763 1.820]
Smoothness(FWHM) in mm
0
1
2
3
4
0
10
20
30
40
50
60
70
80
90
100
Timepoint

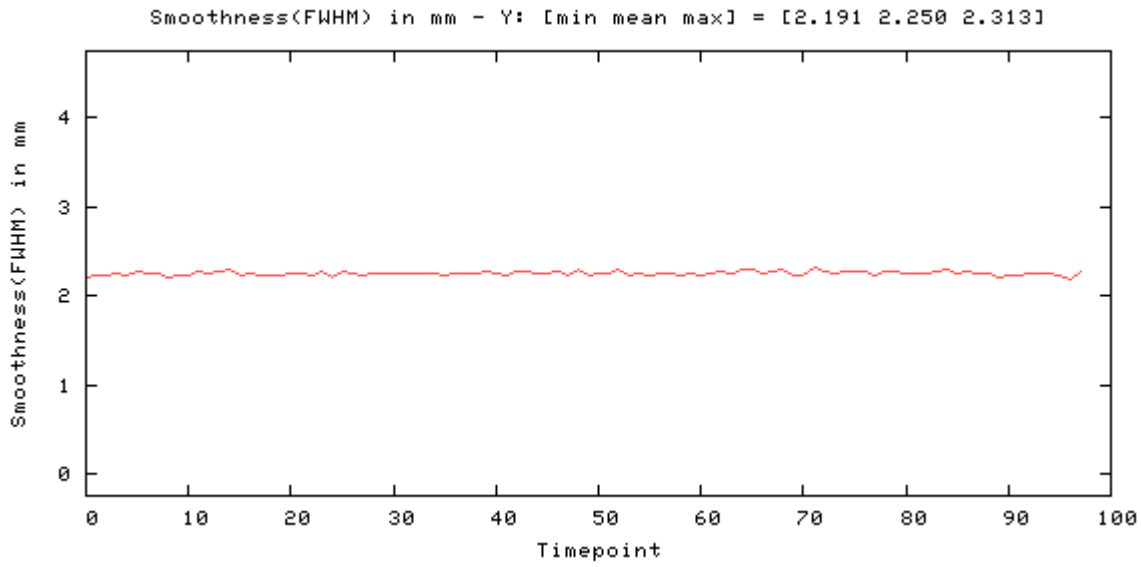

Smoothness(FWHM) in mm - Y: [min mean max] = [2.191 2.250 2.313]
Smoothness(FWHM) in mm
0
1
2
3
4
0
10
20
30
40
50
60
70
80
90
100
Timepoint

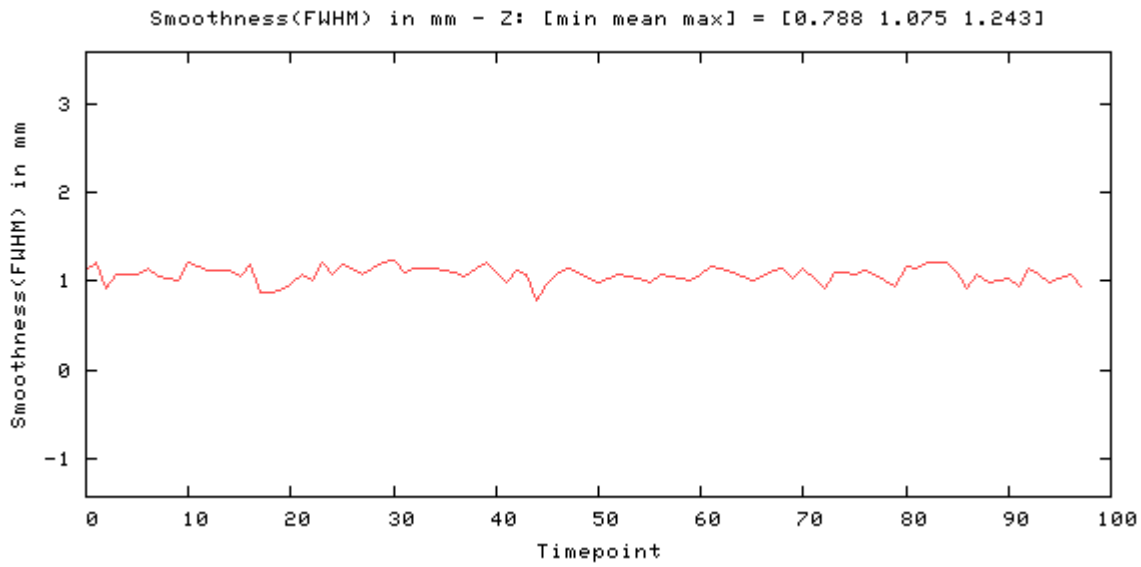
Smoothness(FWHM) in mm - Z: [min mean max] = [0.788 1.075 1.243]
Smoothness(FWHM) in mm
3
2
1
0
-1
0
10
20
30
40
50
60
70
80
90
100
Timepoint

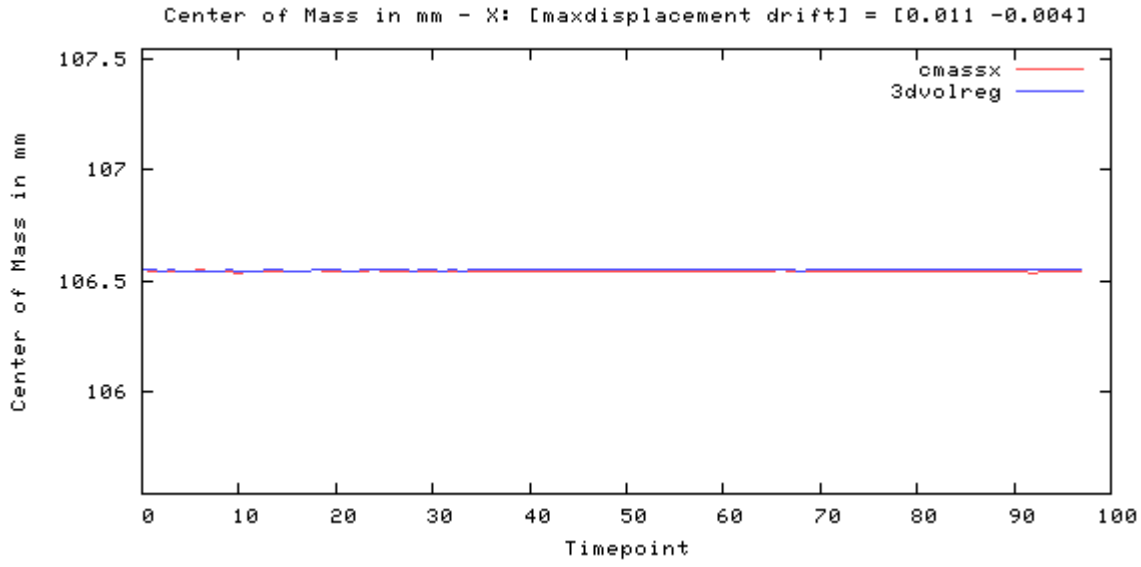
Center of Mass in mm - X: [maxdisplacement drift] = [0.011 -0.004]
Center of Mass in mm
107.5
107
106.5
106
cmassx
3dvolreg
0
10
20
30
40
50
60
70
80
90
100
Timepoint

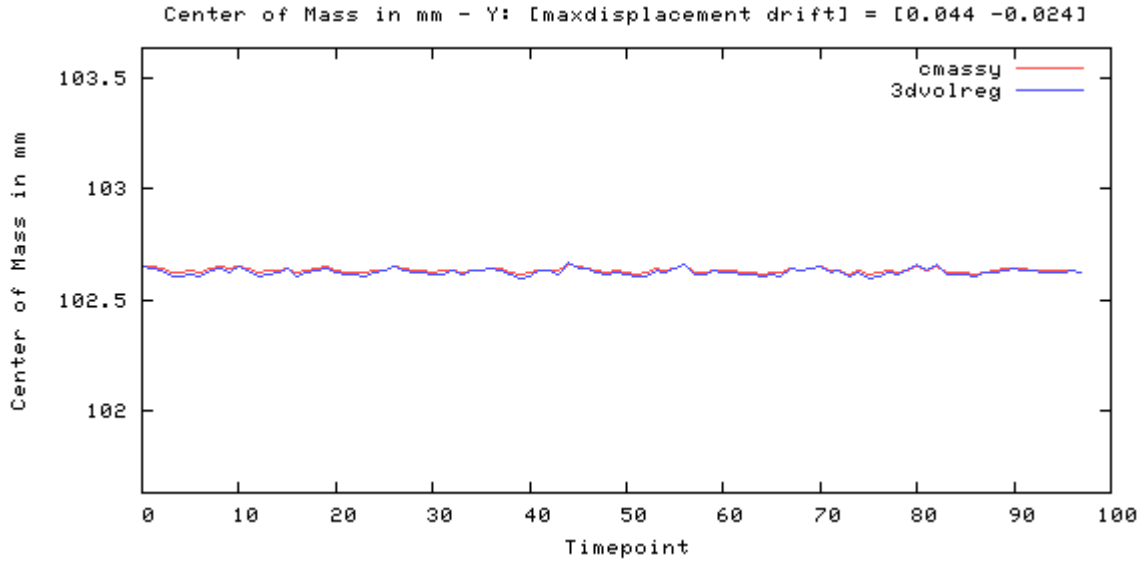
Center of Mass in mm - Y: [maxdisplacement drift] = [0.044 -0.024]
Center of Mass in mm
103.5
103
102.5
102
cmassy
3dvolreg
0
10
20
30
40
50
60
70
80
90
100
Timepoint

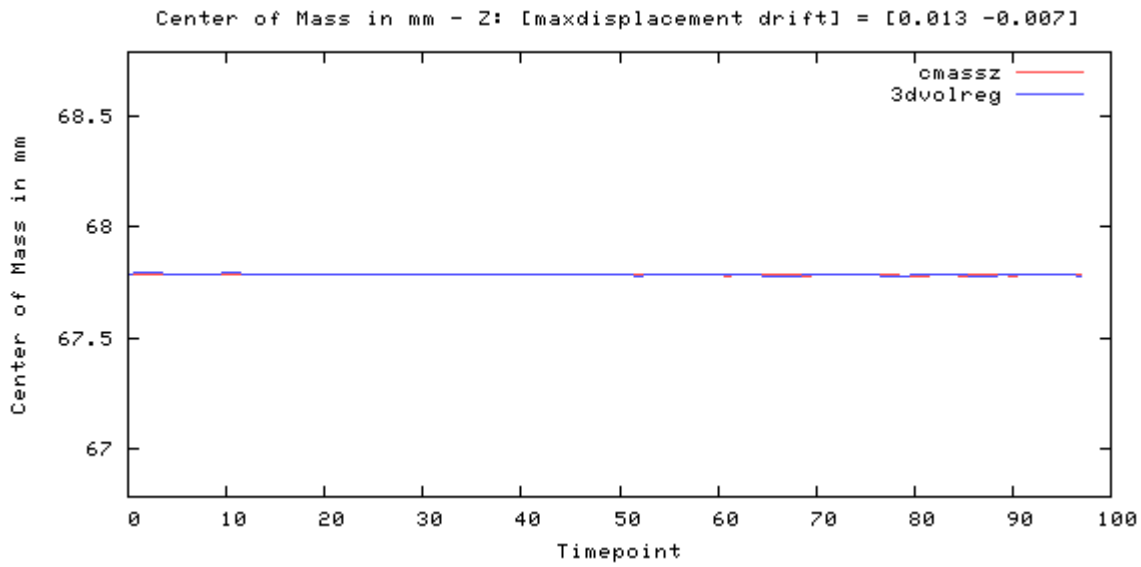


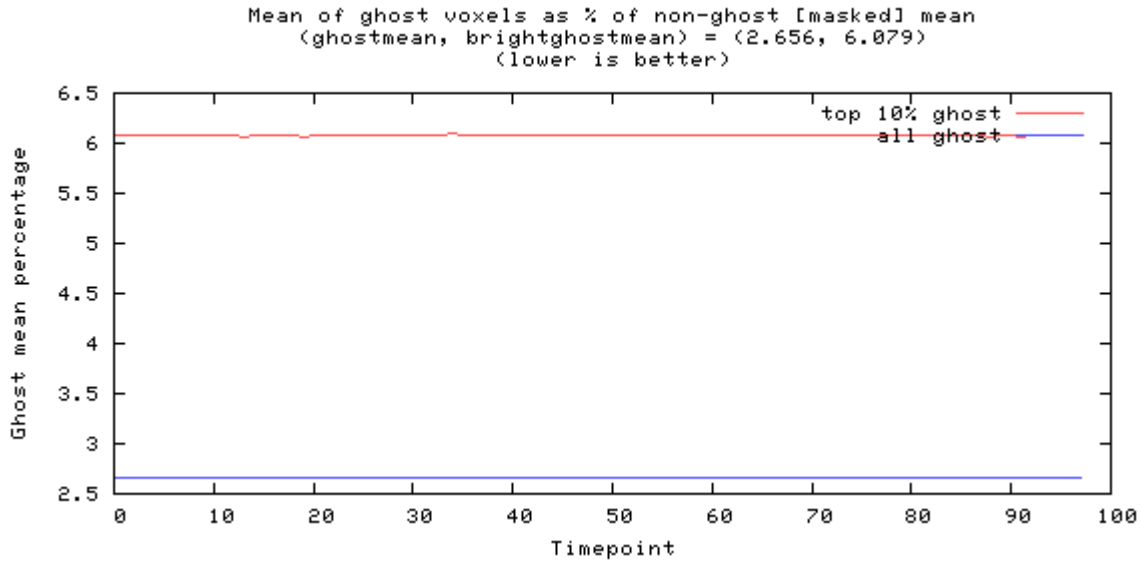

Odd-even difference image




image min: -7609, image max: 8257

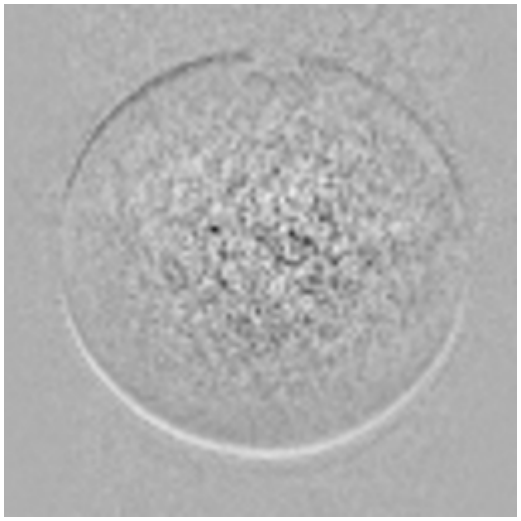

Mean image

0 44558.6


image min: 0, image max: 44558.6

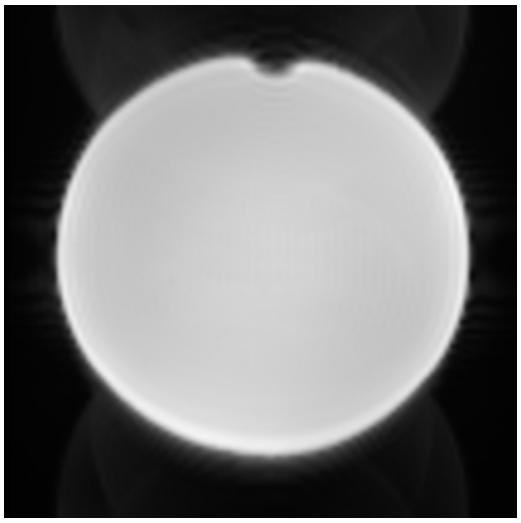

Standard Deviation image

0 347.676


image min: 0, image max: 347.676

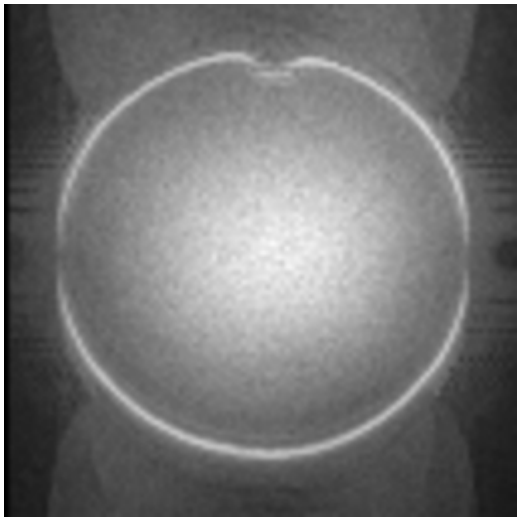

SFNR image

0 724.02

image min: 0, image max: 724.02

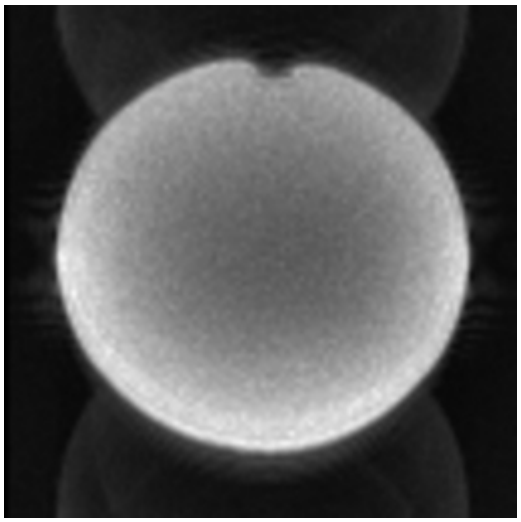

Acquisition parameters

dimensions	106x106x69x100
spacing	2mmx2mmx2mmx2000ms
gap	0mmx0mmx0mmx0ms
scanner	AWP213018
psdname	
examnumber	847307d4-ec84-45
studyid	Stability_20261005
seriesnumber	10
runnumber	1
magneticfield	3

description	ses-64ch_func-bold_acq-cmrrstd_task-tsnrxacpc
scandate	2026-10-05
scantime	11:22:12
tr	2000
te	30
operator	
flipangle	79
prescribedslicespacing	2
frequencydirection	1
receivecoilname	HeadNeck_64_CS
transmitcoilname	Body
institution	THE UNIVERSITY OF PENNSYLVANIA
examdescription	ACTIVE KIRWAN
scanner	AWP213018
scannermanufacturer	Siemens Healthineers
scannermodelname	MAGNETOM Cima.X
protocolname	ses-64ch_func-bold_acq-cmrrstd_task-tsnrxacpc
institutionaddress	Grays Ferry Ave. BLDG 250 STE 140 3401,Philadelphia,69 - KEYSTONE,US,19146
institutionaldepartmentname	MindCORE Neuroimaging Suite 140
acquisitiondatetime	20261005112210.235000
frametype	ORIGINAL
pixelpresentation	MONOCHROME
volumetricproperties	DISTORTED
volumebasedcalculationtechnique	NONE
complexitimagecomponent	MAGNITUDE
acquisitioncontrast	UNKNOWN
mracquisitiontype	2D
numaverages	1
spacingbetweenslices	2
echotrainlength	80
percentsampling	100
percentphasefieldofview	100
scannerserialnumber	213018
softwareversions	syngo MR XA61
inplanephaseencodingdirection	COLUMN
variableflipangleflag	N
contentqualification	RESEARCH
acquisitionduration	217.892

resonantnucleus	1H
applicablesafetystandardagency	IEC
acquisitionnumber	1
instancenumber	1
numtemporalpositions	100
imagecomments	Not for diagnostic use, Unaliased MB3/ PE3/LB
samplesperpixel	1
photometricinterpretation	MONOCHROME2
numberofframes	69
rows	106
columns	106
bitsallocated	16
bitsstored	16
highbit	15
lossyimagecompression	00