



Phantom QA results for / fbirn_out/ses-64ch_func-bold_acq-cmrrstd_task-warmup.xml, slice 34

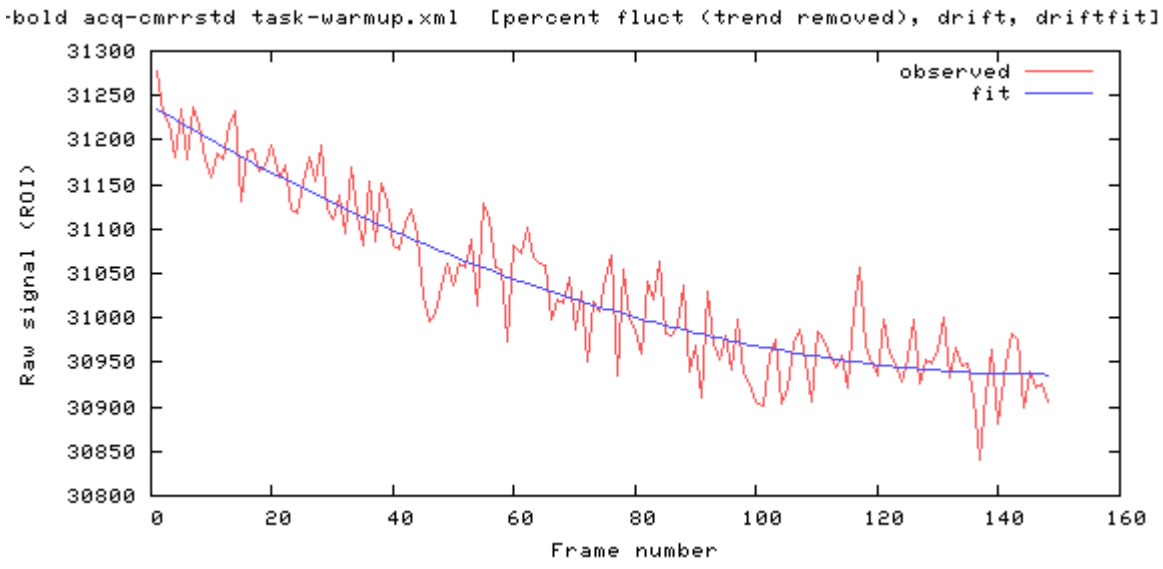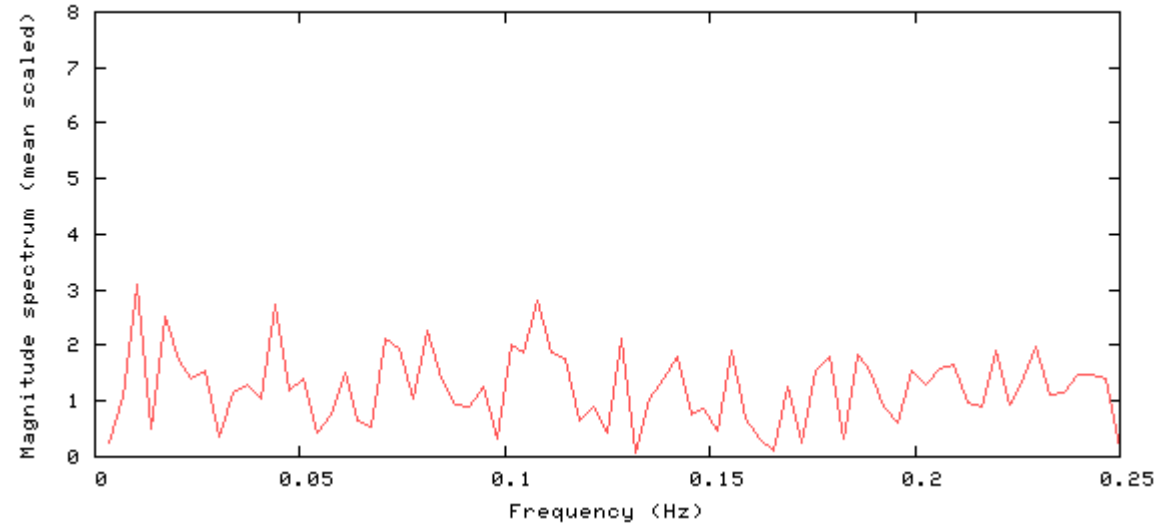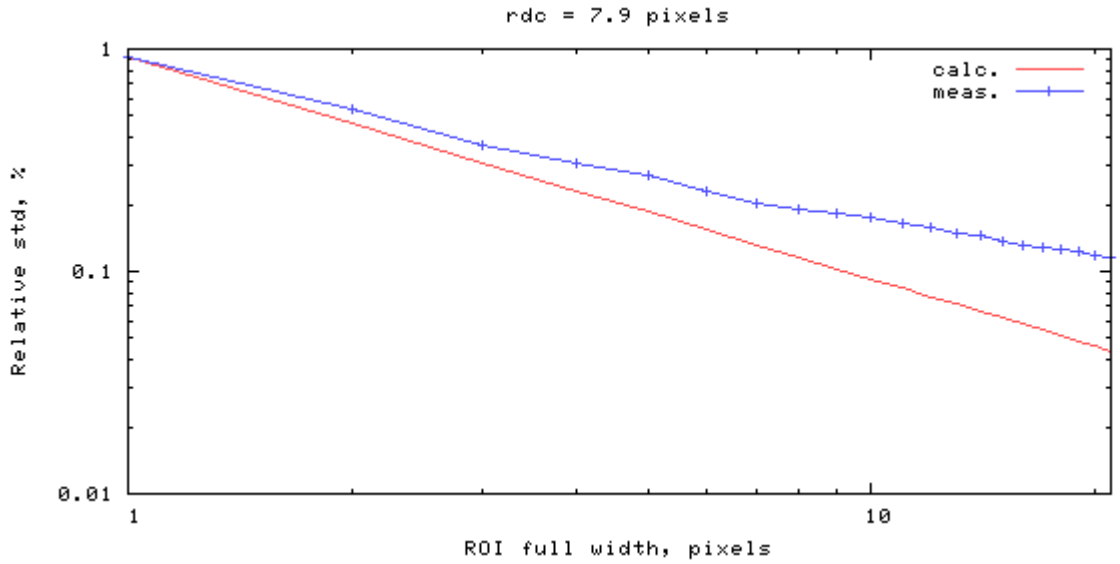



[mean, SNR, SFNR] = [31036.5 119.4 120.6]

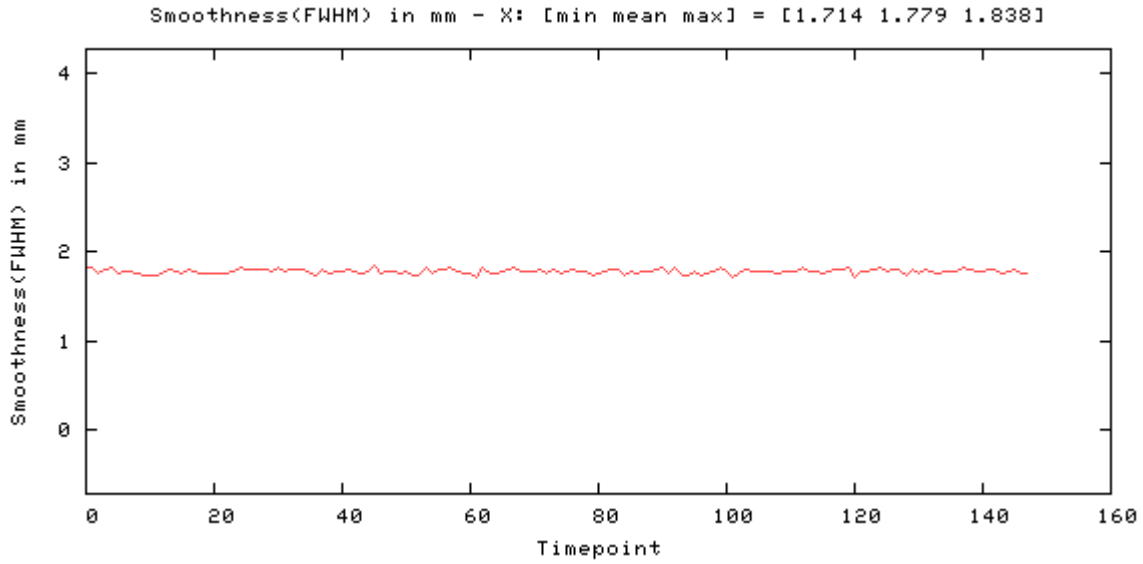




rdc = 7.9 pixels
calc.
meas.
Relative std, %
1
0.1
0.01
1
10
ROI full width, pixels



Smoothness(FWHM) in mm - X: [min mean max] = [1.714 1.779 1.838]
Smoothness(FWHM) in mm
0
1
2
3
4
0
20
40
60
80
100
120
140
160
Timepoint

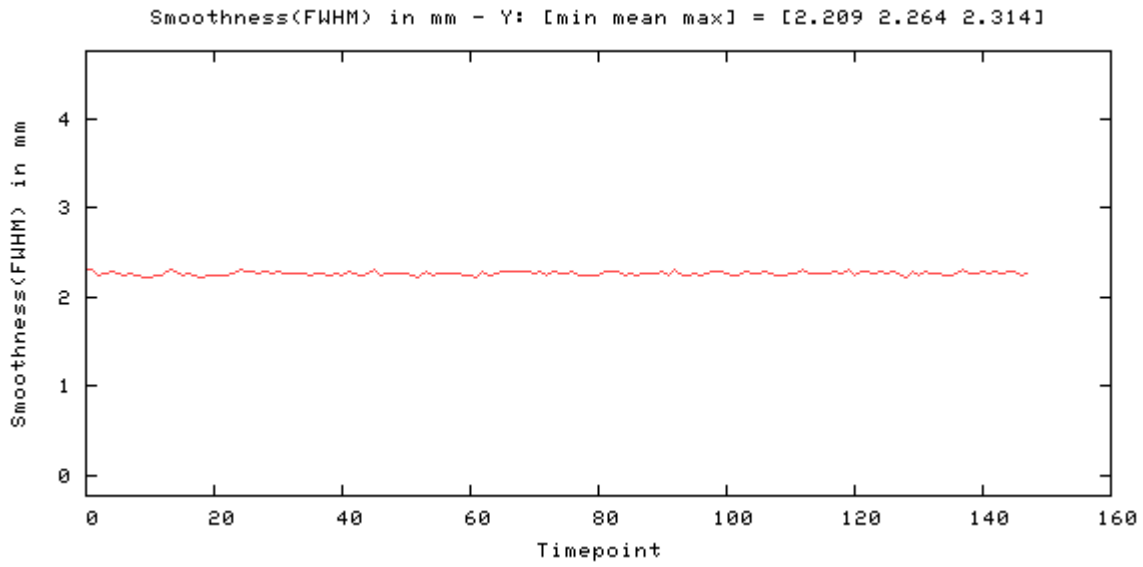

Smoothness(FWHM) in mm - Y: [min mean max] = [2.209 2.264 2.314]
Smoothness(FWHM) in mm
0
1
2
3
4
0
20
40
60
80
100
120
140
160
Timepoint

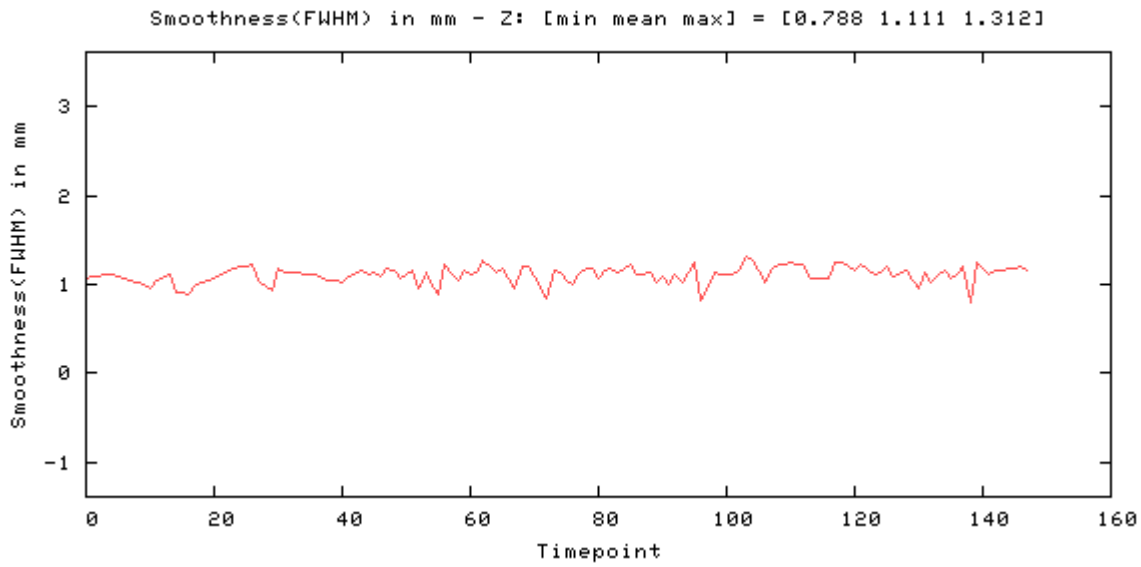
Smoothness(FWHM) in mm - Z: [min mean max] = [0.788 1.111 1.312]
Smoothness(FWHM) in mm
3
2
1
0
-1
0
20
40
60
80
100
120
140
160
Timepoint

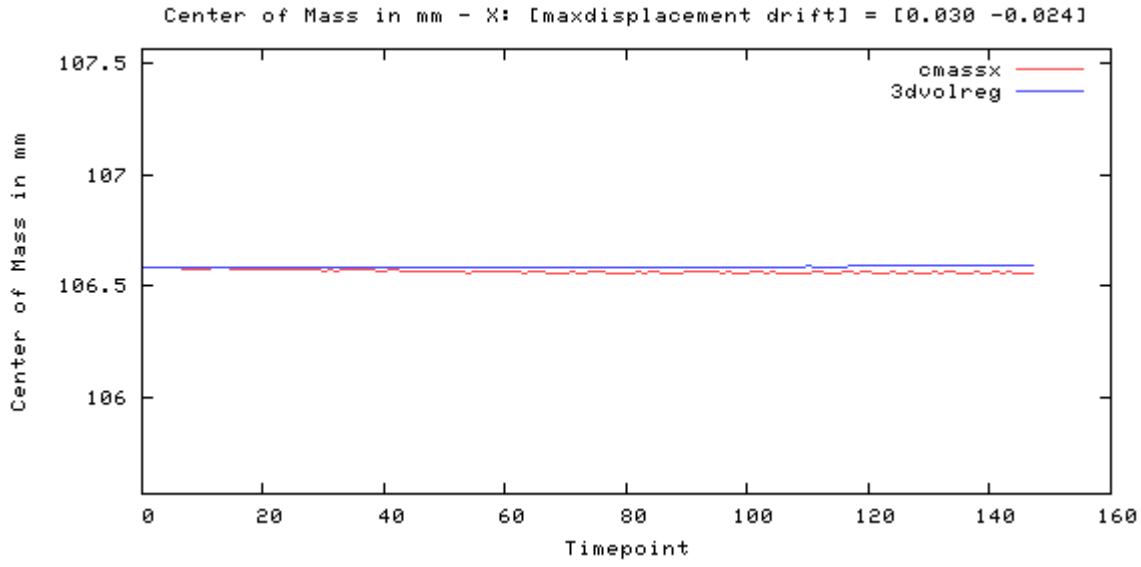
Center of Mass in mm - X: [maxdisplacement drift] = [0.030 -0.024]
Center of Mass in mm
107.5
107
106.5
106
cmassx
3dvolreg
0
20
40
60
80
100
120
140
160
Timepoint

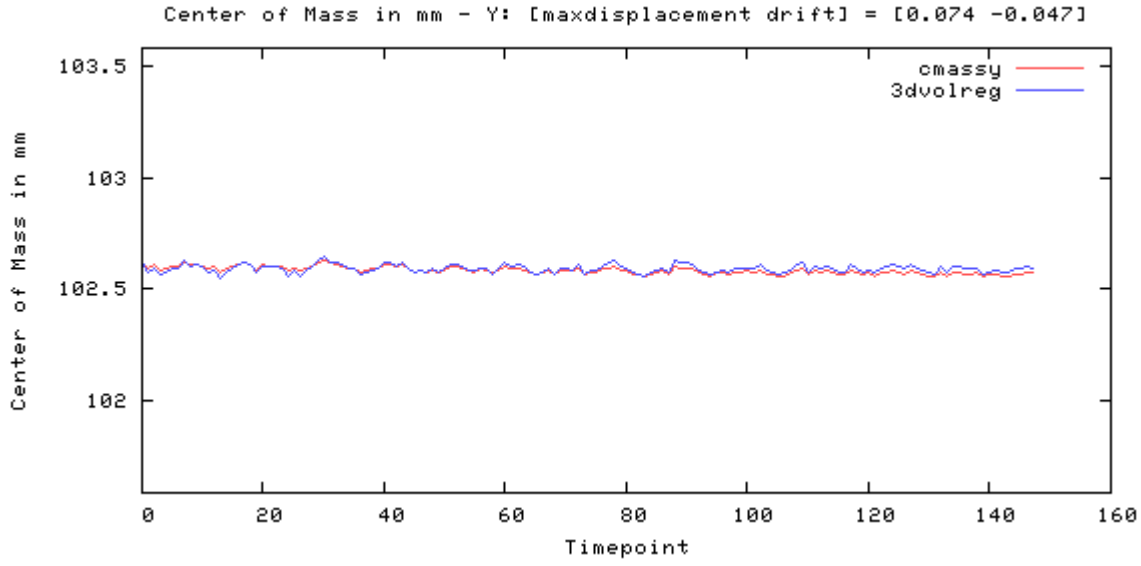
Center of Mass in mm - Y: [maxdisplacement drift] = [0.074 -0.047]
Center of Mass in mm
103.5
103
102.5
102
cmassy
3dvolreg
0
20
40
60
80
100
120
140
160
Timepoint

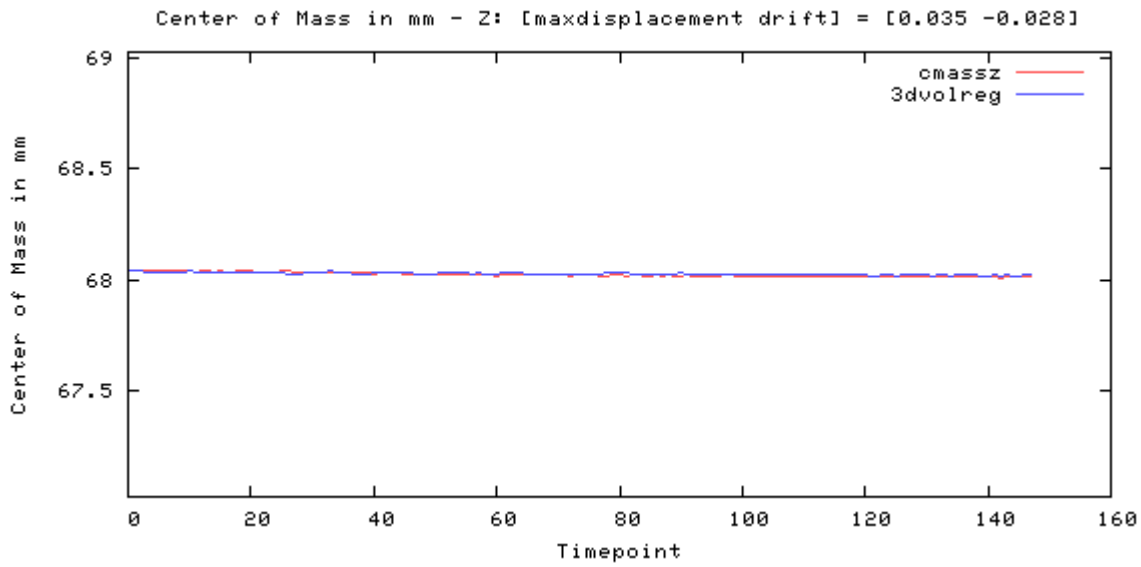


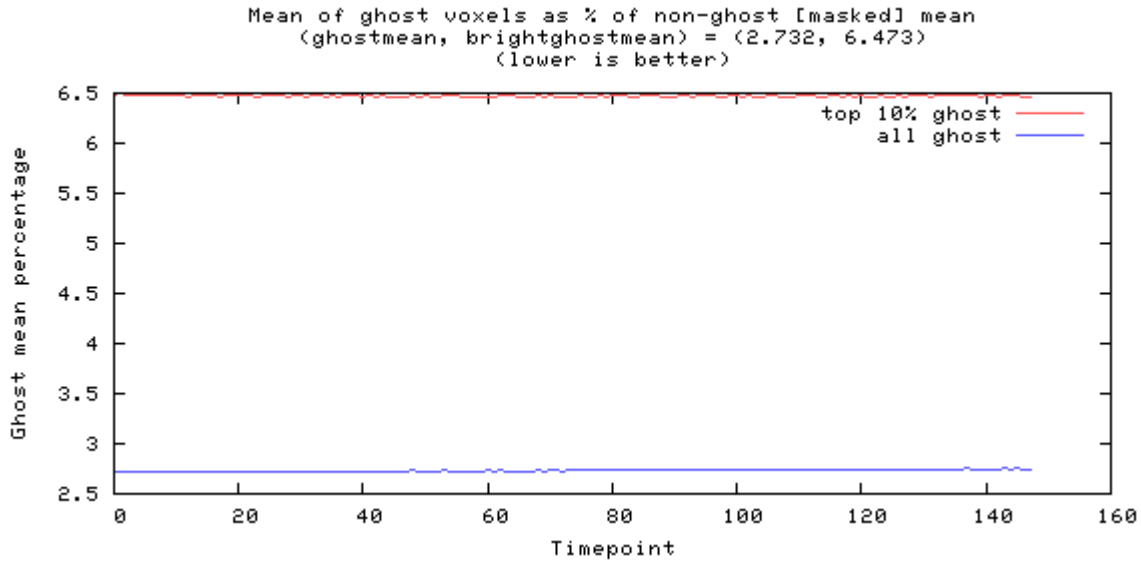

Odd-even difference image




image min: -10253, image max: 10688

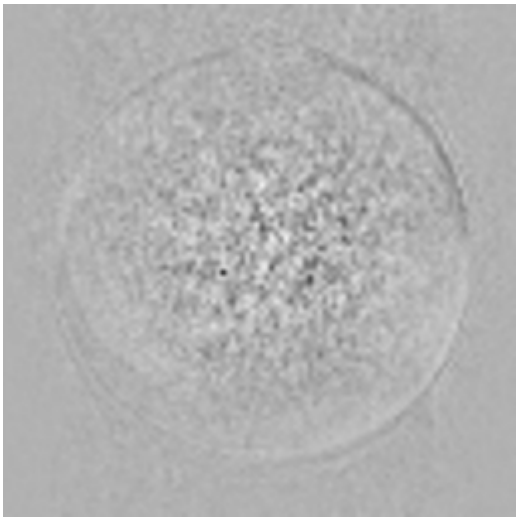

Mean image

0 44493.4


image min: 0, image max: 44493.4

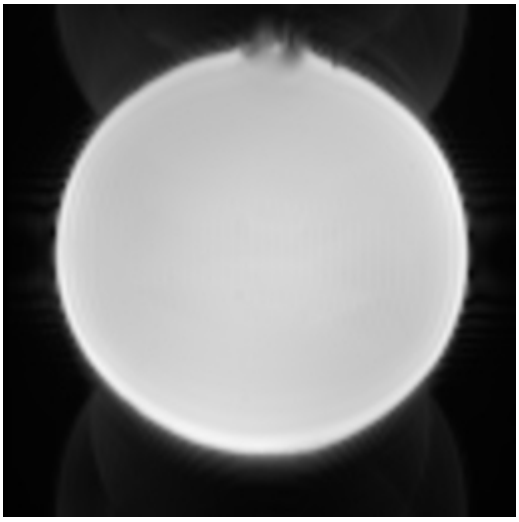

Standard Deviation image

0 323.962


image min: 0, image max: 339.683

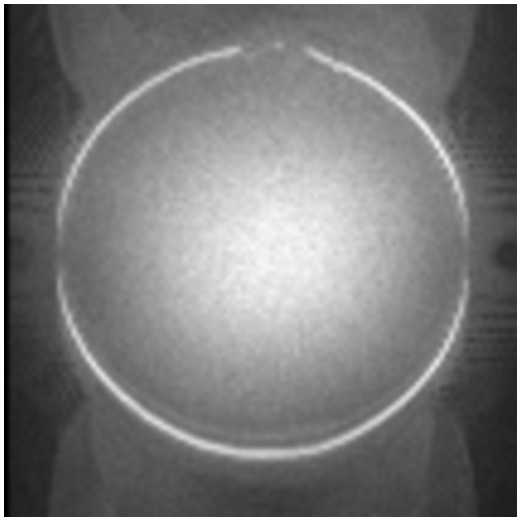

SFNR image



image min: 0, image max: 731.387

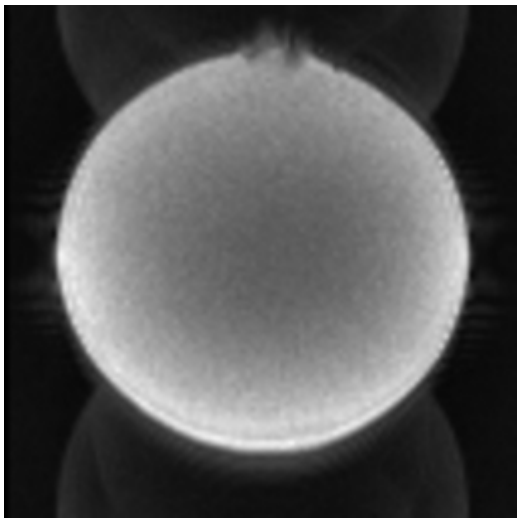

Acquisition parameters

dimensions	106x106x69x150
spacing	2mmx2mmx2mmx2000ms
gap	0mmx0mmx0mmx0ms
scanner	AWP213018
psdname	
examnumber	847307d4-ec84-45
studyid	Stability_20261005
seriesnumber	2
runnumber	1
magneticfield	3

description	ses-64ch_func-bold_acq-cmrrstd_task-warmup
scandate	2026-10-05
scantime	10:54:14
tr	2000
te	30
operator	
flipangle	79
prescribedslicespacing	2
frequencydirection	1
receivecoilname	HeadNeck_64_CS
transmitcoilname	Body
institution	THE UNIVERSITY OF PENNSYLVANIA
examdescription	ACTIVE KIRWAN
scanner	AWP213018
scannermanufacturer	Siemens Healthineers
scannermodelname	MAGNETOM Cima.X
protocolname	ses-64ch_func-bold_acq-cmrrstd_task-warmup
institutionaddress	Grays Ferry Ave. BLDG 250 STE 140 3401,Philadelphia,69 - KEYSTONE,US,19146
institutionaldepartmentname	MindCORE Neuroimaging Suite 140
acquisitiondatetime	20261005105411.987500
frametype	ORIGINAL
pixelpresentation	MONOCHROME
volumetricproperties	DISTORTED
volumebasedcalculationtechnique	NONE
complexitimagecomponent	MAGNITUDE
acquisitioncontrast	UNKNOWN
mracquisitiontype	2D
numaverages	1
spacingbetweenslices	2
echotrainlength	80
percentsampling	100
percentphasefieldofview	100
scannerserialnumber	213018
softwareversions	syngo MR XA61
inplanephaseencodingdirection	COLUMN
variableflipangleflag	N
contentqualification	RESEARCH
acquisitionduration	317.892

resonantnucleus	1H
applicablesafetystandardagency	IEC
acquisitionnumber	1
instancenumber	1
numtemporalpositions	150
imagecomments	Not for diagnostic use, Unaliased MB3/ PE3/LB
samplesperpixel	1
photometricinterpretation	MONOCHROME2
numberofframes	69
rows	106
columns	106
bitsallocated	16
bitsstored	16
highbit	15
lossyimagecompression	00