






Phantom QA results for / fbirn_out/ ses20ch_funcbold_acqcmrrstd_tasktsnr slice 34




.d acqcmrrstd tasktsnrxaopo 28.xml [percent fluct (trend removed), drift, driftfit


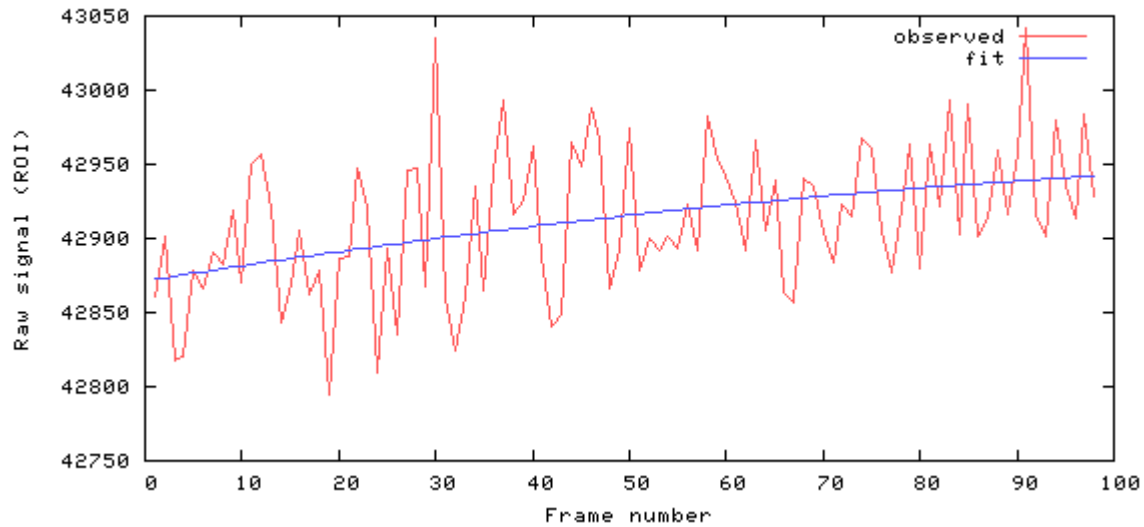


[mean, SNR, SFNR] = [42912.6 124.8 129.1]

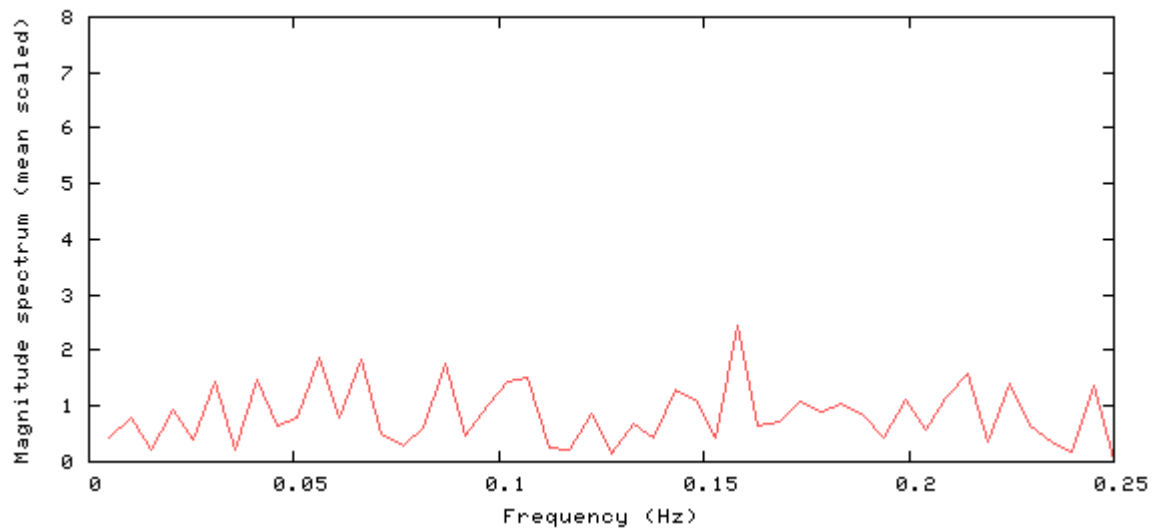

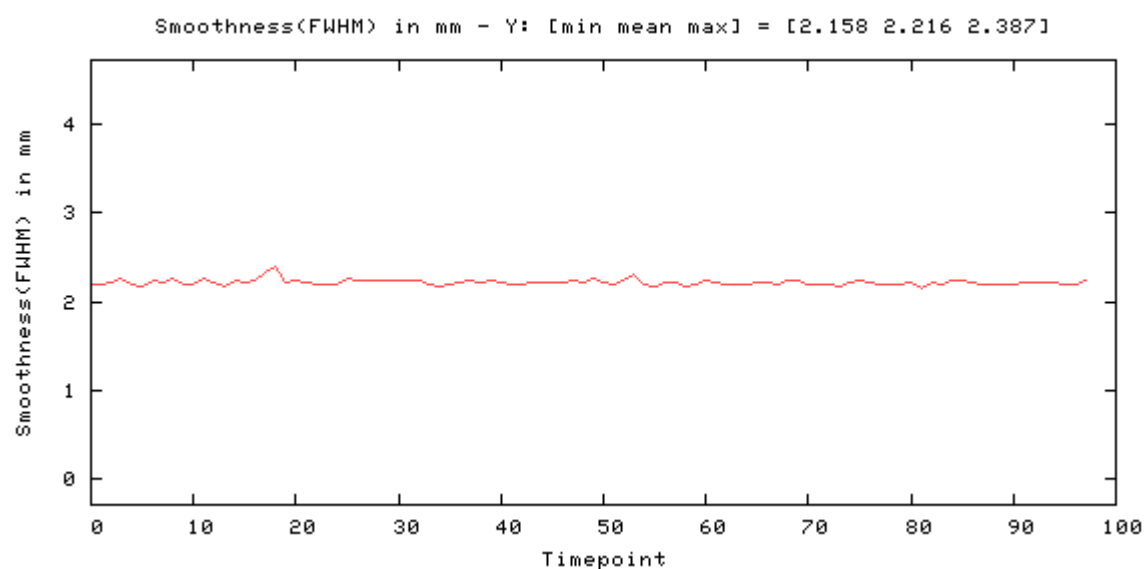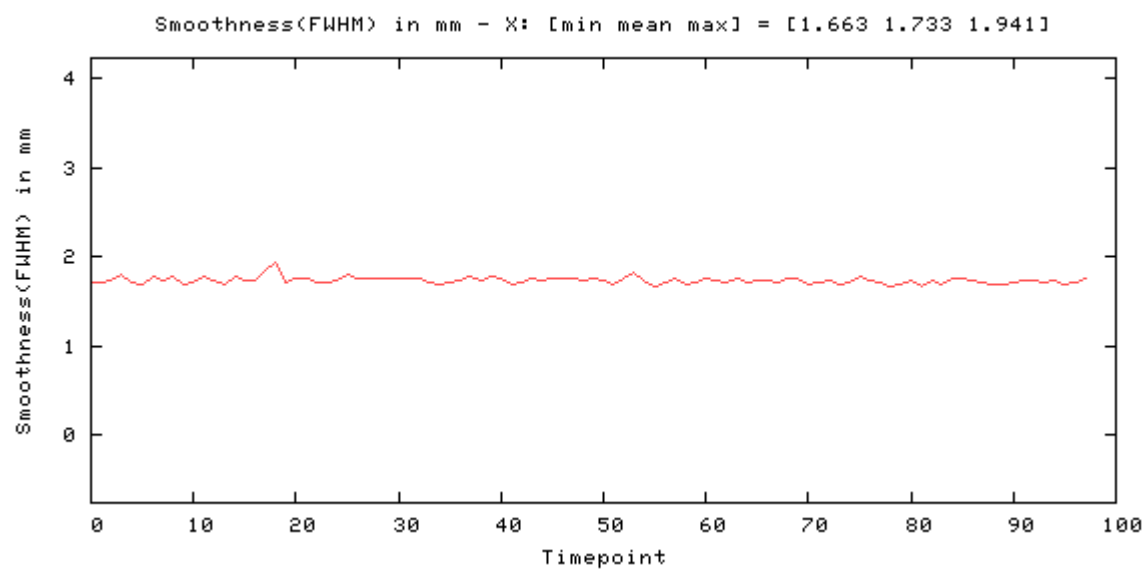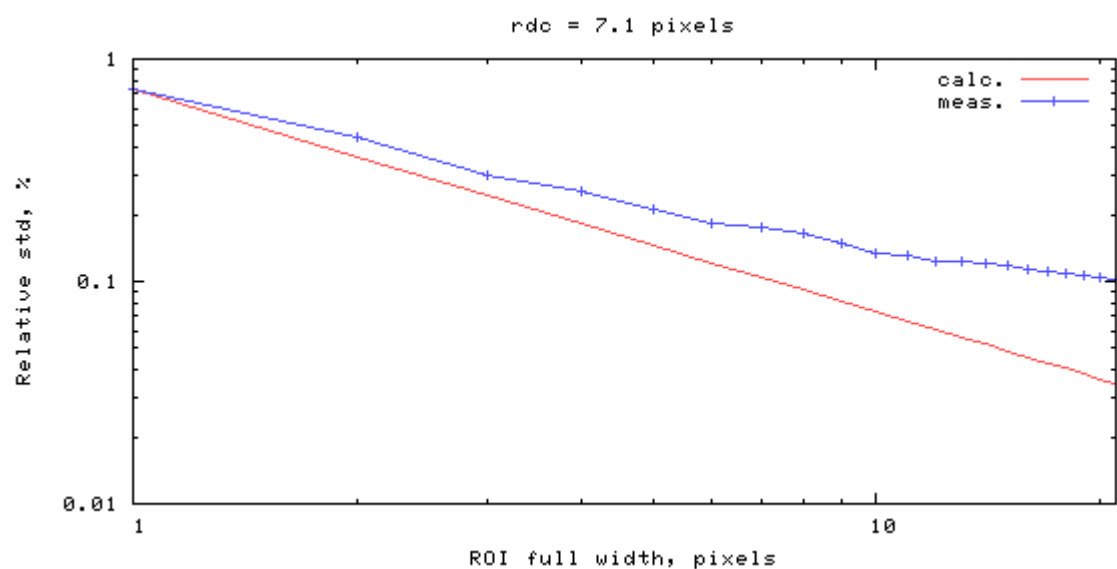

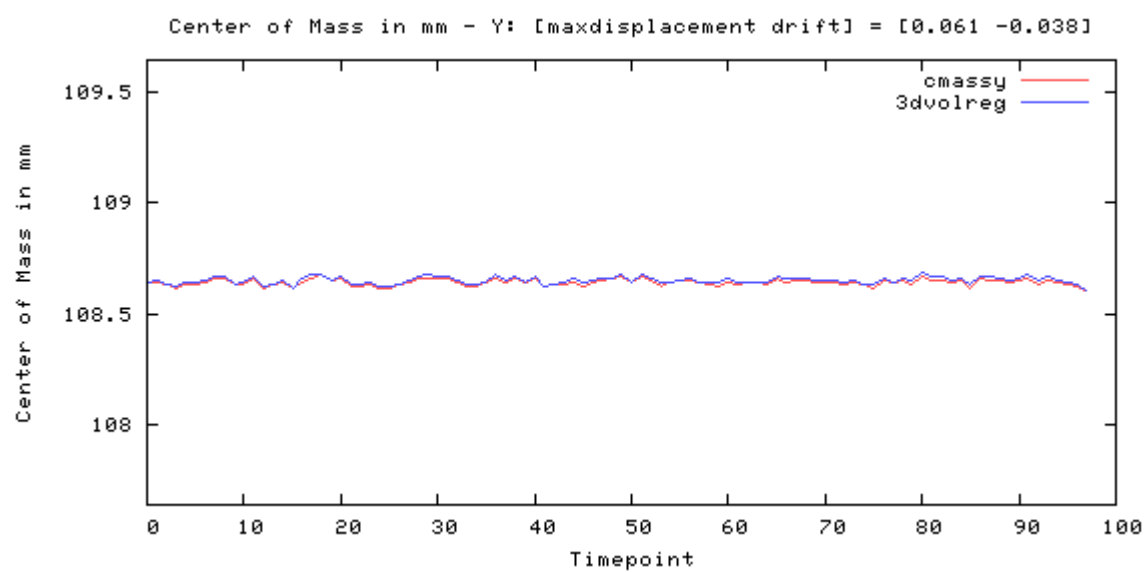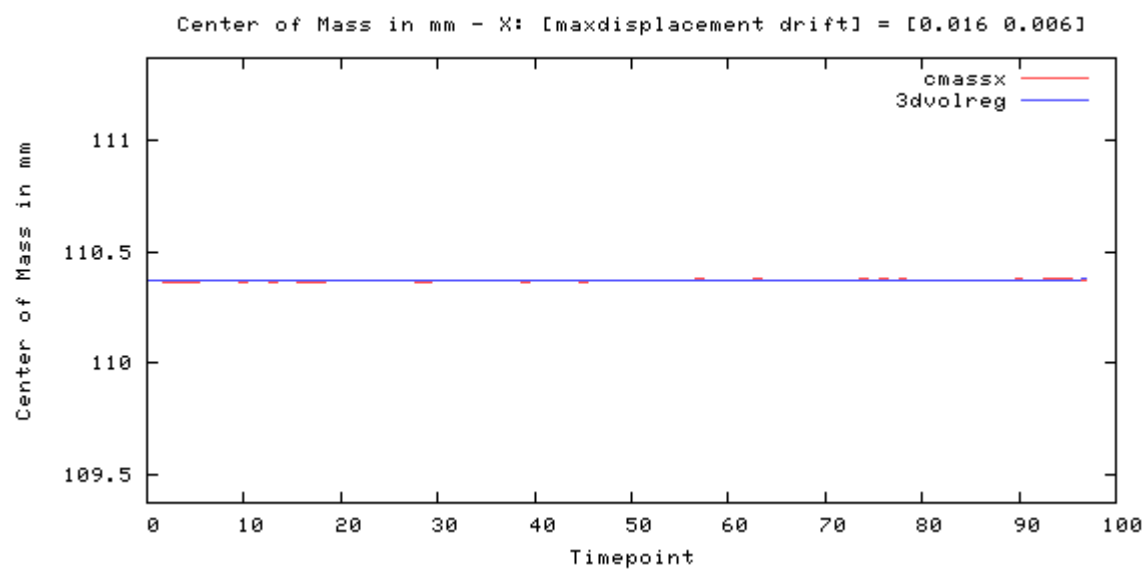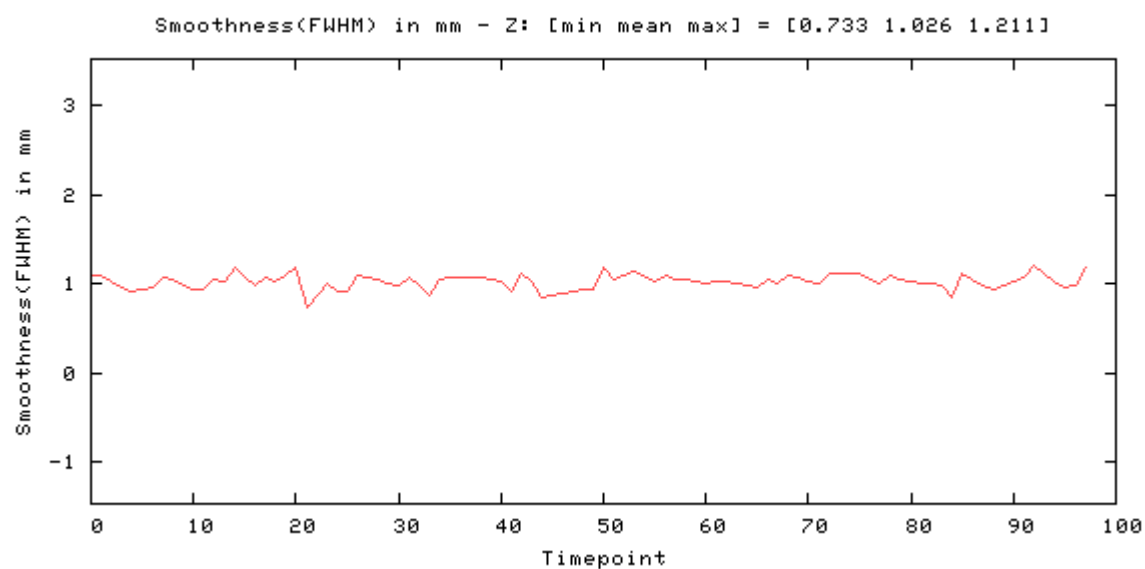

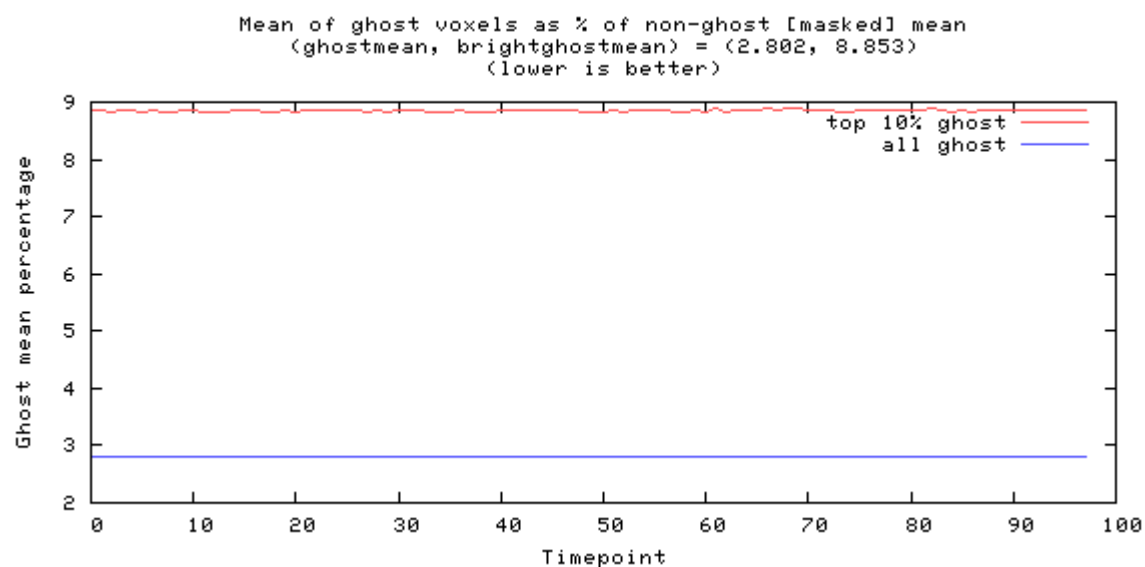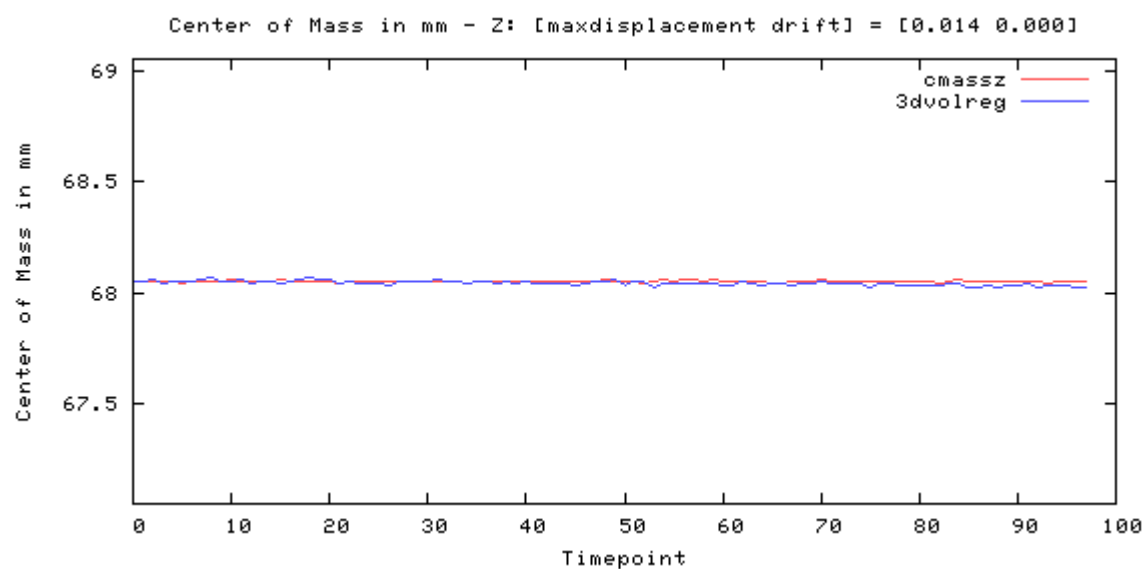


Odd-even difference image

-9170 10494



image min: -11364, image max: 10494

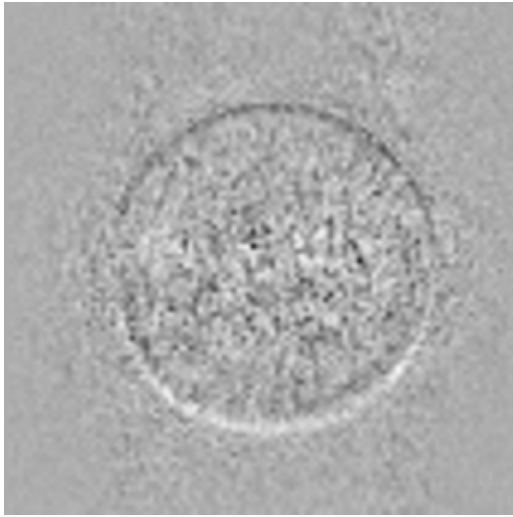

Mean image




image min: 0, image max: 52646.2



Standard Deviation image




image min: 0, image max: 452.585

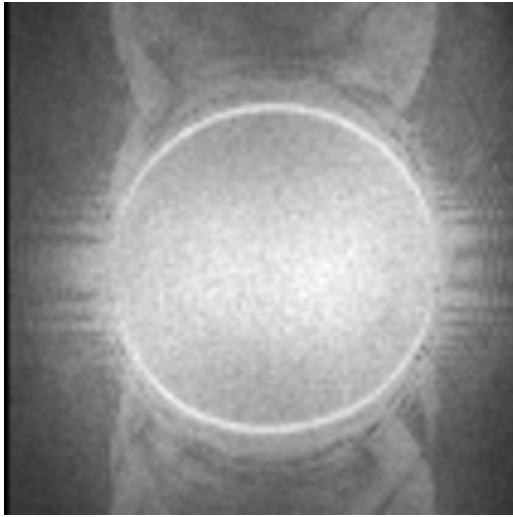

SFNR image



image min: 0, image max: 295.828

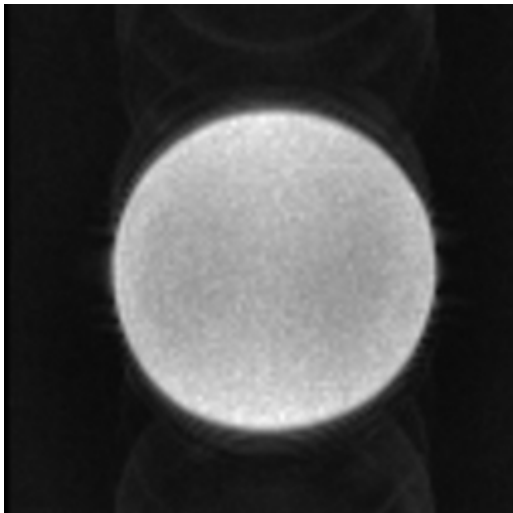

Acquisition parameters

dimensions	106x106x69x100
spacing	2mmx2mmx2mmx1[units?]
gap	0mmx0mmx0mmx0[units?]
scanner	AWP213018
psdname	
examnumber	fe7f7f2a-37d0-4b
studyid	Stability_20250121
seriesnumber	28
runnumber	1-100
scanningsequence	GR/EP

sequencevariant	SK
magneticfield	3
description	ses-20ch_func-bold_acq-cmrrstd_task-tsnrxacpc
scandate	2025-01-21
scantime	11:14:53
tr	2000
te	30
operator	
flipangle	79
prescribedslicespacing	2
frequencydirection	1
acquisitionmatrix	106 106
bandwidth	192.284
receivecoilname	HeadNeck_20_TCS
transmitcoilname	Body
institution	THE UNIVERSITY OF PENNSYLVANIA
examdescription	ACTIVE KIRWAN
scanner	AWP213018
scannermanufacturer	Siemens Healthineers
scannermodelname	MAGNETOM Cima.X
ti	
protocolname	ses-20ch_func-bold_acq-cmrrstd_task-tsnrxacpc
institutionaddress	Grays Ferry Ave. BLDG 250 STE 140 3401,Philadelphia,69 - KEYSTONE,US,19146
institutionaldepartmentname	MindCORE Neuroimaging Suite 140
acquisitiondatetime	20250121111451.210000
volumetricproperties	DISTORTED
scanoptions	PFP/FS/PER
mracquisitiontype	2D
sequencename	epfid2d1_106
angioflag	N
numaverages	1
imagingfrequency	123.253092
imagednucleus	1H
spacingbetweenslices	2
numphaseencodingsteps	106
echotrainlength	80
percentsampling	100
percentphasefieldofview	100

scannerserialnumber	213018
softwareversions	syngo MR XA61
triggertime	
beatrejectionflag	N
cardiacnumberofimages	1
inplane phase encoding direction	COL
variableflipangleflag	N
sar	0.01564417402136
contentqualification	RESEARCH
acquisitionnumber	1
instancenumber	1
numtemporalpositions	100
imagecomments	Not for diagnostic use, Unaliased MB3/PE3/LB
samplesperpixel	1
photometricinterpretation	MONOCHROME2
rows	106
columns	106
bitsallocated	16
bitsstored	16
highbit	15
lossyimagecompression	00
echonumber	0
pixelbandwidth	1814