






Phantom QA results for /fbirn_out/ses64ch_funcbold_acqsiemensstd_task slice 34




old acqsiemensstd tasktsnr 4.xml [percent fluct (trend removed), drift, driftfit]


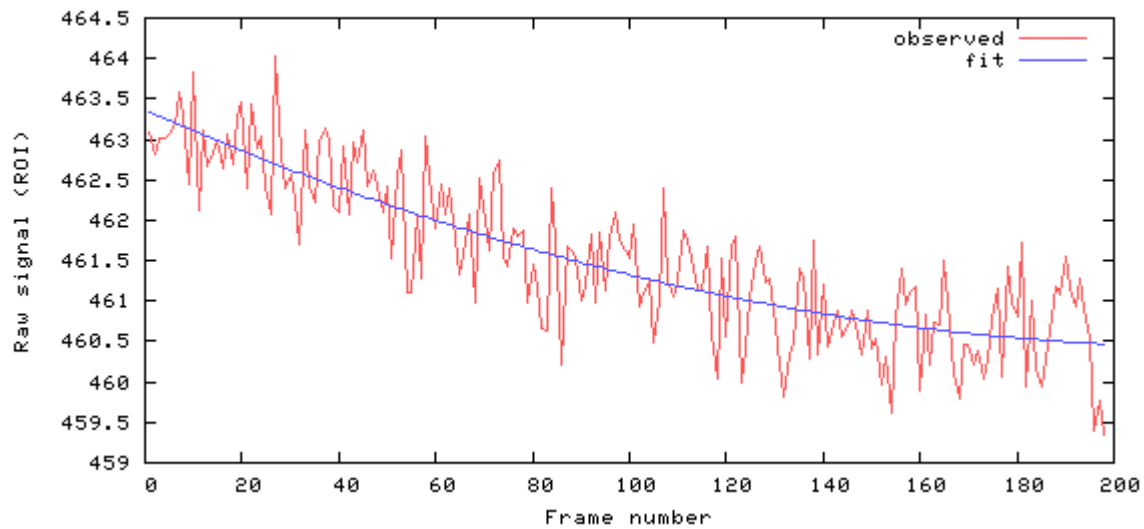


[mean, SNR, SFNR] = [461.5 65.2 62.4]

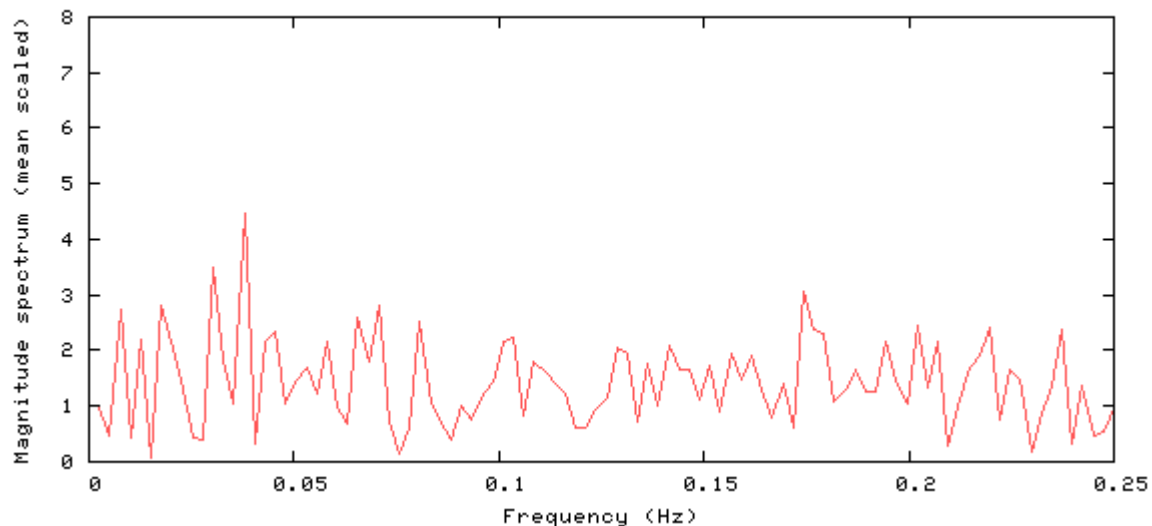

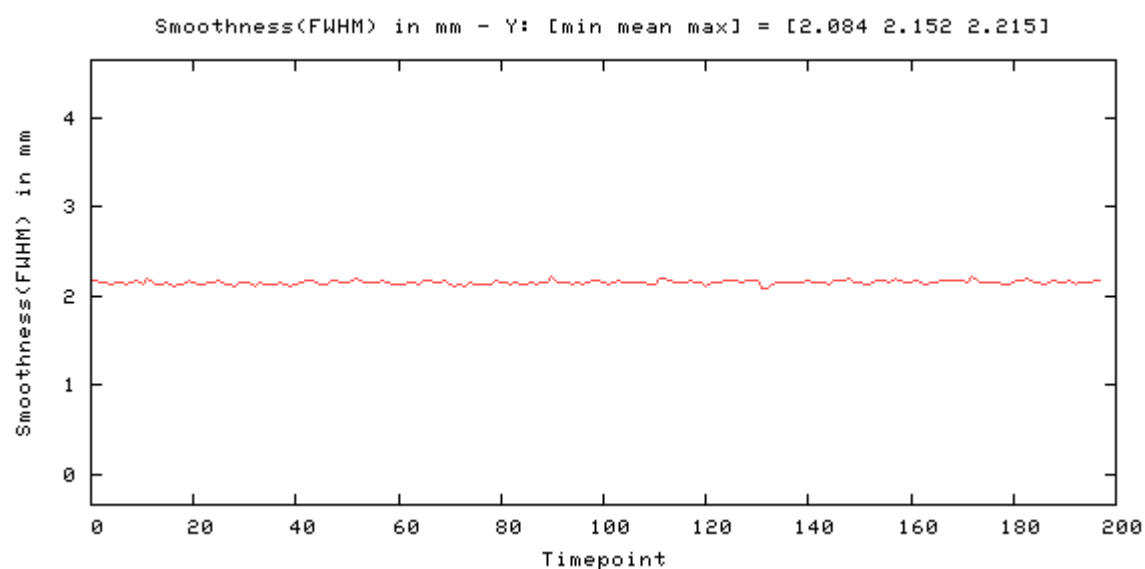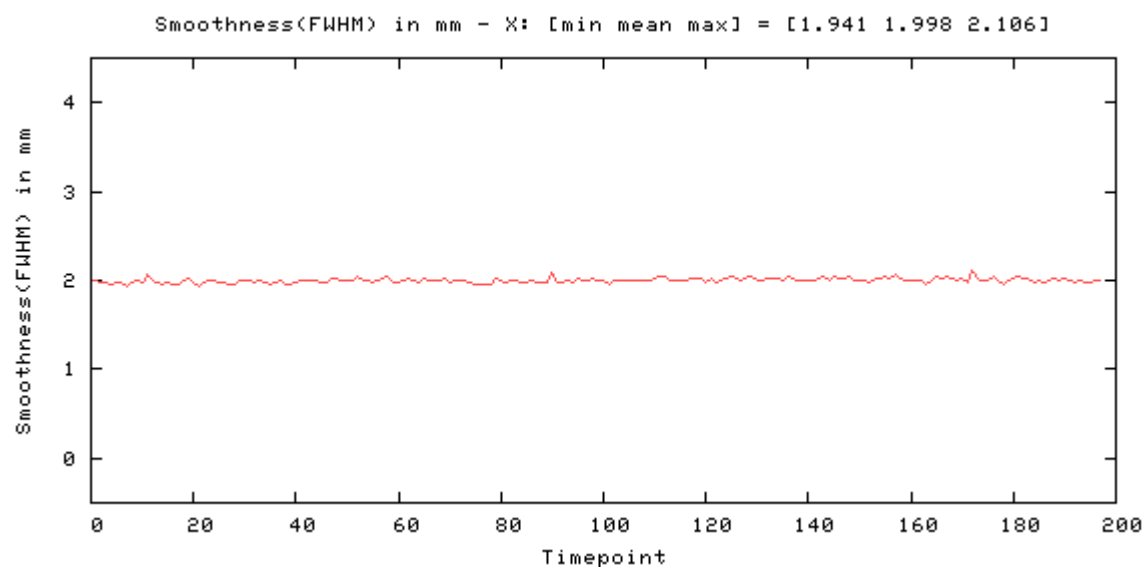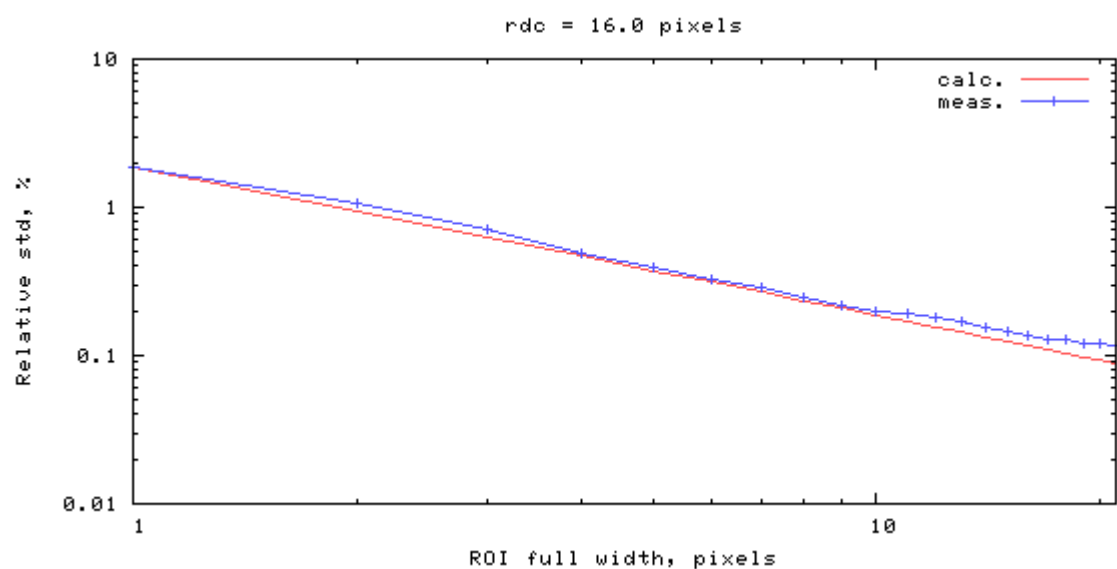

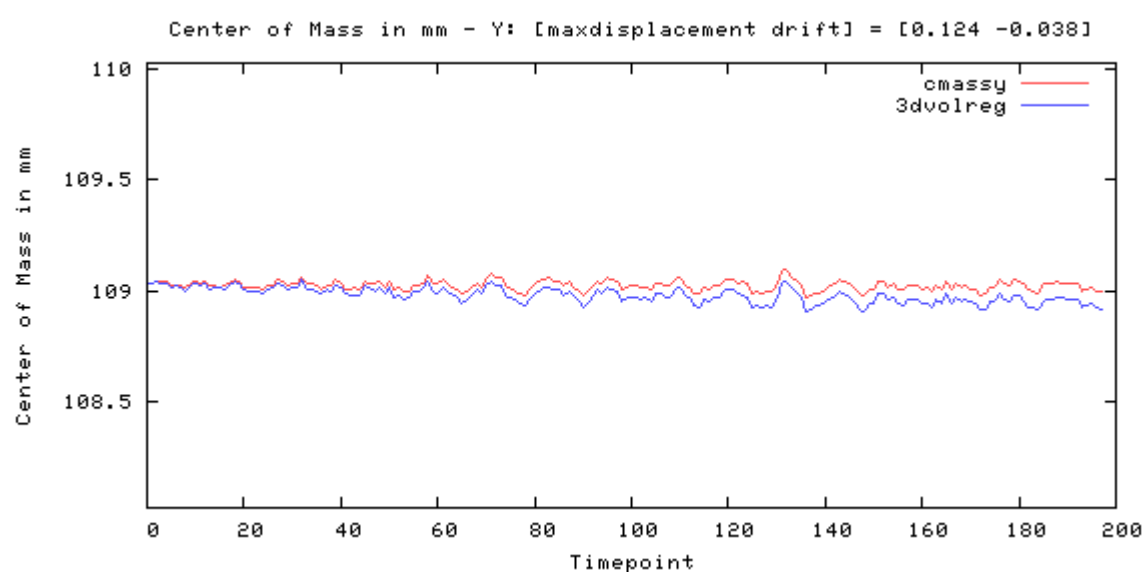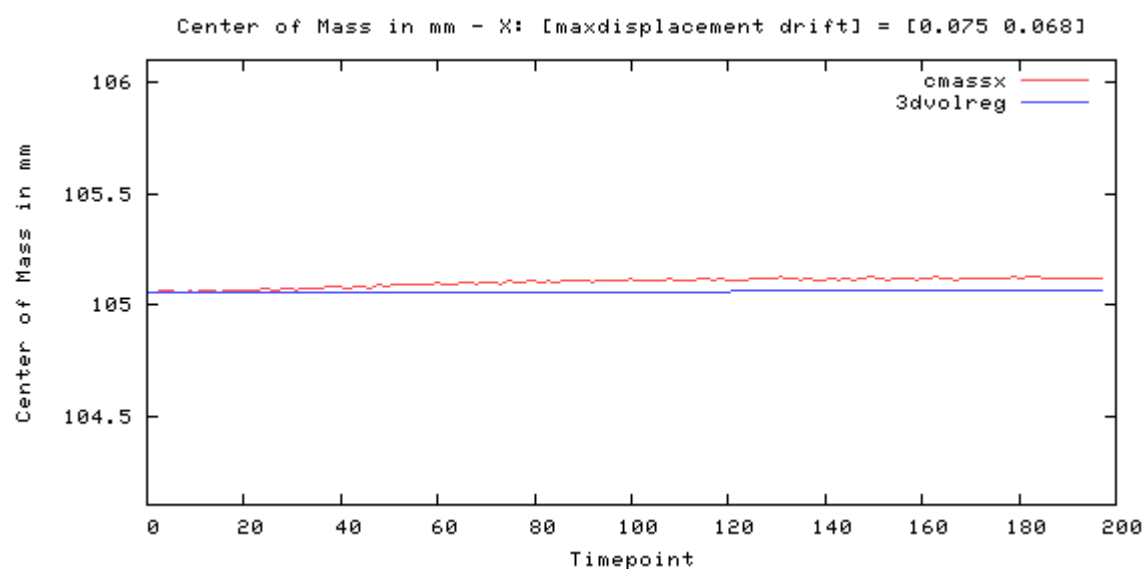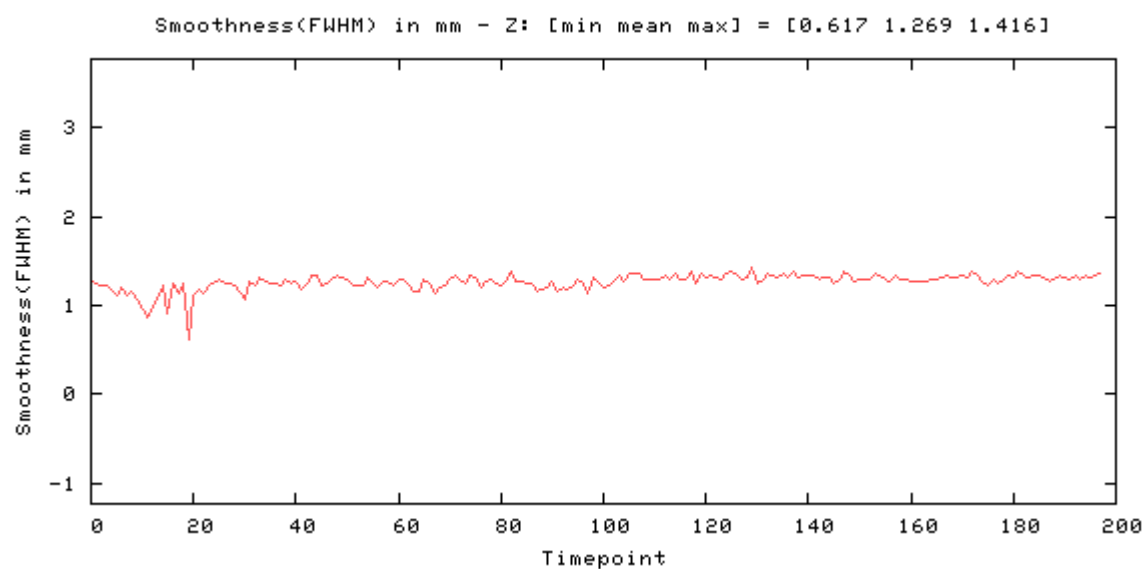


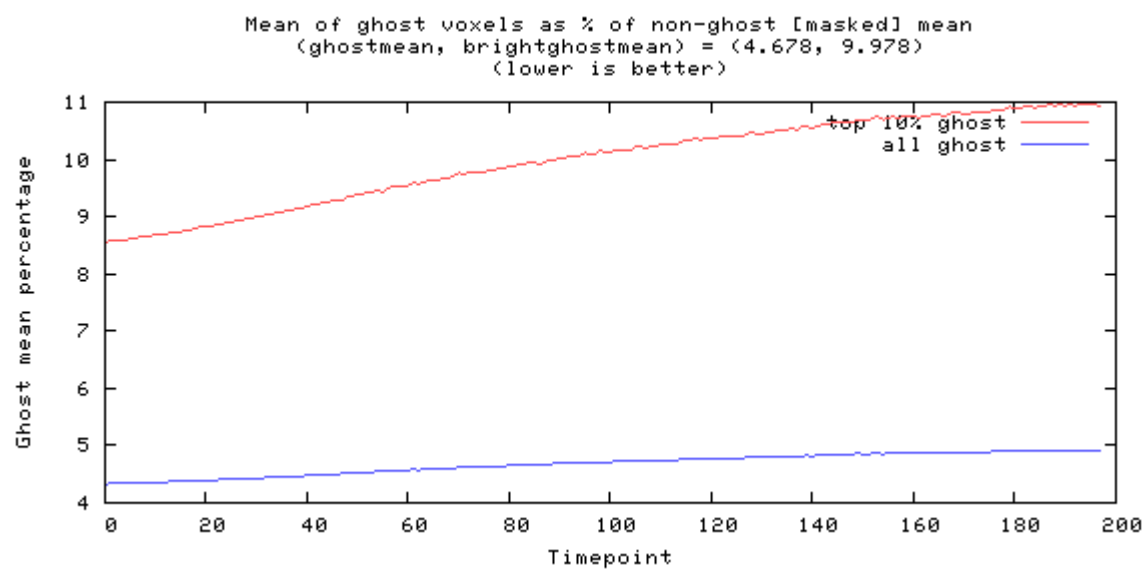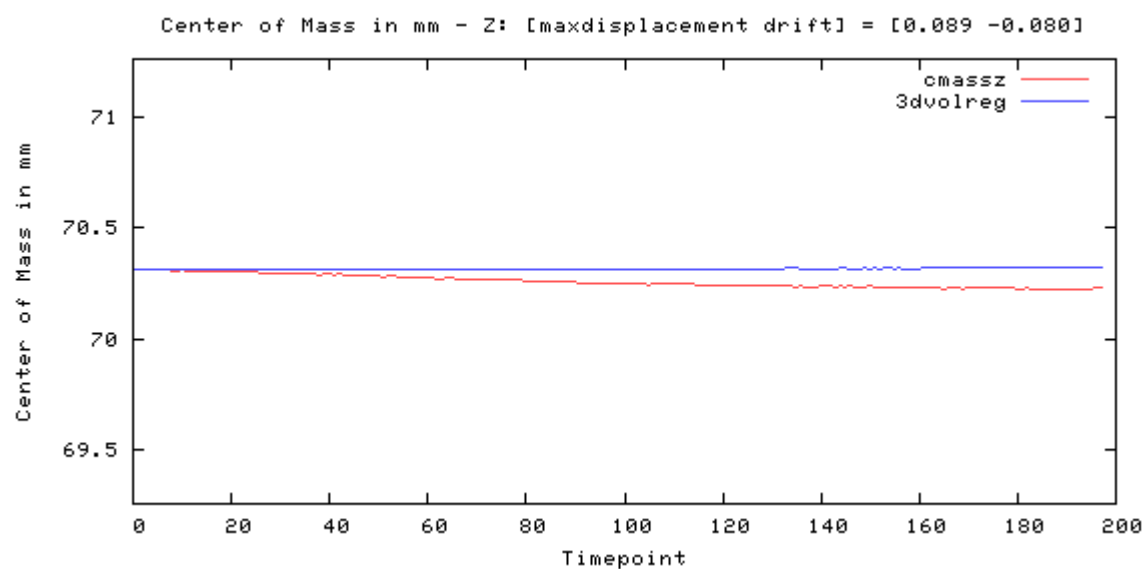

Odd-even difference image




image min: -733, image max: 527

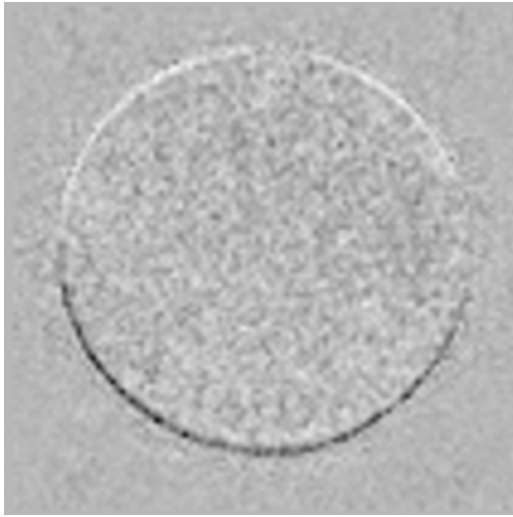

Mean image




image min: 0, image max: 3406.57

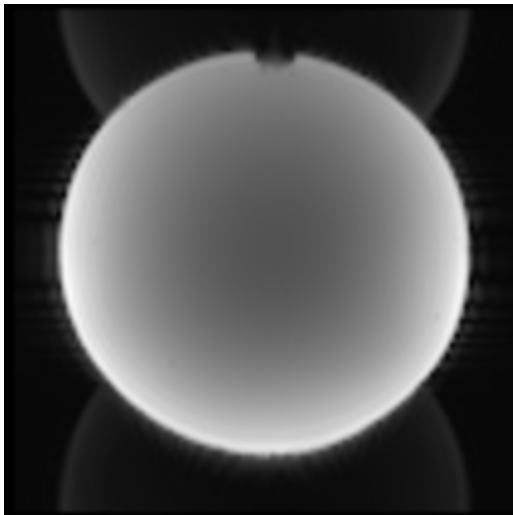

Standard Deviation image




image min: 0, image max: 29.6302

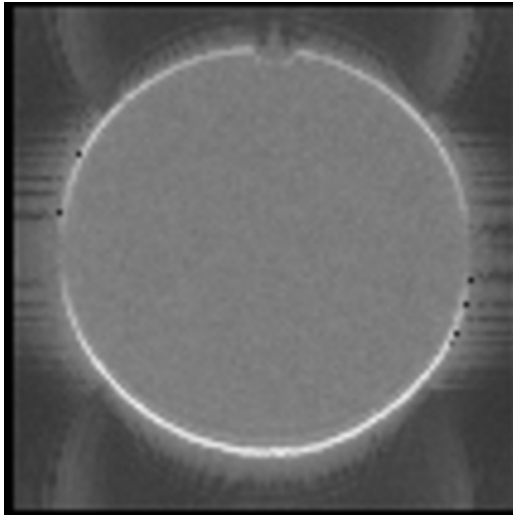

SFNR image



image min: 0, image max: 444.326

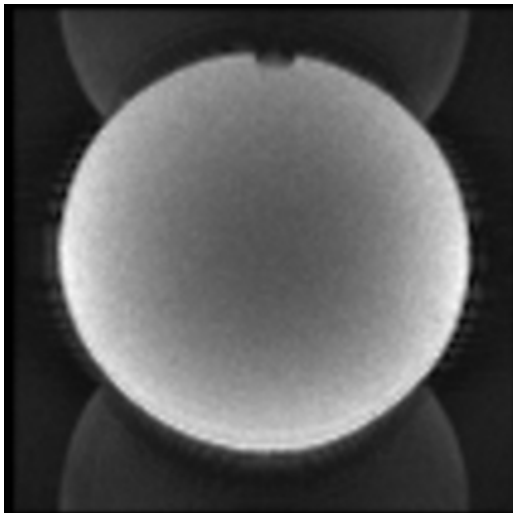

Acquisition parameters

dimensions	106x106x69x200
spacing	2mmx2mmx2mmx1[units?]
gap	0mmx0mmx0mmx0[units?]
scanner	AWP213018
psdname	
examnumber	d9a9a0b2-2cfa-4d
studyid	Stability_20250408
seriesnumber	4
runnumber	1-200
scanningsequence	GR/EP

sequencevariant	SK
magneticfield	3
description	ses-64ch_func-bold_acq-siemensstd_task-tsnr
scandate	2025-04-08
scantime	09:40:37
tr	2000
te	30
operator	
flipangle	79
prescribedslicespacing	2
frequencydirection	1
acquisitionmatrix	106 106
bandwidth	249.948
receivecoilname	HeadNeck_64_CS
transmitcoilname	Body
institution	THE UNIVERSITY OF PENNSYLVANIA
examdescription	ACTIVE KIRWAN
scanner	AWP213018
scannermanufacturer	Siemens Healthineers
scannermodelname	MAGNETOM Cima.X
ti	
protocolname	ses-64ch_func-bold_acq-siemensstd_task-tsnr
institutionaddress	Grays Ferry Ave. BLDG 250 STE 140 3401,Philadelphia,69 - KEYSTONE,US,19146
institutionaldepartmentname	MindCORE Neuroimaging Suite 140
acquisitiondatetime	20250408094034.510000
volumetricproperties	VOLUME
scanoptions	PFP/FS/PER
mracquisitiontype	2D
sequencename	*epfid2d1_106
angioflag	N
numaverages	1
imagingfrequency	123.253282
imagednucleus	1H
spacingbetweenslices	2
numphaseencodingsteps	106
echotrainlength	93
percentsampling	100
percentphasefieldofview	100

scannerserialnumber	213018
softwareversions	syngo MR XA61
triggertime	
beatrejectionflag	N
cardiacnumberofimages	1
inplane phase encoding direction	COL
variableflipangleflag	N
sar	0.11439636473538
contentqualification	PRODUCT
acquisitionnumber	1
instancenumber	1
numtemporalpositions	200
samplesperpixel	1
photometricinterpretation	MONOCHROME2
rows	106
columns	106
bitsallocated	16
bitsstored	12
highbit	11
lossyimagecompression	00
echonumber	0
pixelbandwidth	2358