



Phantom QA results for / fbirn_out/ses-64ch_func-bold_acq-cmrrstd_task-warmup.xml, slice 34

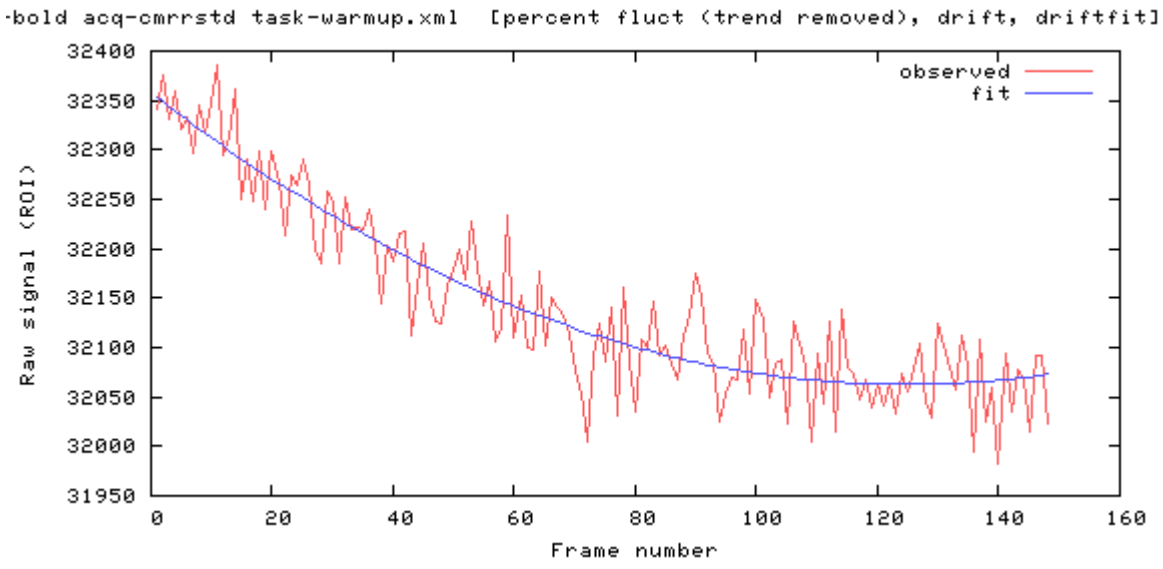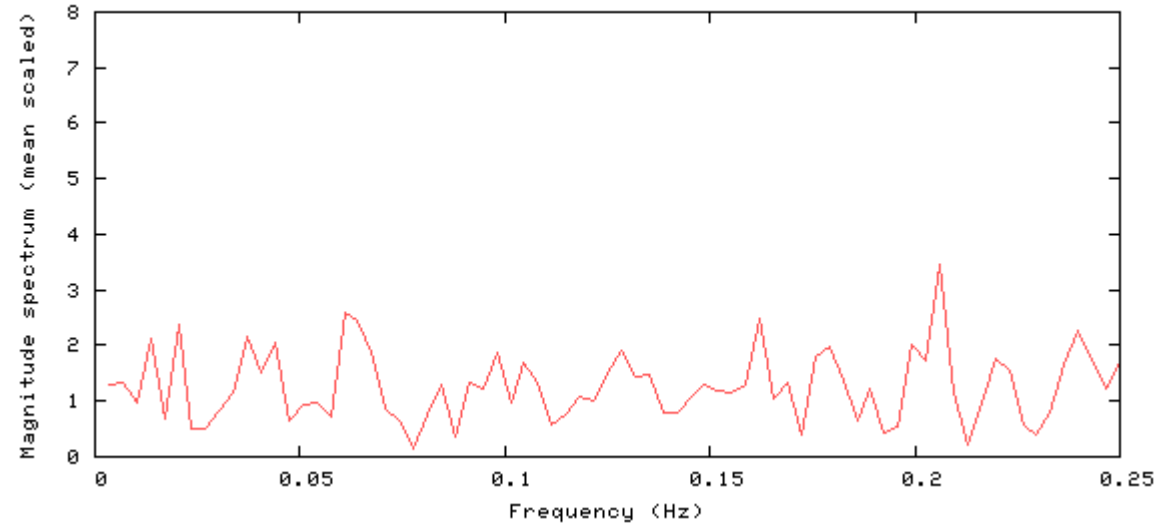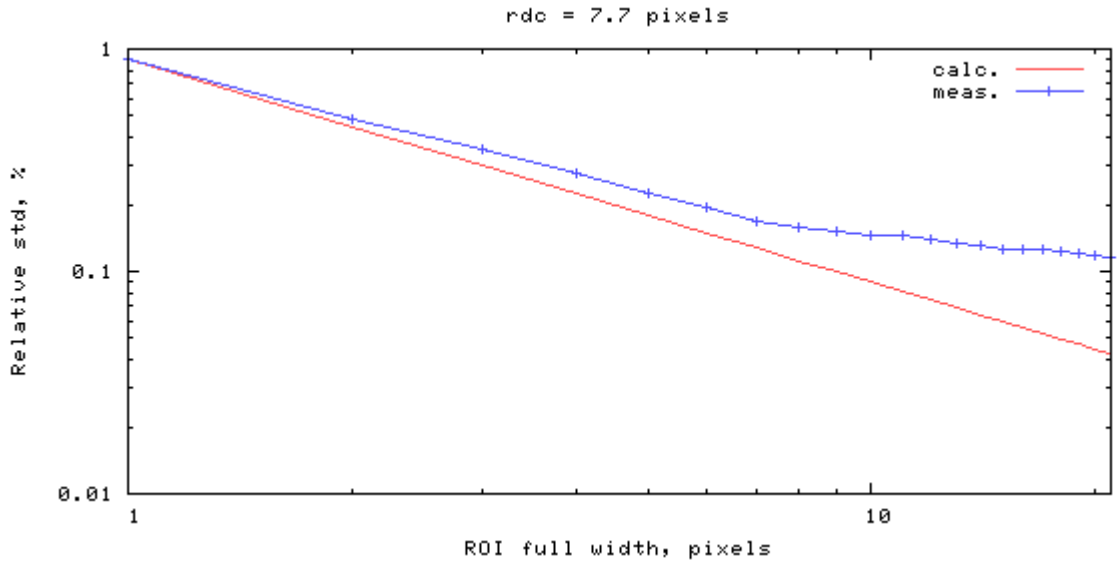



[mean, SNR, SFNR] = [32145.0 121.4 125.2]

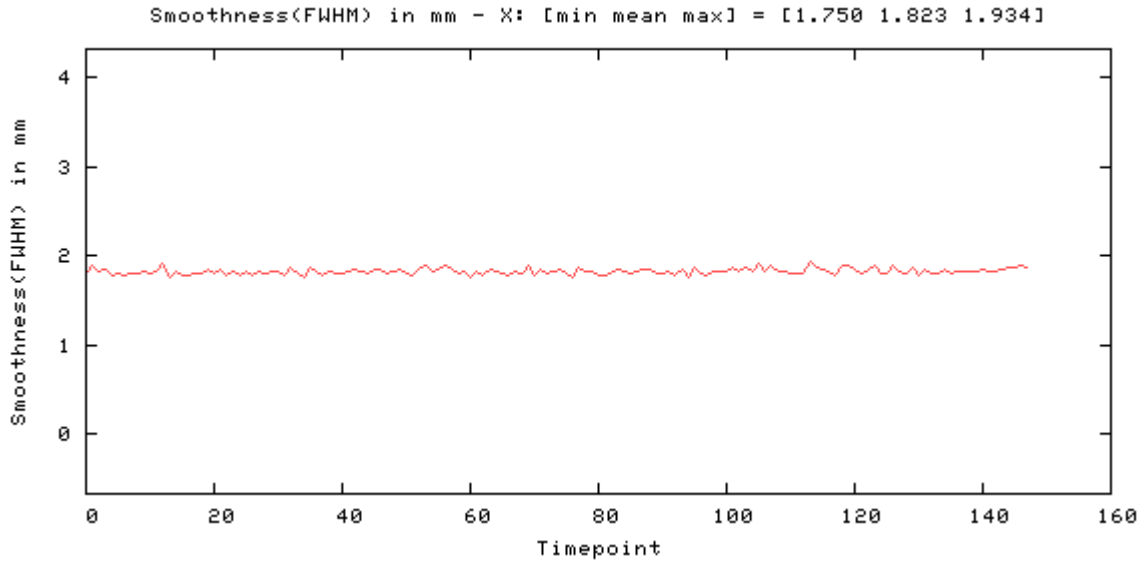




rdc = 7.7 pixels
calc.
meas.
Relative std, %
1
0.1
0.01
1
10
ROI full width, pixels



Smoothness(FWHM) in mm - X: [min mean max] = [1.750 1.823 1.934]
Smoothness(FWHM) in mm
0
1
2
3
4
0
20
40
60
80
100
120
140
160
Timepoint

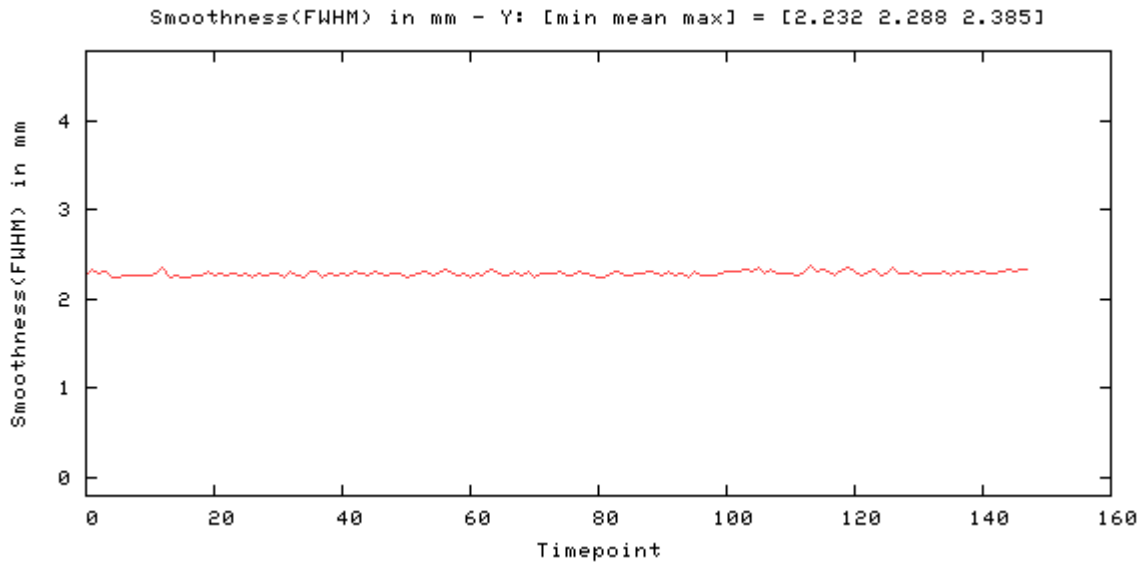

Smoothness(FWHM) in mm - Y: [min mean max] = [2.232 2.288 2.385]
Smoothness(FWHM) in mm
0
1
2
3
4
0
20
40
60
80
100
120
140
160
Timepoint

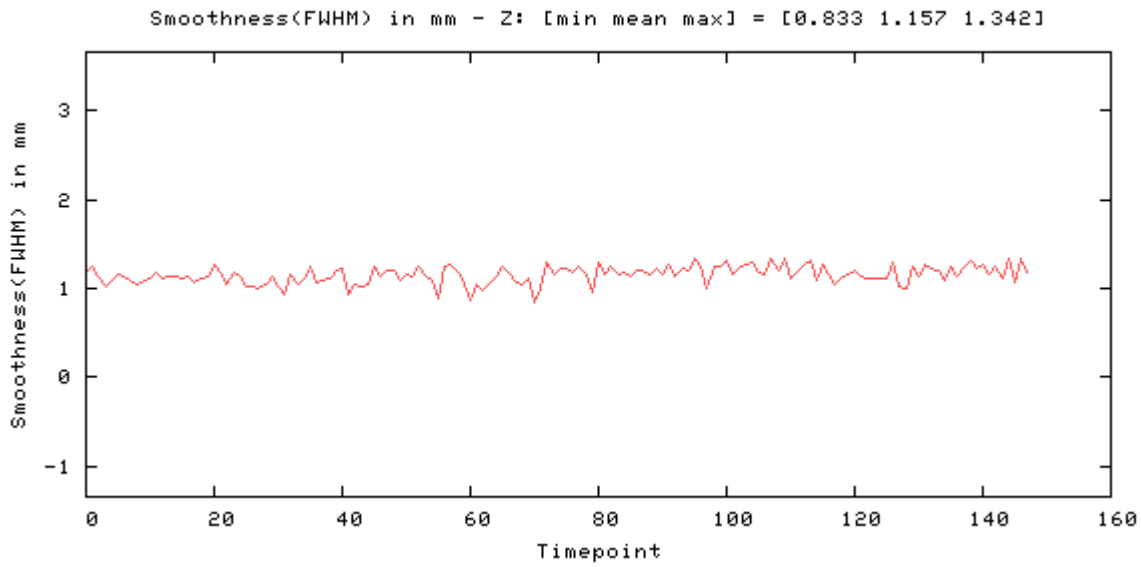
Smoothness(FWHM) in mm - Z: [min mean max] = [0.833 1.157 1.342]
Smoothness(FWHM) in mm
Timepoint

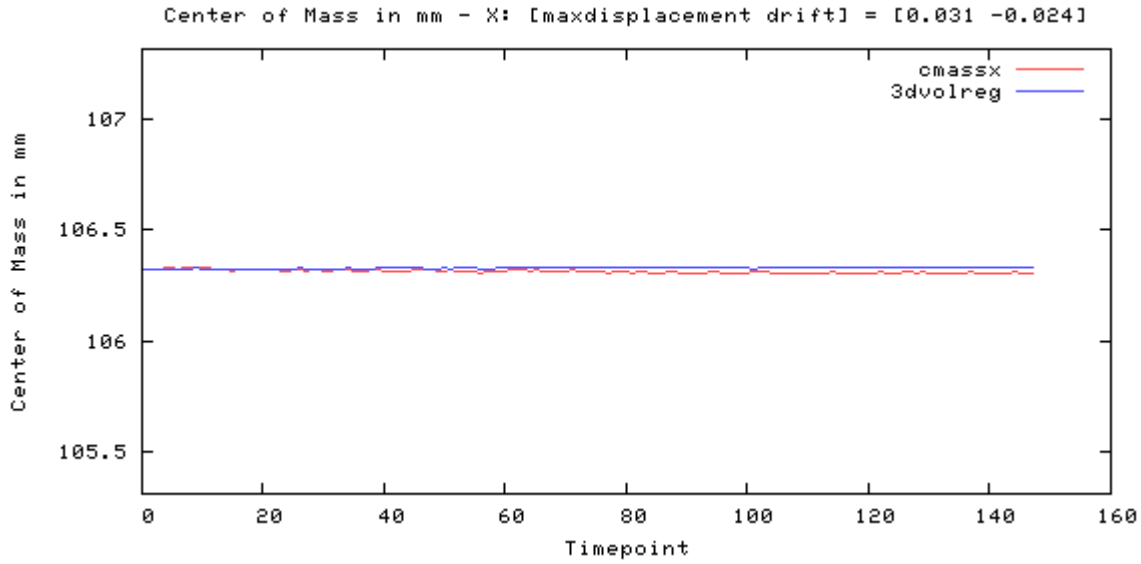
Center of Mass in mm - X: [maxdisplacement drift] = [0.031 -0.024]
cmassx
3dvolreg
Center of Mass in mm
Timepoint

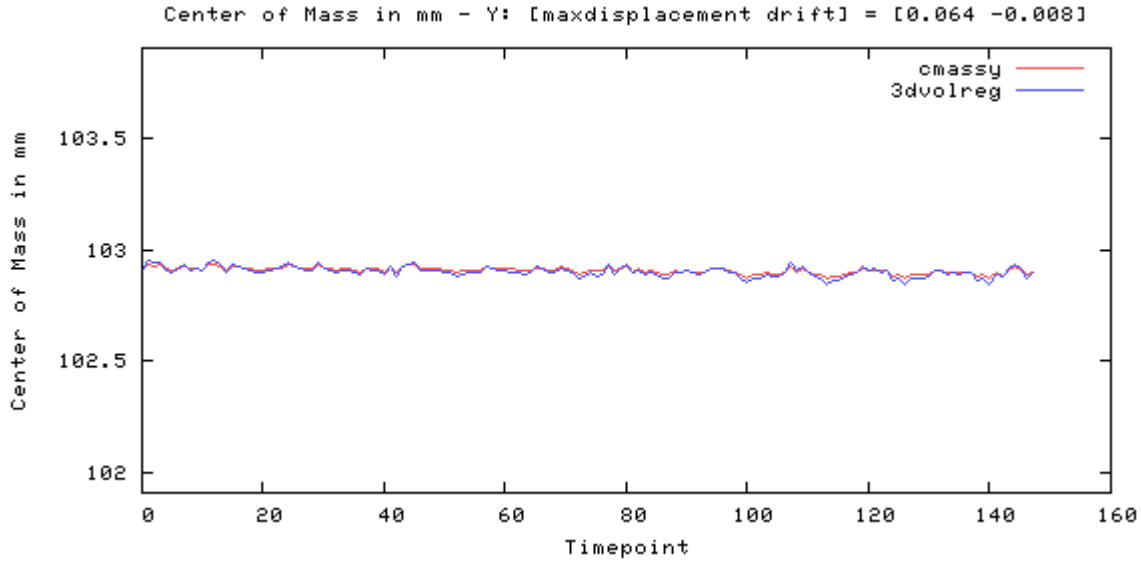
Center of Mass in mm - Y: [maxdisplacement drift] = [0.064 -0.008]
cmassy
3dvolreg
Center of Mass in mm
Timepoint

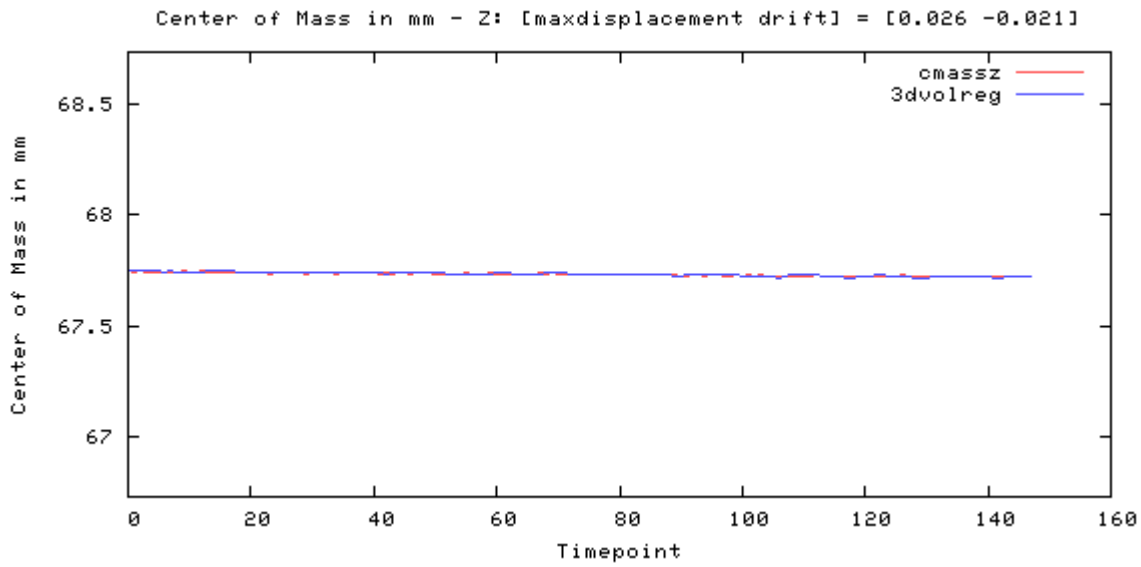


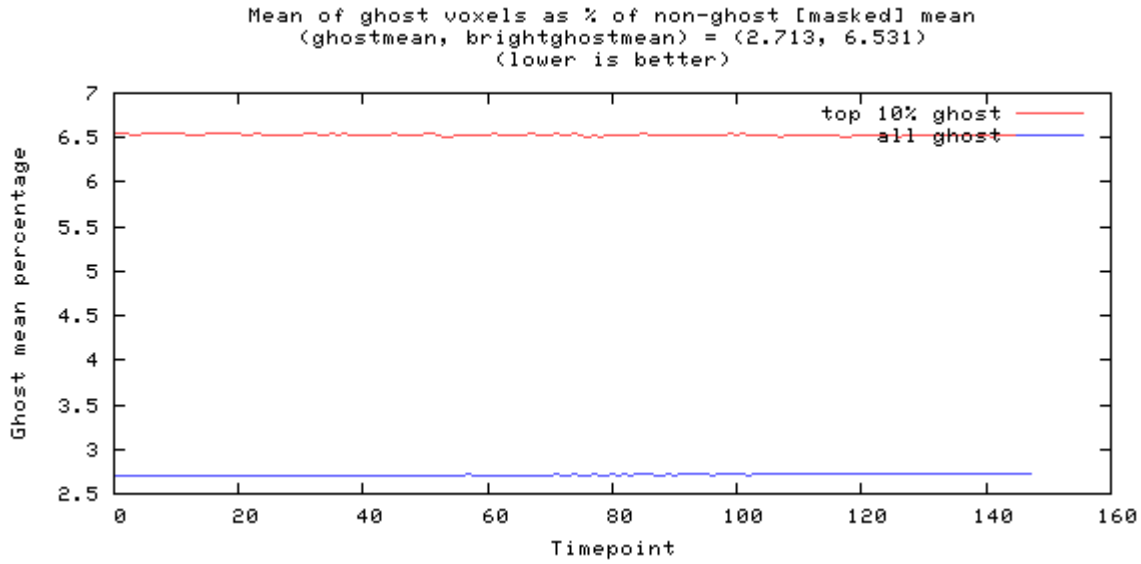

Odd-even difference image




image min: -10196, image max: 9747

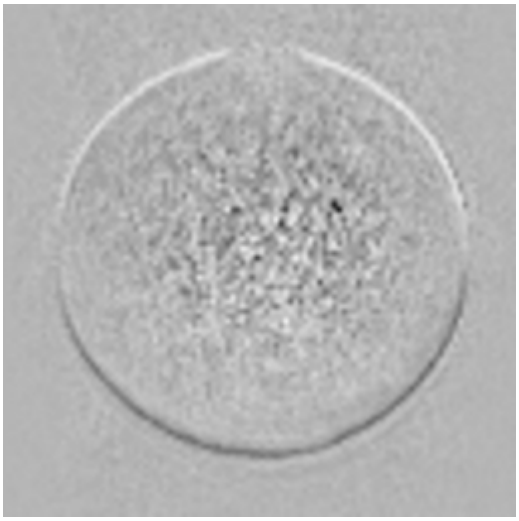

Mean image




image min: 0, image max: 44292.7

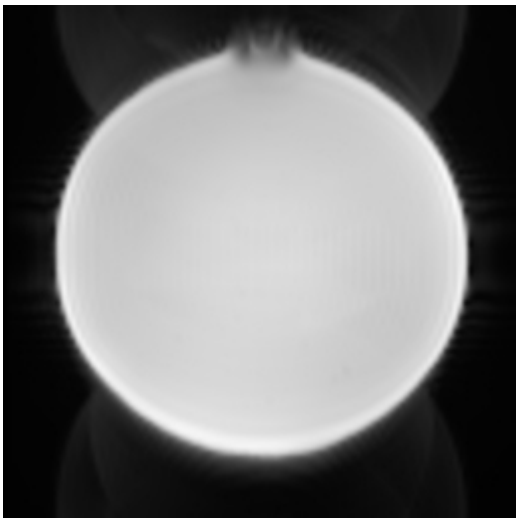

Standard Deviation image




image min: 0, image max: 324.443

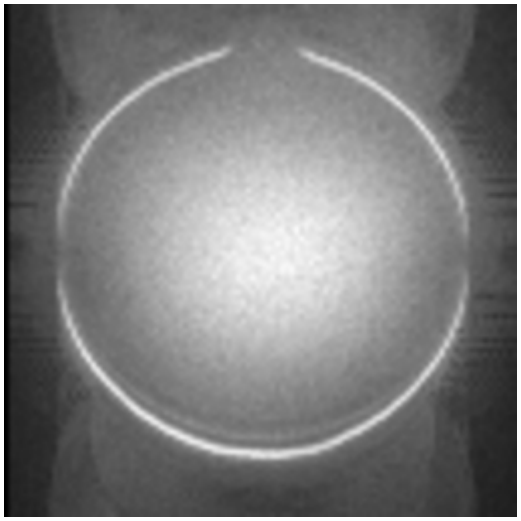

SFNR image



image min: 0, image max: 663.418

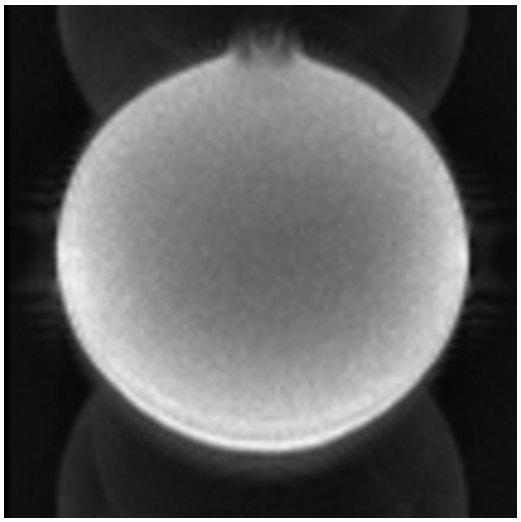

Acquisition parameters

dimensions	106x106x69x150
spacing	2mmx2mmx2mmx2000ms
gap	0mmx0mmx0mmx0ms
scanner	AWP213018
psdname	
examnumber	31ad03b6-d380-44
studyid	Stability_20261028
seriesnumber	2
runnumber	1
magneticfield	3

description	ses-64ch_func-bold_acq-cmrrstd_task-warmup
scandate	2026-10-28
scantime	10:25:04
tr	2000
te	30
operator	
flipangle	79
prescribedslicespacing	2
frequencydirection	1
receivecoilname	HeadNeck_64_CS
transmitcoilname	Body
institution	THE UNIVERSITY OF PENNSYLVANIA
examdescription	ACTIVE KIRWAN
scanner	AWP213018
scannermanufacturer	Siemens Healthineers
scannermodelname	MAGNETOM Cima.X
protocolname	ses-64ch_func-bold_acq-cmrrstd_task-warmup
institutionaddress	Grays Ferry Ave. BLDG 250 STE 140 3401,Philadelphia,69 - KEYSTONE,US,19146
institutionaldepartmentname	MindCORE Neuroimaging Suite 140
acquisitiondatetime	20261028102502.622500
frametype	ORIGINAL
pixelpresentation	MONOCHROME
volumetricproperties	DISTORTED
volumebasedcalculationtechnique	NONE
complexitimagecomponent	MAGNITUDE
acquisitioncontrast	UNKNOWN
mracquisitiontype	2D
numaverages	1
spacingbetweenslices	2
echotrainlength	80
percentsampling	100
percentphasefieldofview	100
scannerserialnumber	213018
softwareversions	syngo MR XA61
inplanephaseencodingdirection	COLUMN
variableflipangleflag	N
contentqualification	RESEARCH
acquisitionduration	317.89499999999998

resonantnucleus	1H
applicablesafetystandardagency	IEC
acquisitionnumber	1
instancenumber	1
numtemporalpositions	150
imagecomments	Not for diagnostic use, Unaliased MB3/ PE3/LB
samplesperpixel	1
photometricinterpretation	MONOCHROME2
numberofframes	69
rows	106
columns	106
bitsallocated	16
bitsstored	16
highbit	15
lossyimagecompression	00