




Phantom QA results for / fbirn_out/ses-32ch_func-bold_acq-cmrrstd_task-tsnr.xml, slice 34

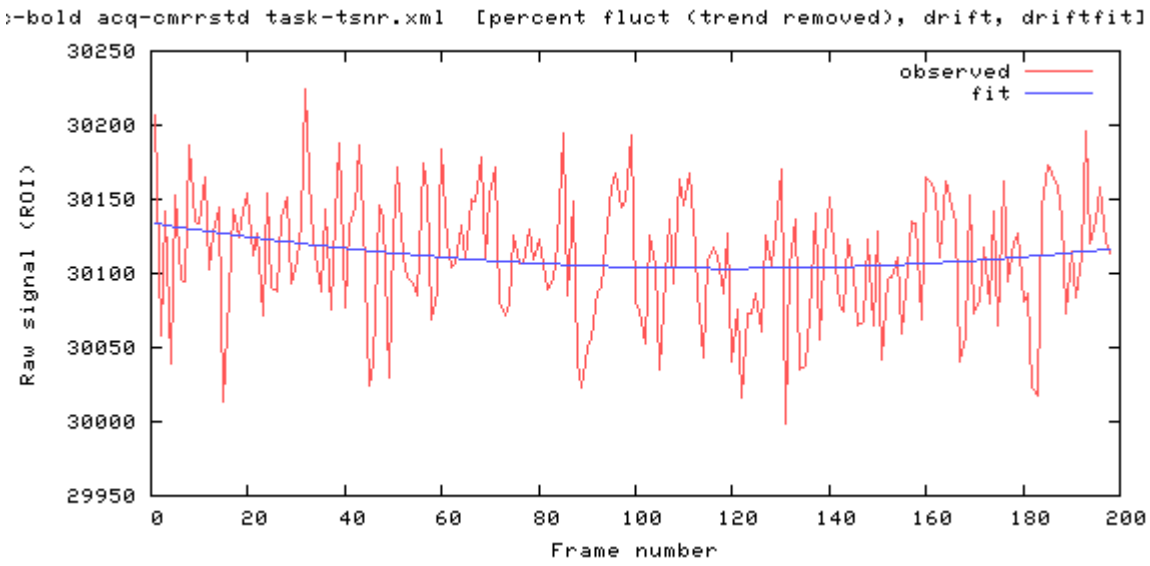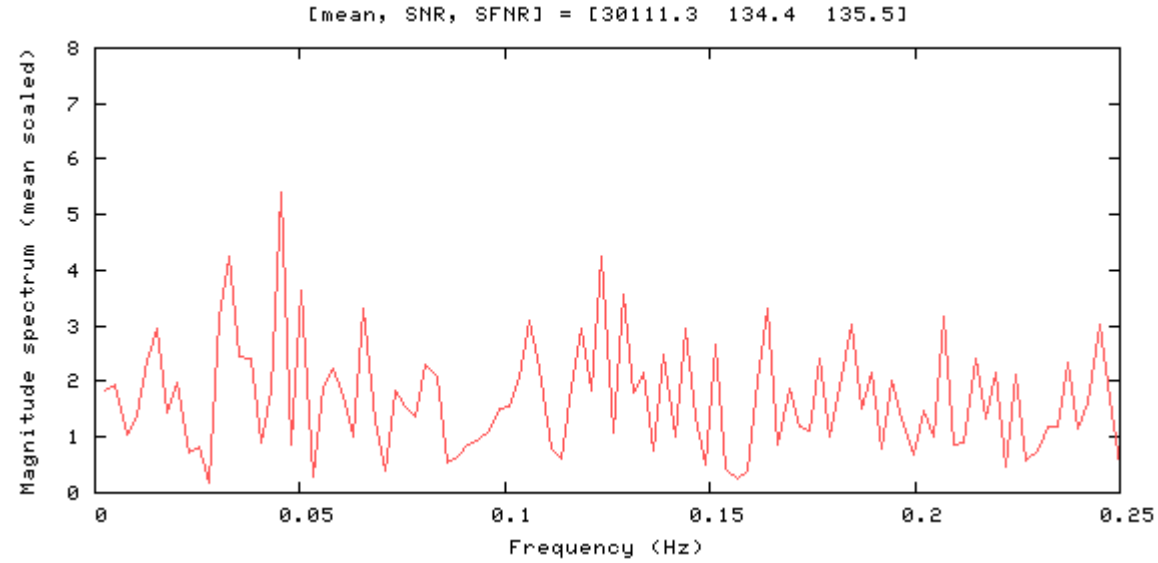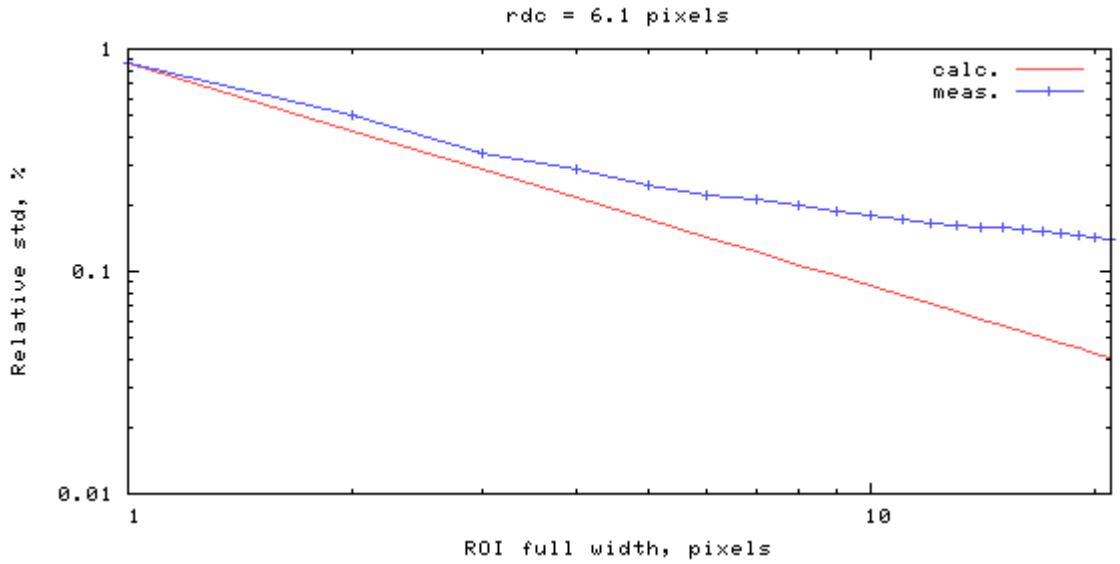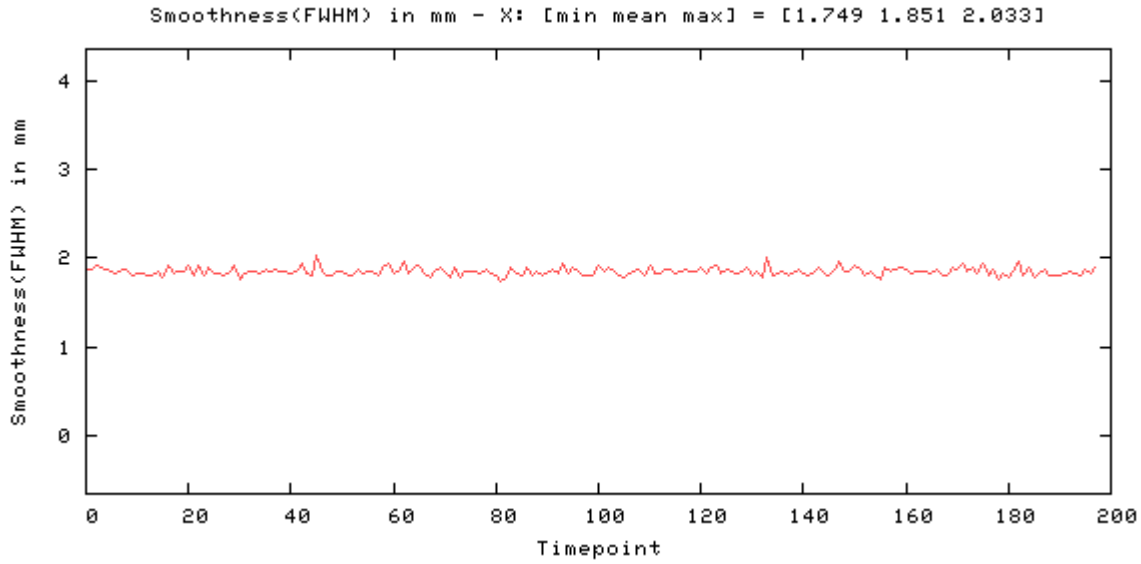


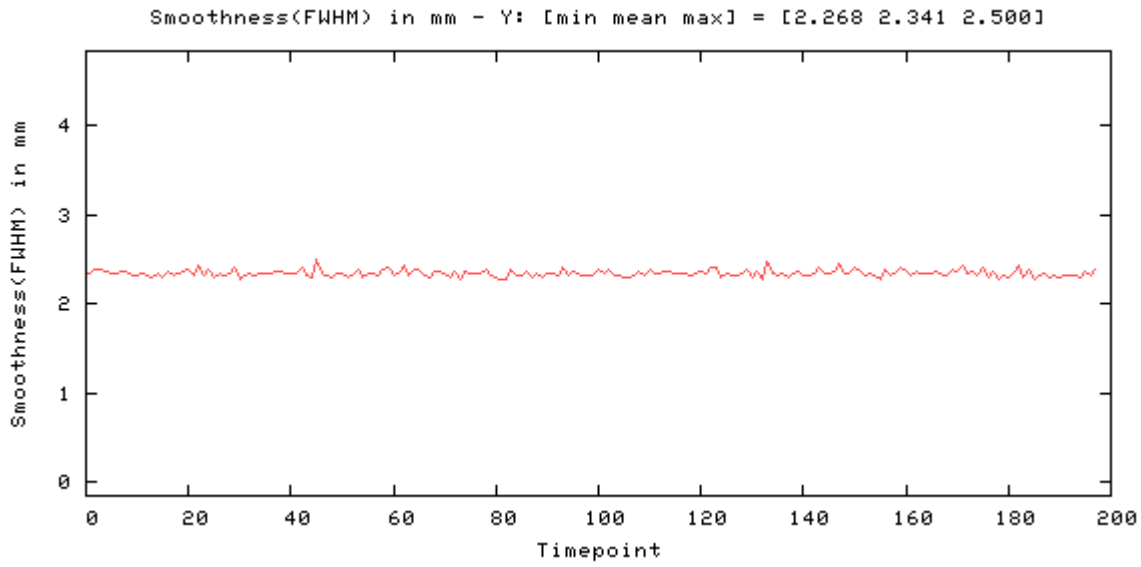




rdc = 6.1 pixels
calc.
meas.
Relative std, %
1
0.1
0.01
1
10
ROI full width, pixels



Smoothness(FWHM) in mm - X: [min mean max] = [1.749 1.851 2.033]
Smoothness(FWHM) in mm
0
1
2
3
4
0
20
40
60
80
100
120
140
160
180
200
Timepoint



Smoothness(FWHM) in mm - Y: [min mean max] = [2.268 2.341 2.500]
Smoothness(FWHM) in mm
0
1
2
3
4
0
20
40
60
80
100
120
140
160
180
200
Timepoint

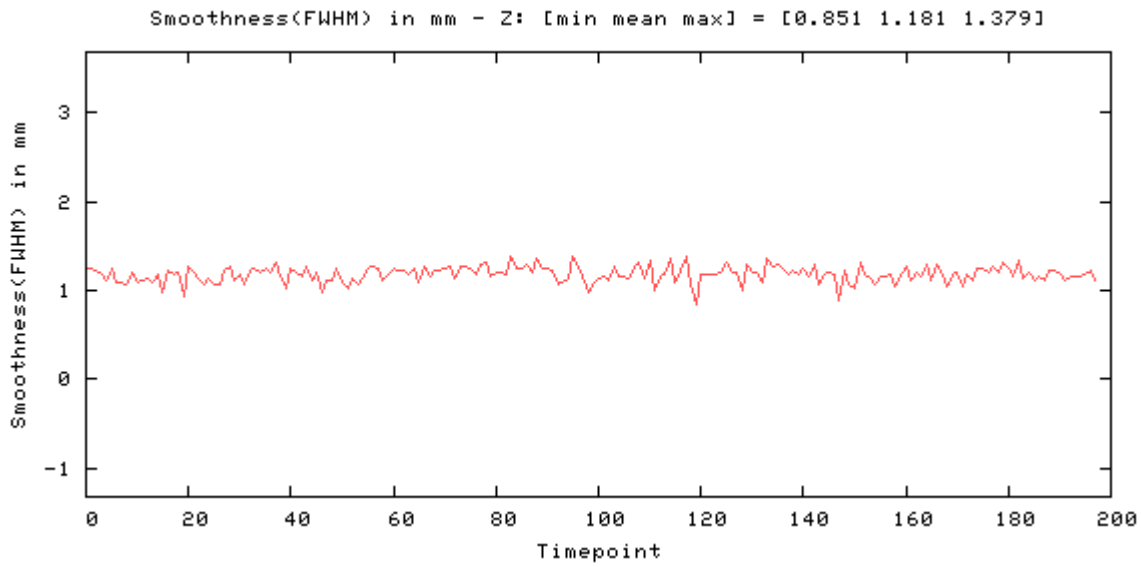
Smoothness(FWHM) in mm - Z: [min mean max] = [0.851 1.181 1.379]
Smoothness(FWHM) in mm
3
2
1
0
-1
0
20
40
60
80
100
120
140
160
180
200
Timepoint

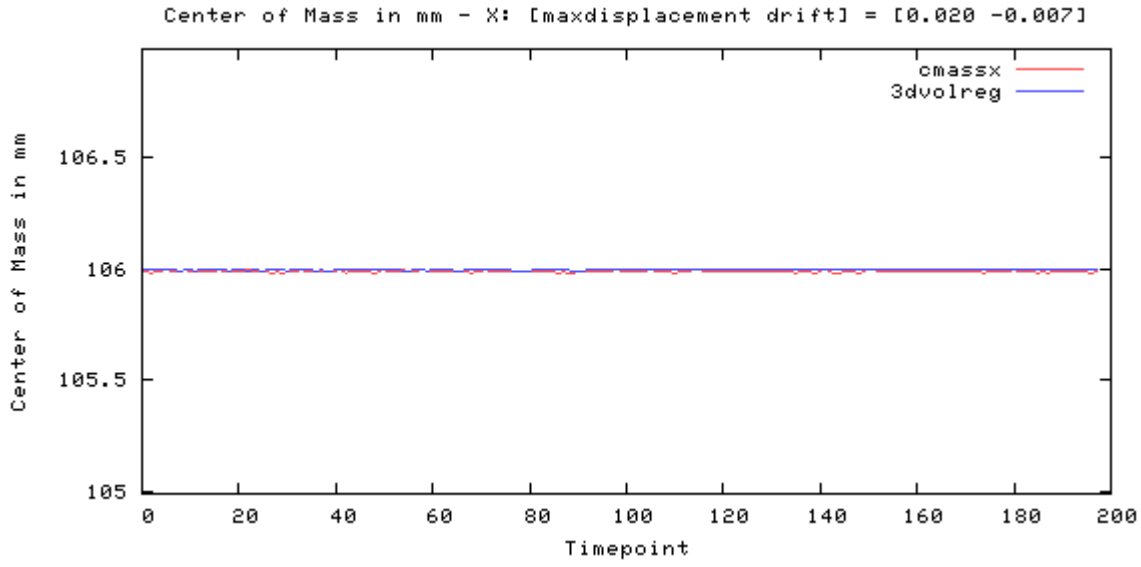
Center of Mass in mm - X: [maxdisplacement drift] = [0.020 -0.007]
cmassx
3dvolreg
Center of Mass in mm
106.5
106
105.5
105
0
20
40
60
80
100
120
140
160
180
200
Timepoint

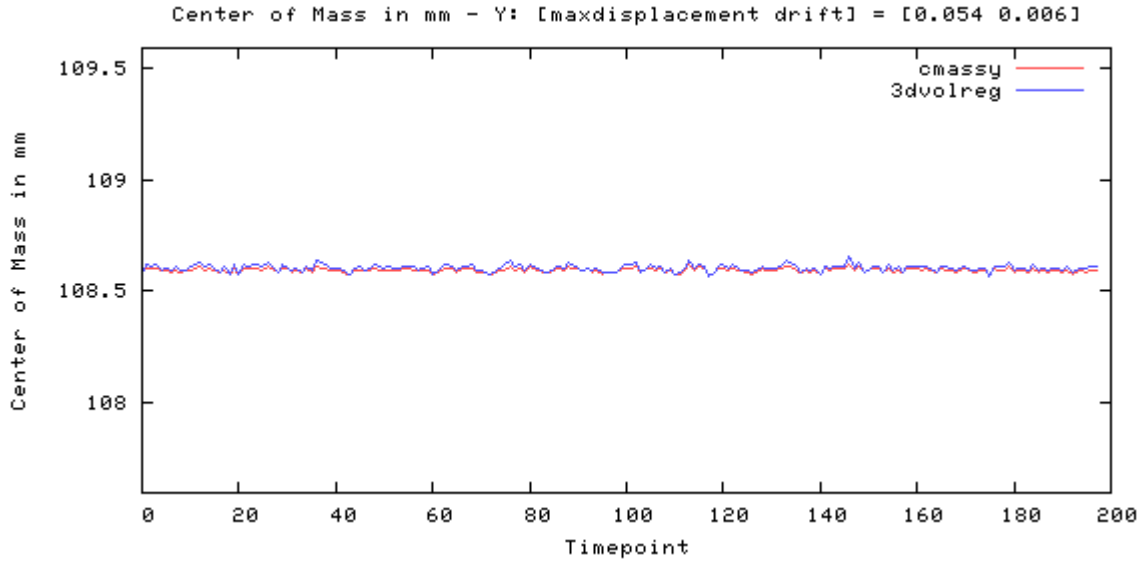
Center of Mass in mm - Y: [maxdisplacement drift] = [0.054 0.006]
cmassy
3dvolreg
Center of Mass in mm
109.5
109
108.5
108
0
20
40
60
80
100
120
140
160
180
200
Timepoint

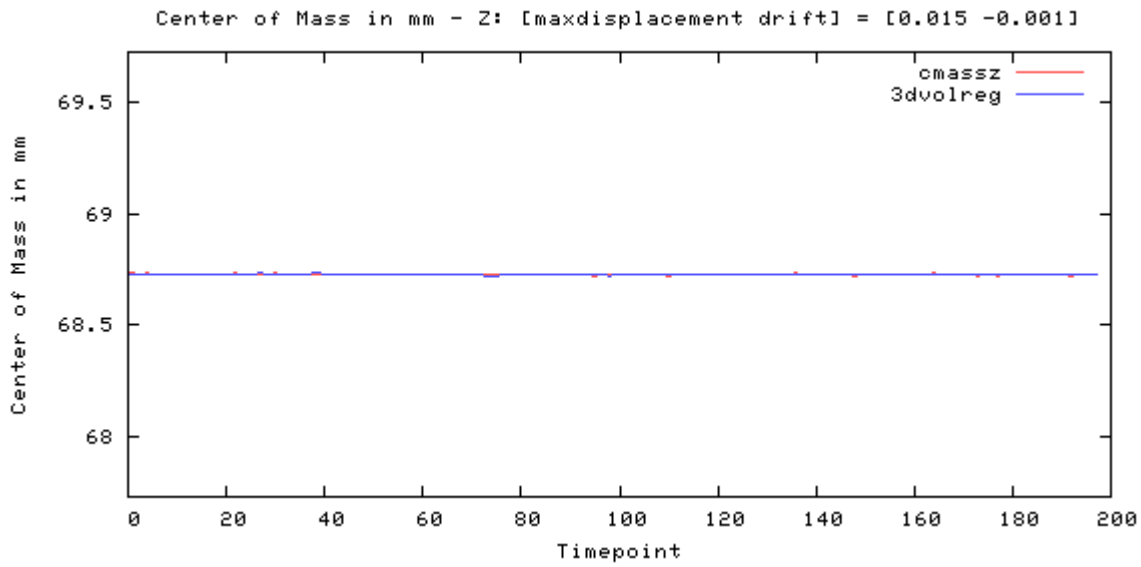


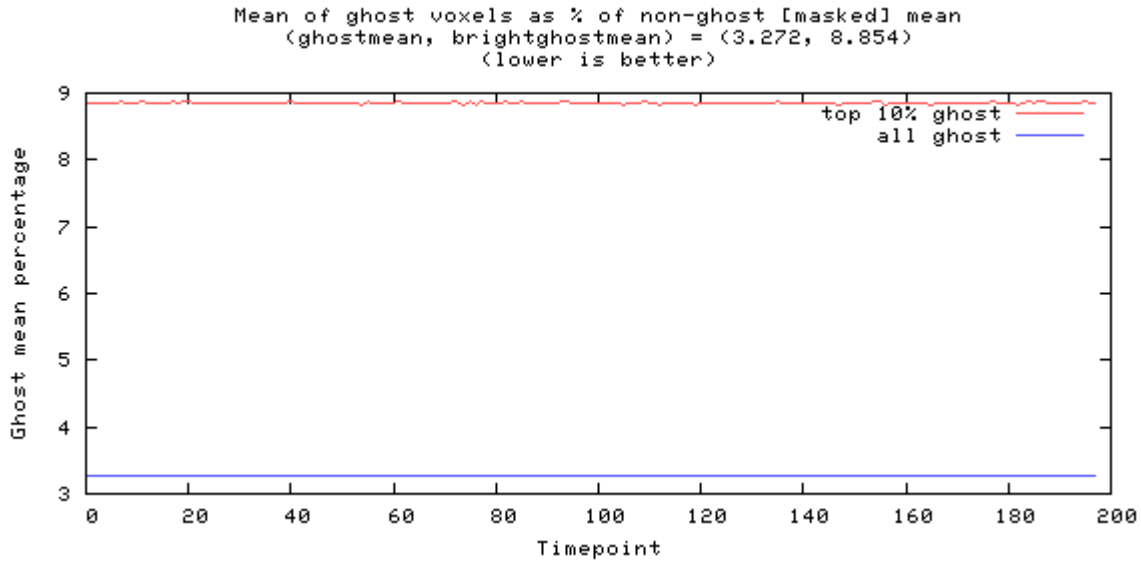

Odd-even difference image




image min: -11124, image max: 9340

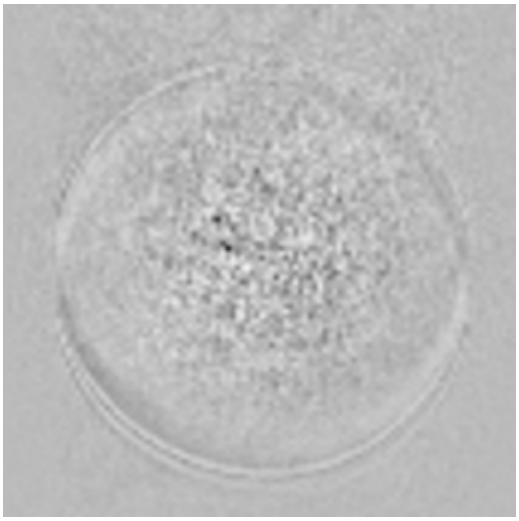

Mean image




image min: 0, image max: 42883.2

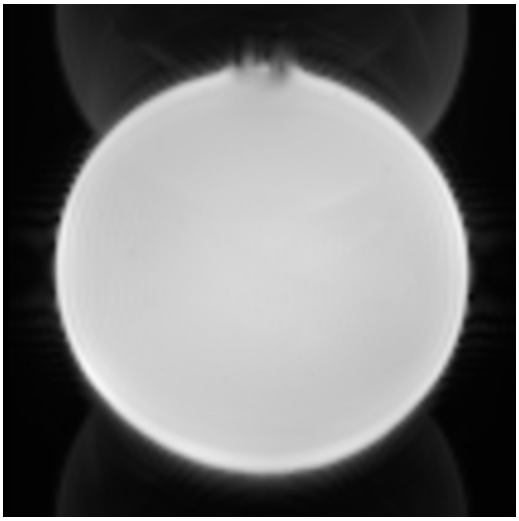

Standard Deviation image




image min: 0, image max: 284.389

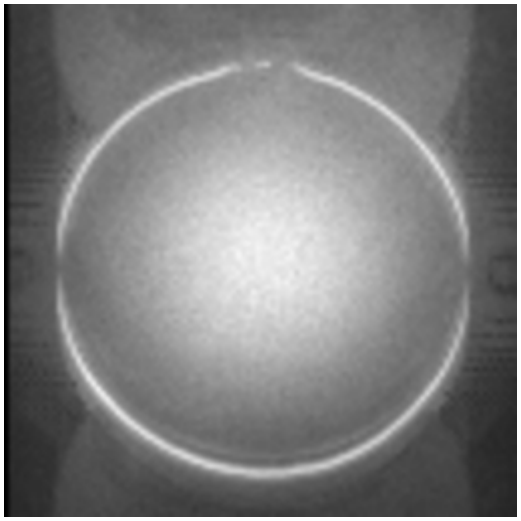

SFNR image

0 711.533

image min: 0, image max: 740.435

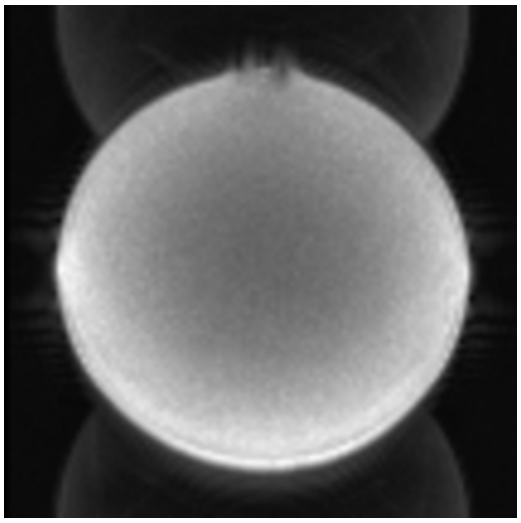

Acquisition parameters

dimensions	106x106x69x200
spacing	2mmx2mmx2mmx2000ms
gap	0mmx0mmx0mmx0ms
scanner	AWP213018
psdname	
examnumber	a0f8a673-da21-44
studyid	Stability_20261019
seriesnumber	23
runnumber	1
magneticfield	3

description	ses-32ch_func-bold_acq-cmrrstd_task-tsnr
scandate	2026-10-19
scantime	12:18:57
tr	2000
te	30
operator	
flipangle	79
prescribedslicespacing	2
frequencydirection	1
receivecoilname	Head_32
transmitcoilname	Body
institution	THE UNIVERSITY OF PENNSYLVANIA
examdescription	ACTIVE KIRWAN
scanner	AWP213018
scannermanufacturer	Siemens Healthineers
scannermodelname	MAGNETOM Cima.X
protocolname	ses-32ch_func-bold_acq-cmrrstd_task-tsnr
institutionaddress	Grays Ferry Ave. BLDG 250 STE 140 3401,Philadelphia,69 - KEYSTONE,US,19146
institutionaldepartmentname	MindCORE Neuroimaging Suite 140
acquisitiondatetime	20261019121855.605000
frametype	ORIGINAL
pixelpresentation	MONOCHROME
volumetricproperties	DISTORTED
volumebasedcalculationtechnique	NONE
complexitimagecomponent	MAGNITUDE
acquisitioncontrast	UNKNOWN
mracquisitiontype	2D
numaverages	1
spacingbetweenslices	2
echotrainlength	80
percentsampling	100
percentphasefieldofview	100
scannerserialnumber	213018
softwareversions	syngo MR XA61
inplanephaseencodingdirection	COLUMN
variableflipangleflag	N
contentqualification	RESEARCH
acquisitionduration	417.89499999999998
resonantnucleus	1H

applicablesafetystandardagency	IEC
acquisitionnumber	1
instancenumber	1
numtemporalpositions	200
imagecomments	Not for diagnostic use, Unaliased MB3/ PE3/LB
samplesperpixel	1
photometricinterpretation	MONOCHROME2
numberofframes	69
rows	106
columns	106
bitsallocated	16
bitsstored	16
highbit	15
lossyimagecompression	00