



Phantom QA results for / fbirn_out/ses-32ch_func-bold_acq-siemensbasic_task-tsnr.xml, slice 14

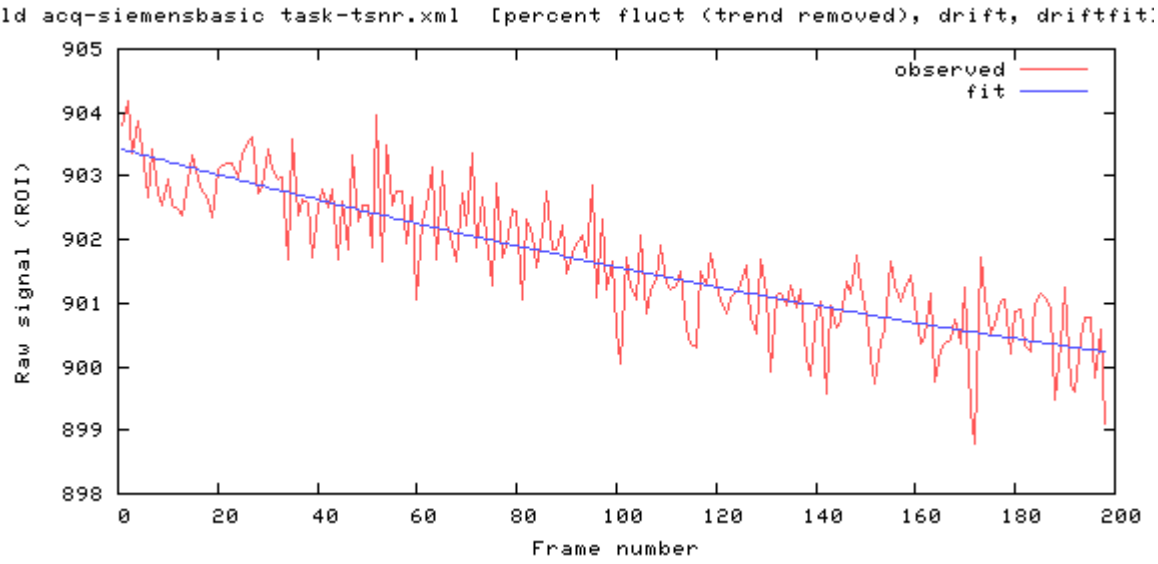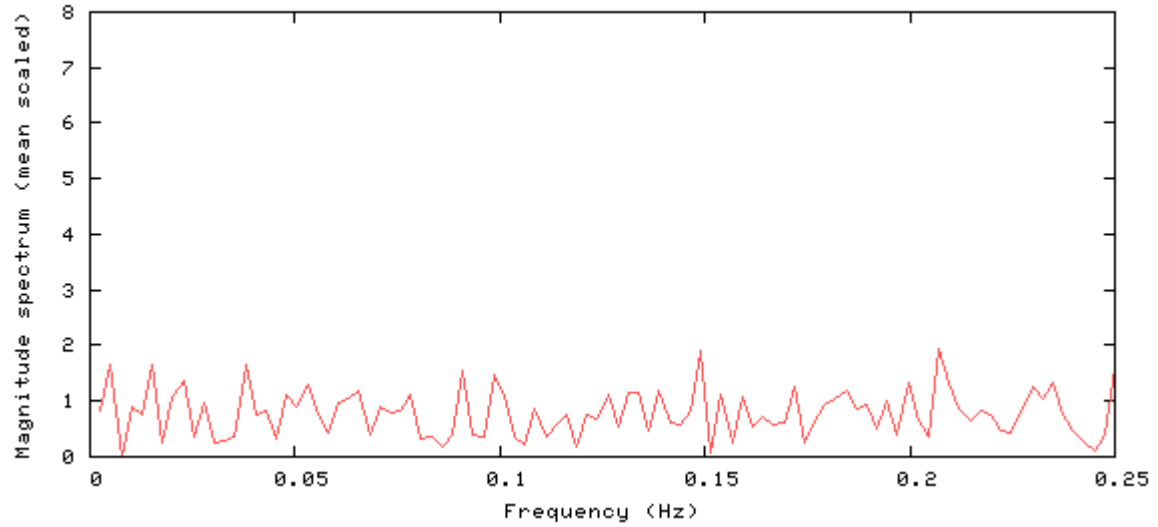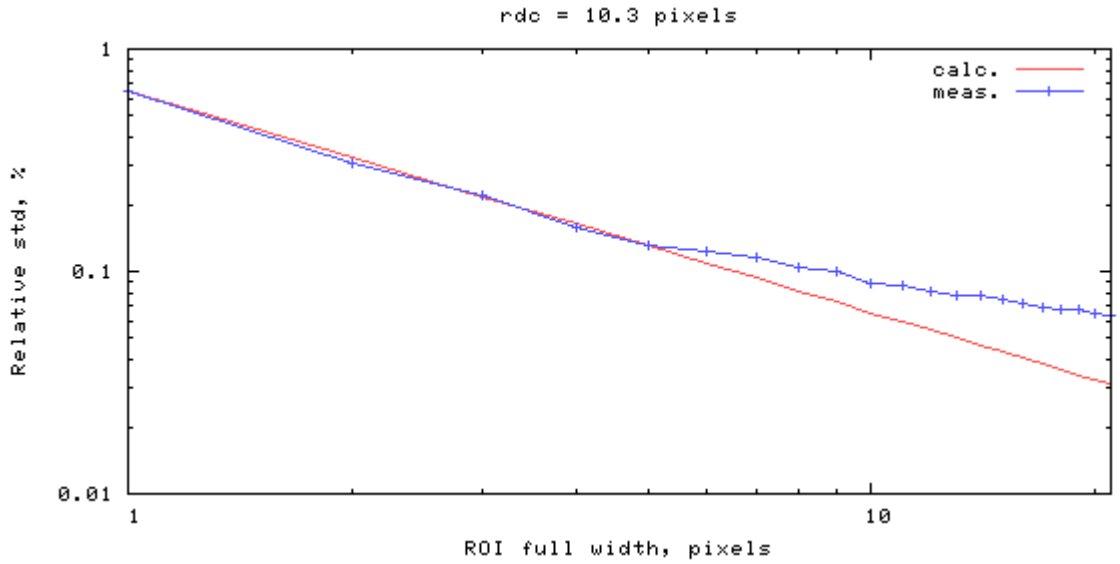



[mean, SNR, SFNR] = [901.7 174.1 183.9]

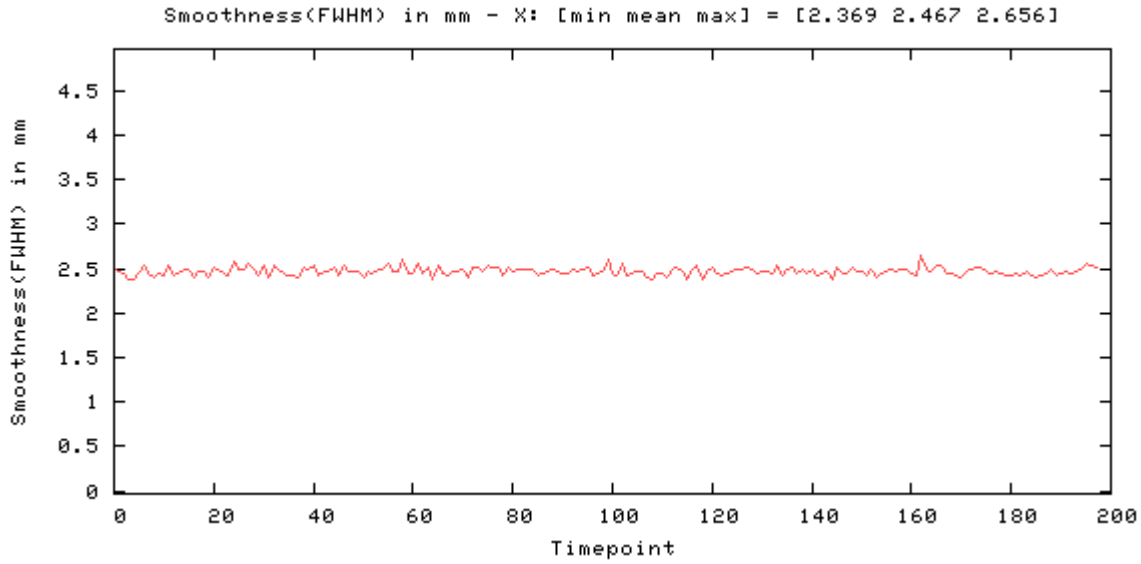




rdc = 10.3 pixels
calc.
meas.
Relative std, %
1
0.1
0.01
1
10
ROI full width, pixels



Smoothness(FWHM) in mm - X: [min mean max] = [2.369 2.467 2.656]
Smoothness(FWHM) in mm
4.5
4
3.5
3
2.5
2
1.5
1
0.5
0
0
20
40
60
80
100
120
140
160
180
200
Timepoint

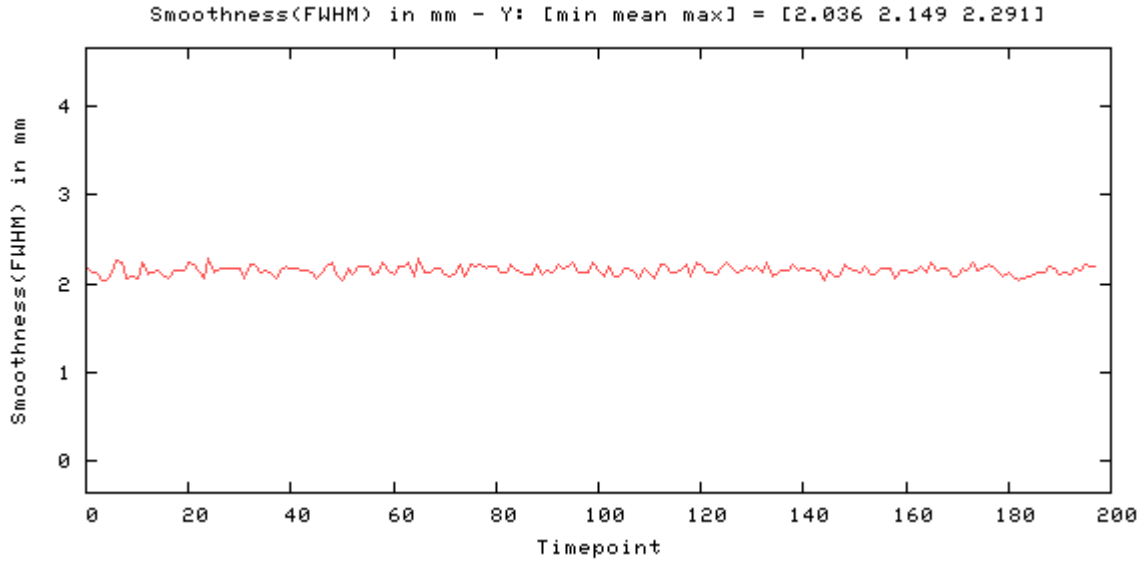

Smoothness(FWHM) in mm - Y: [min mean max] = [2.036 2.149 2.291]
Smoothness(FWHM) in mm
4
3
2
1
0
0
20
40
60
80
100
120
140
160
180
200
Timepoint

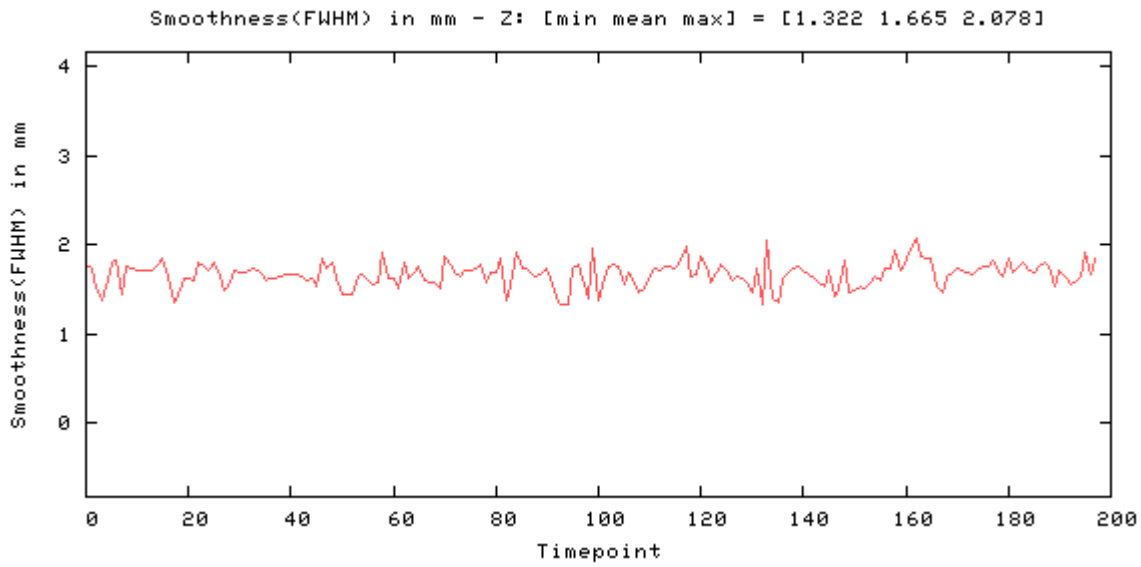
Smoothness(FWHM) in mm - Z: [min mean max] = [1.322 1.665 2.078]
Smoothness(FWHM) in mm
Timepoint
0
1
2
3
4
0
20
40
60
80
100
120
140
160
180
200

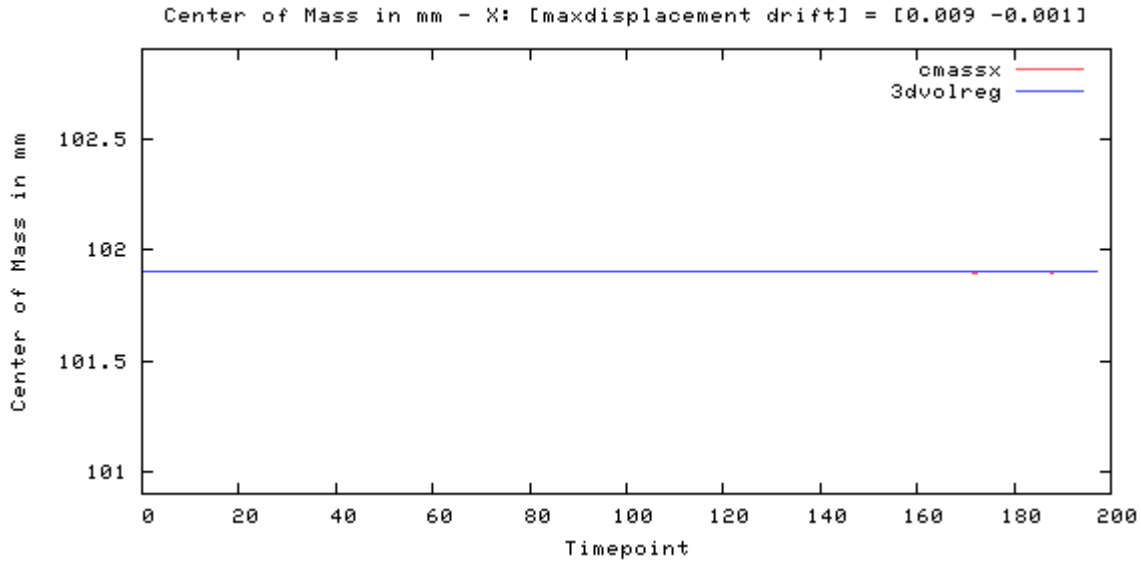
Center of Mass in mm - X: [maxdisplacement drift] = [0.009 -0.001]
Center of Mass in mm
Timepoint
cmassx
3dvolreg
101
101.5
102
102.5
0
20
40
60
80
100
120
140
160
180
200

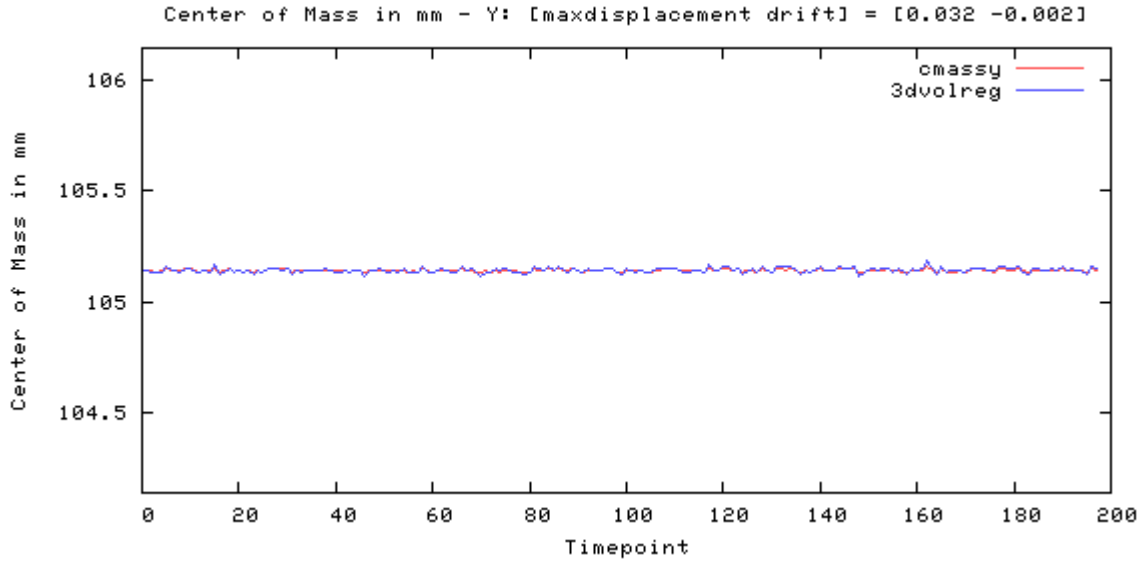
Center of Mass in mm - Y: [maxdisplacement drift] = [0.032 -0.002]
Center of Mass in mm
Timepoint
cmassy
3dvolreg
104.5
105
105.5
106
0
20
40
60
80
100
120
140
160
180
200

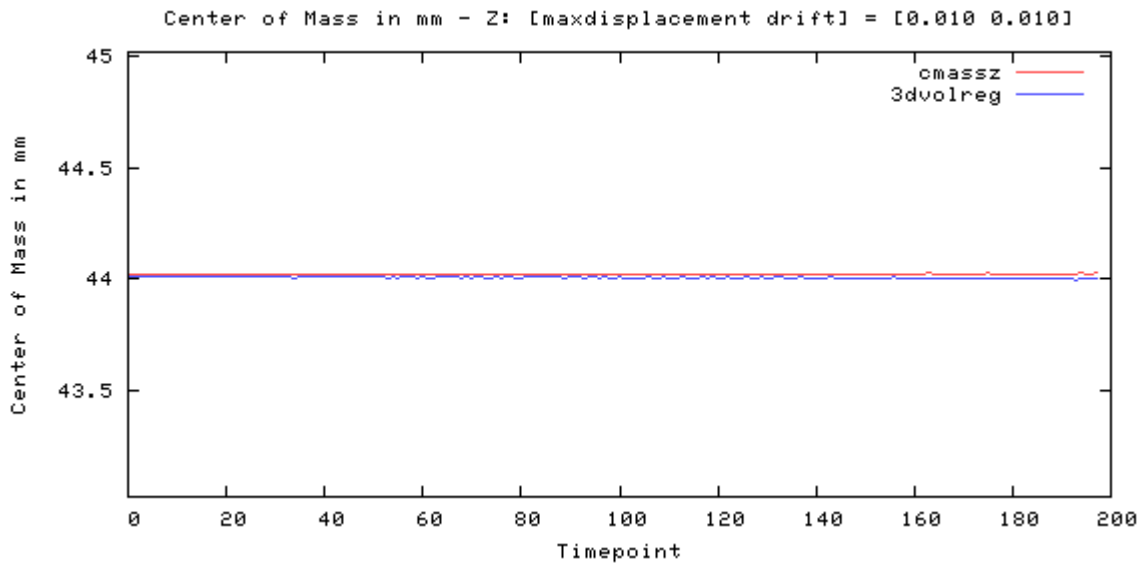


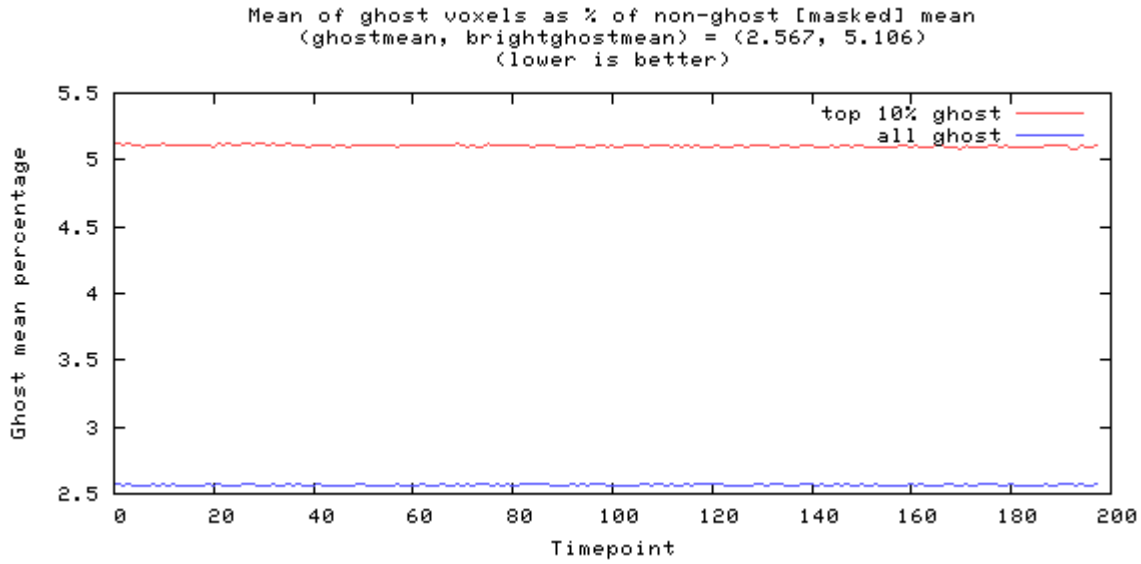

Odd-even difference image



image min: -223, image max: 243

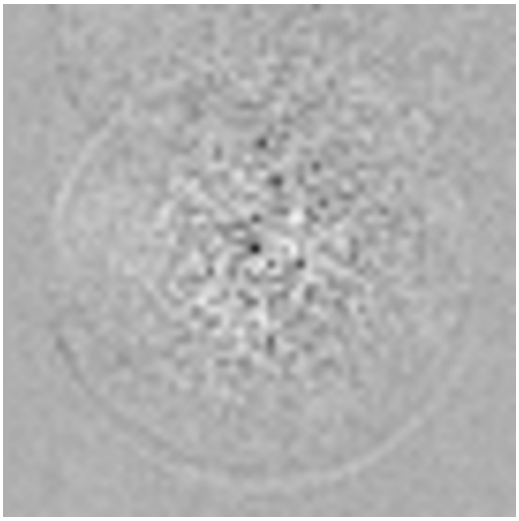

Mean image

0 1296.79


image min: 0, image max: 1314.76



Standard Deviation image

0 6.47521


image min: 0, image max: 6.47521

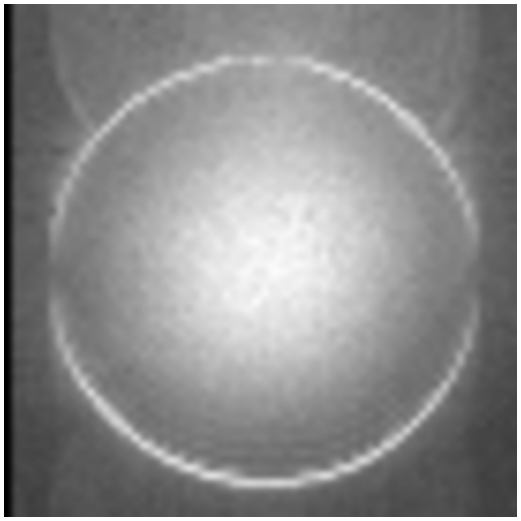

SFNR image



image min: 0, image max: 826.963

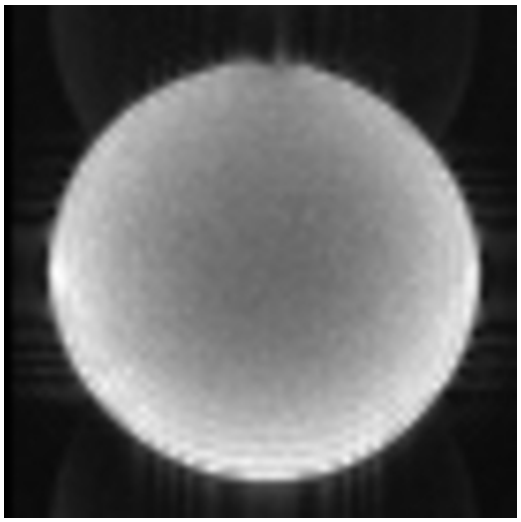

Acquisition parameters

dimensions	68x68x30x200
spacing	3mmx3mmx3mmx2000ms
gap	0mmx0mmx0mmx0ms
scanner	AWP213018
psdname	
examnumber	a0f8a673-da21-44
studyid	Stability_20261019
seriesnumber	21
runnumber	1
magneticfield	3

description	ses-32ch_func-bold_acq-siemensbasic_task-tsnr
scandate	2026-10-19
scantime	12:11:57
tr	2000
te	30
operator	
flipangle	79
prescribedslicespacing	3
frequencydirection	1
receivecoilname	Head_32
transmitcoilname	Body
institution	THE UNIVERSITY OF PENNSYLVANIA
examdescription	ACTIVE KIRWAN
scanner	AWP213018
scannermanufacturer	Siemens Healthineers
scannermodelname	MAGNETOM Cima.X
protocolname	ses-32ch_func-bold_acq-siemensbasic_task-tsnr
institutionaddress	Grays Ferry Ave. BLDG 250 STE 140 3401,Philadelphia,69 - KEYSTONE,US,19146
institutionaldepartmentname	MindCORE Neuroimaging Suite 140
acquisitiondatetime	20261019121155.617500
frametype	ORIGINAL
pixelpresentation	MONOCHROME
volumetricproperties	DISTORTED
volumebasedcalculationtechnique	NONE
complexiimagecomponent	MAGNITUDE
acquisitioncontrast	UNKNOWN
mracquisitiontype	2D
numaverages	1
spacingbetweenslices	3
echotrainlength	68
percentsampling	100
percentphasefieldofview	100
scannerserialnumber	213018
softwareversions	syngo MR XA61
inplanephaseencodingdirection	COLUMN
variableflipangleflag	N
contentqualification	PRODUCT
acquisitionduration	405.91200000000003

resonantnucleus	1H
applicablesafetystandardagency	IEC
acquisitionnumber	1
instancenumber	1
numtemporalpositions	200
samplesperpixel	1
photometricinterpretation	MONOCHROME2
numberofframes	30
rows	68
columns	68
bitsallocated	16
bitsstored	12
highbit	11
lossyimagecompression	00