




Phantom QA results for / fbirn_out/ses-64ch_func-bold_acq-cmrrme_task-tsnrxacpc.xml, slice 35

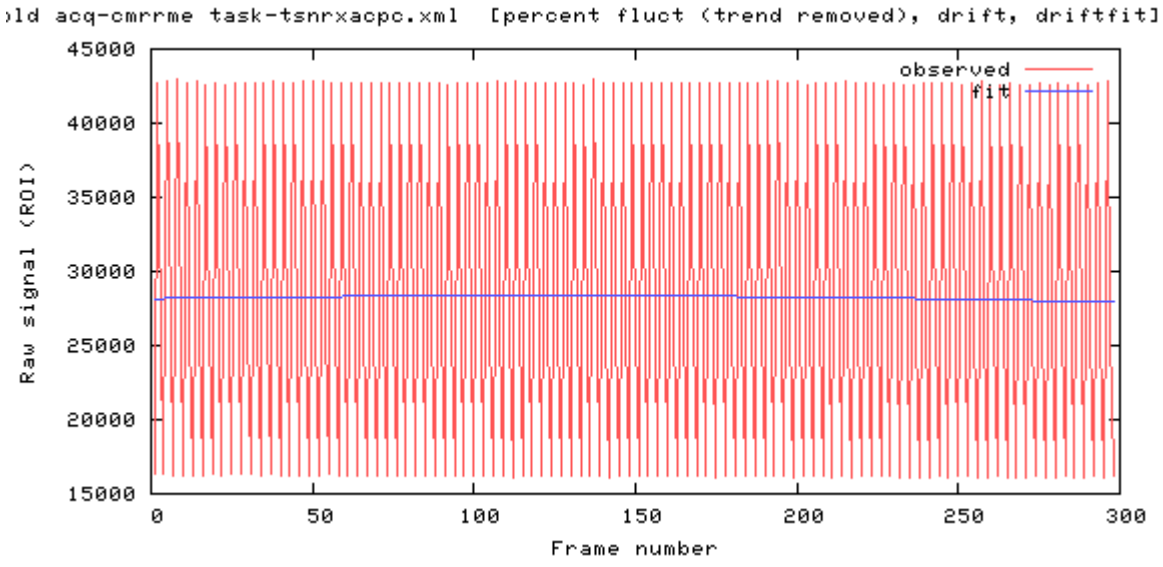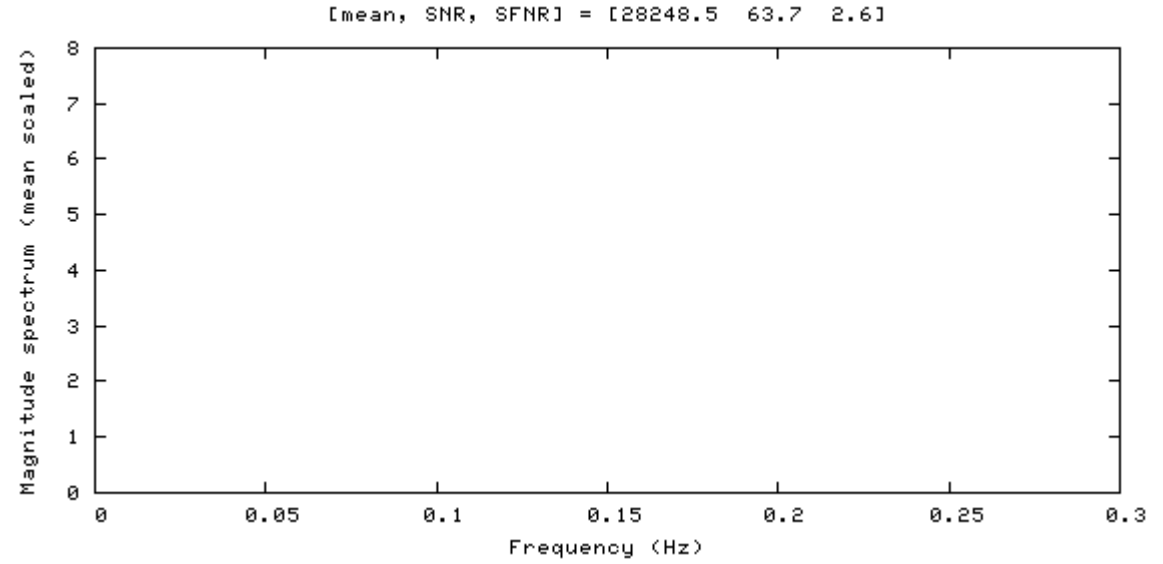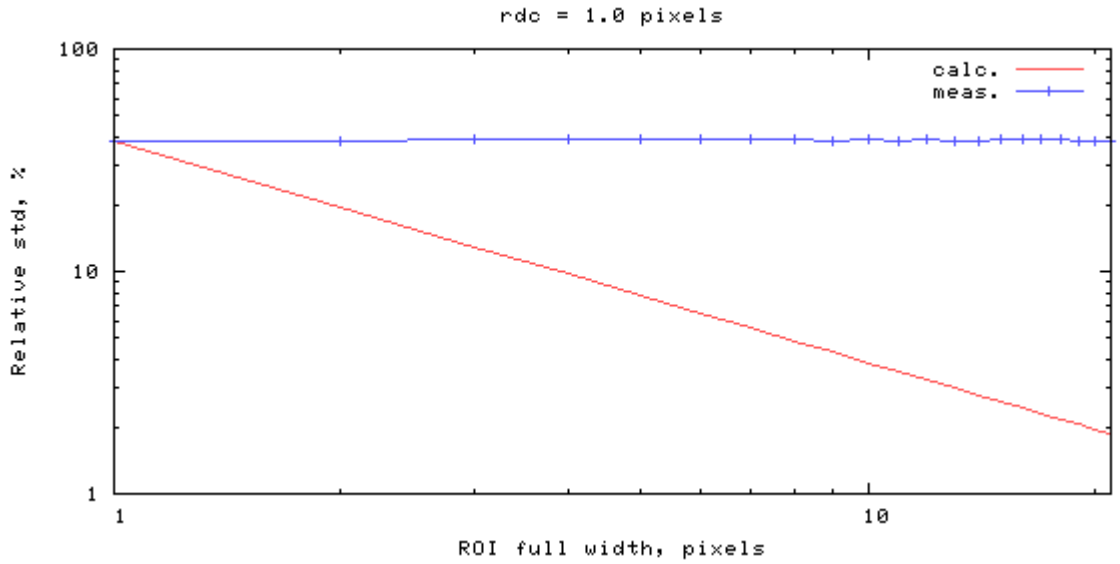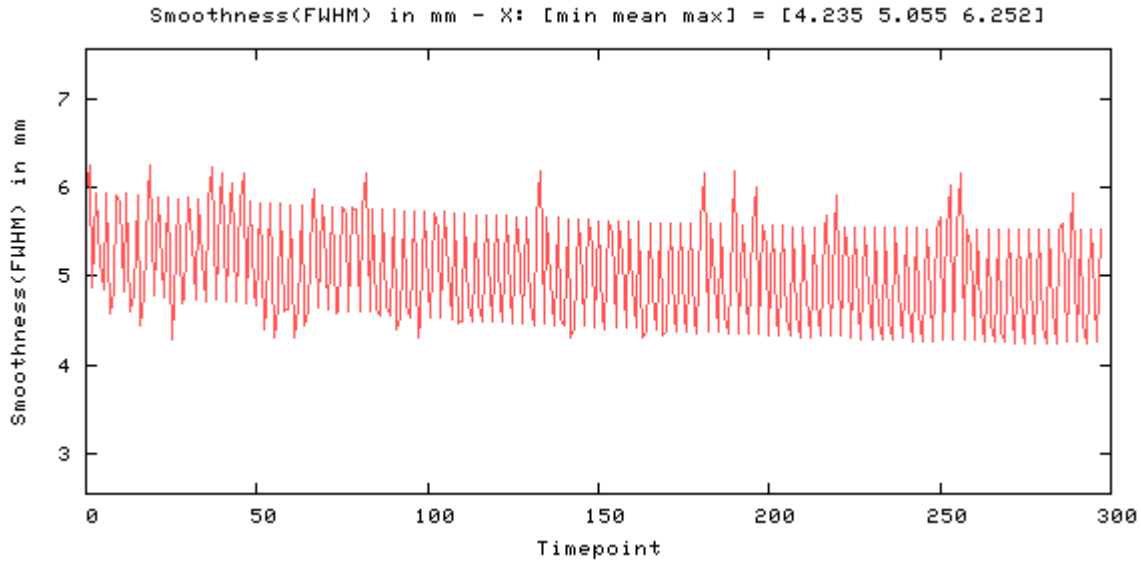


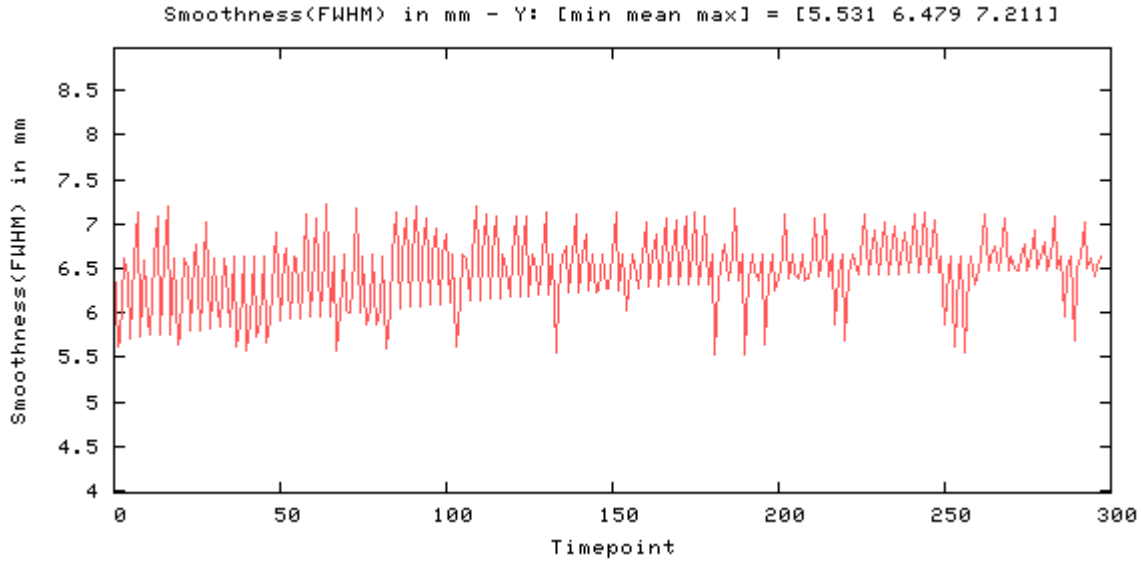




rdc = 1.0 pixels
calc.
meas.
Relative std, %
100
10
1
1
10
ROI full width, pixels



Smoothness(FWHM) in mm - X: [min mean max] = [4.235 5.055 6.252]
Smoothness(FWHM) in mm
7
6
5
4
3
0
50
100
150
200
250
300
Timepoint



Smoothness(FWHM) in mm - Y: [min mean max] = [5.531 6.479 7.211]
Smoothness(FWHM) in mm
8.5
8
7.5
7
6.5
6
5.5
5
4.5
4
0
50
100
150
200
250
300
Timepoint

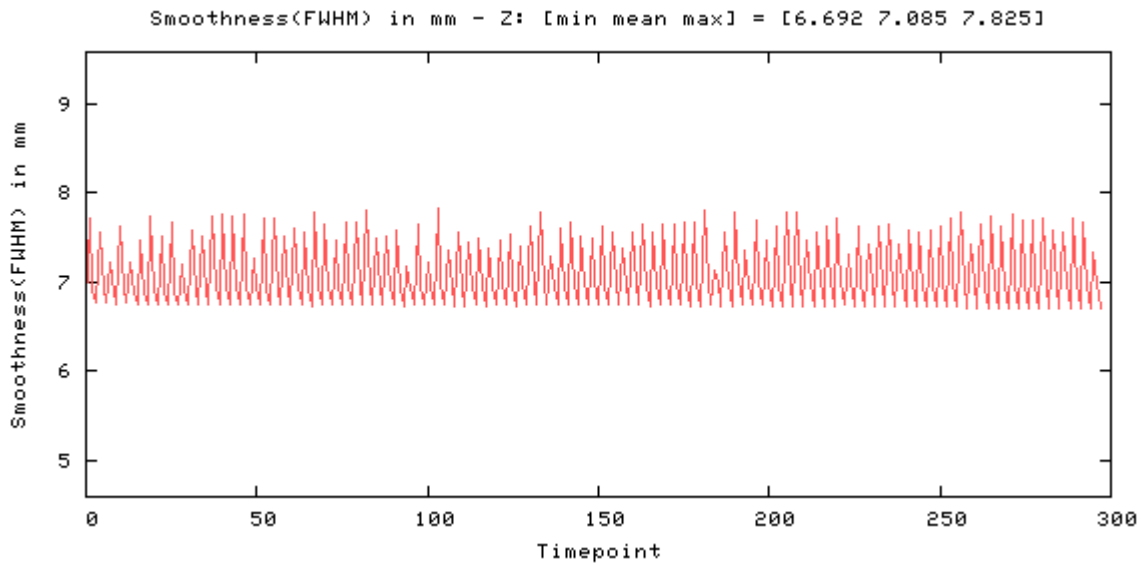
Smoothness(FWHM) in mm - Z: [min mean max] = [6.692 7.085 7.825]
Smoothness(FWHM) in mm
9
8
7
6
5
0
50
100
150
200
250
300
Timepoint

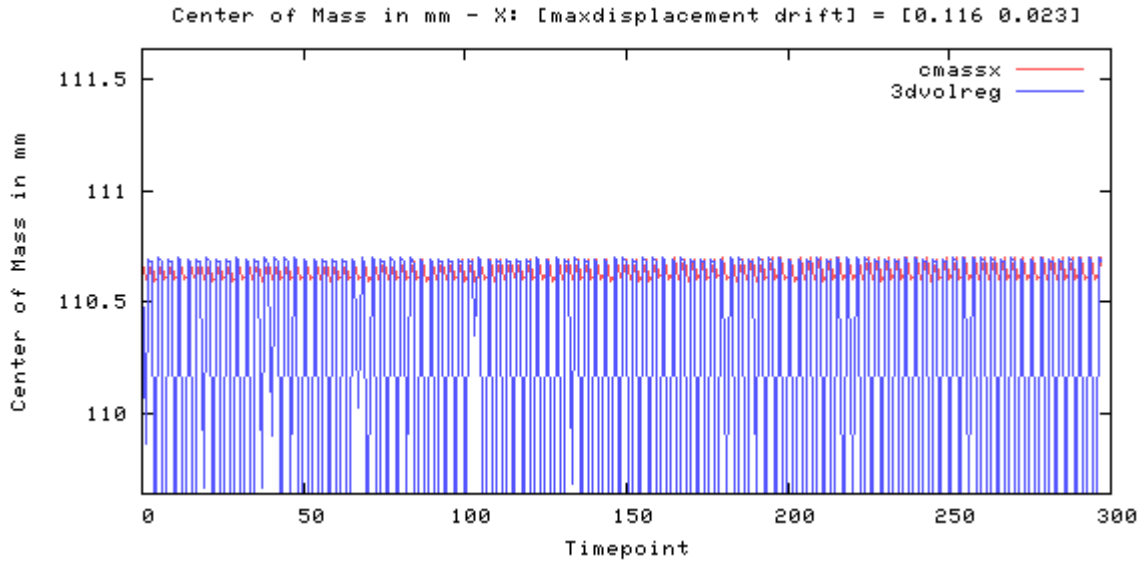
Center of Mass in mm - X: [maxdisplacement drift] = [0.116 0.023]
Center of Mass in mm
111.5
111
110.5
110
cmassx
3dvolreg
0
50
100
150
200
250
300
Timepoint

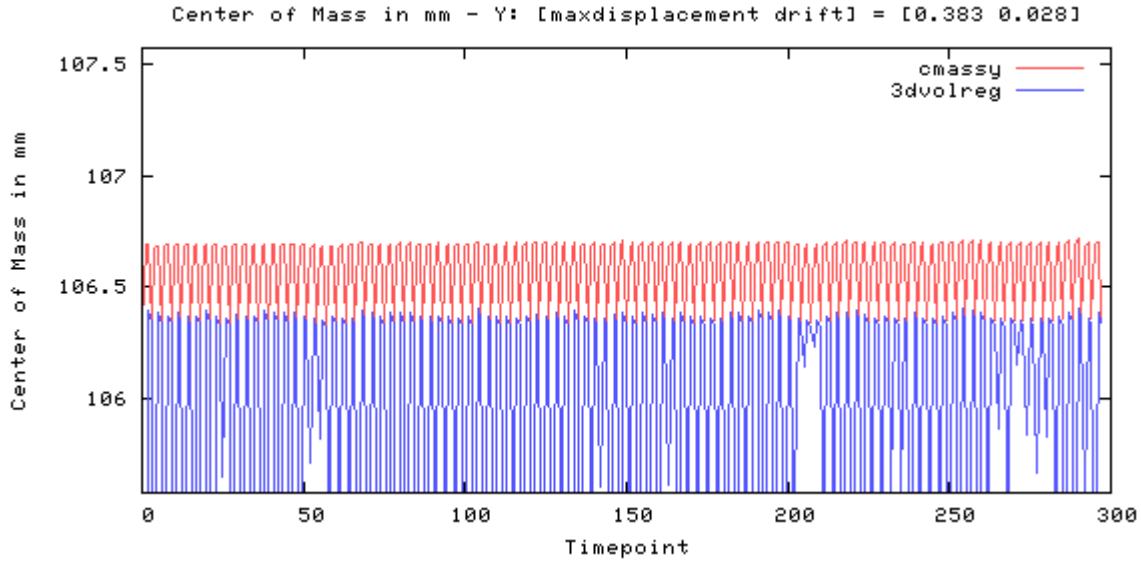
Center of Mass in mm - Y: [maxdisplacement drift] = [0.383 0.028]
Center of Mass in mm
107.5
107
106.5
106
cmassy
3dvolreg
0
50
100
150
200
250
300
Timepoint

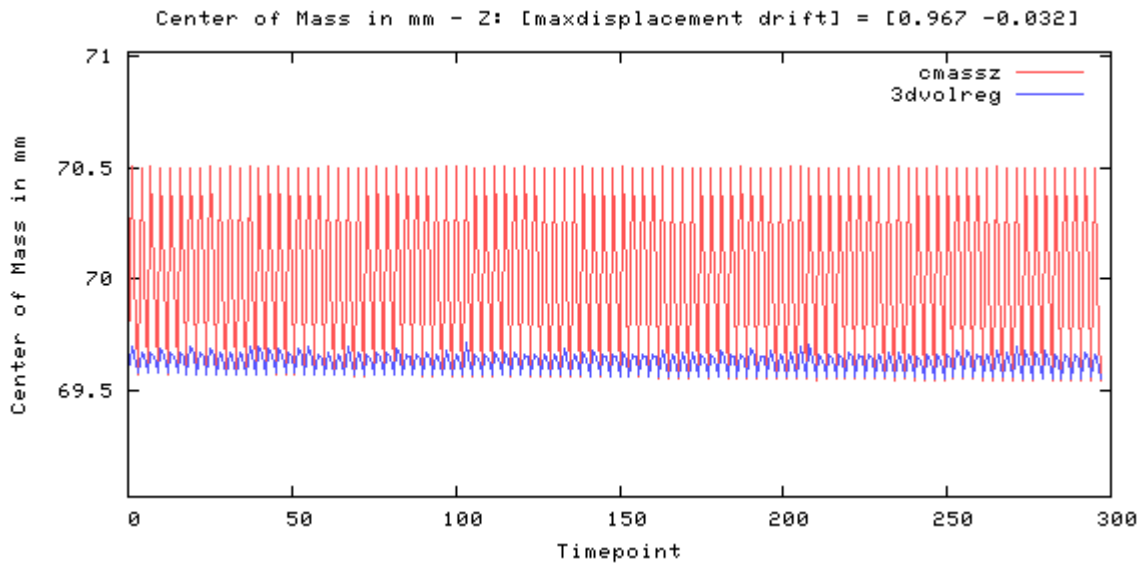

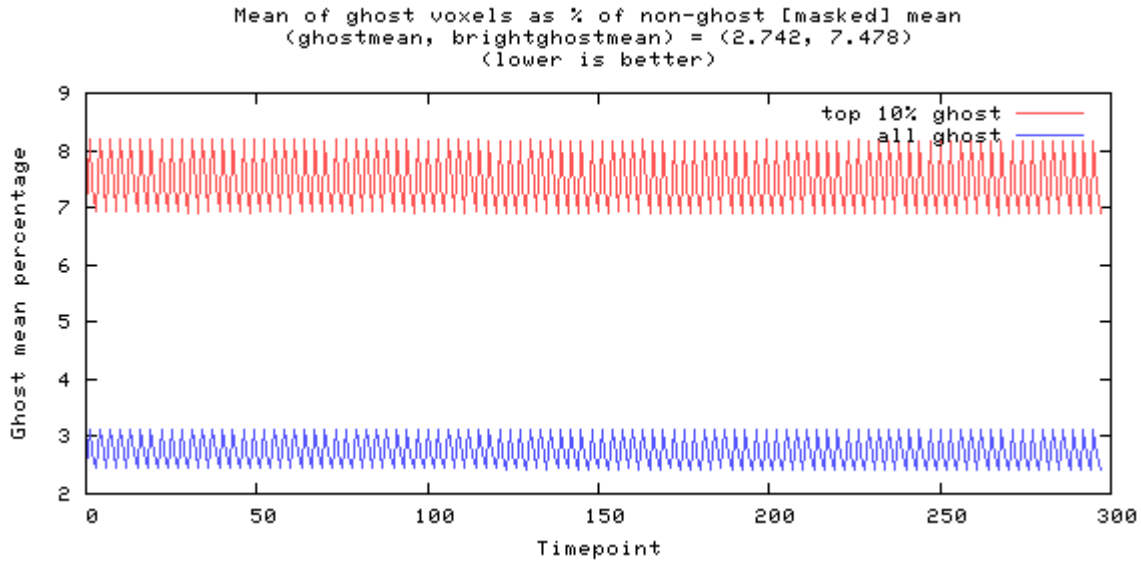


Odd-even difference image

-44362	5652




image min: -44362, image max: 5652

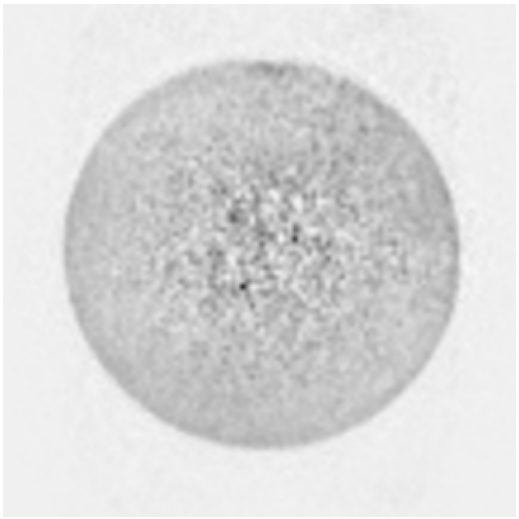

Mean image

0 38558.6


image min: 0, image max: 38558.6

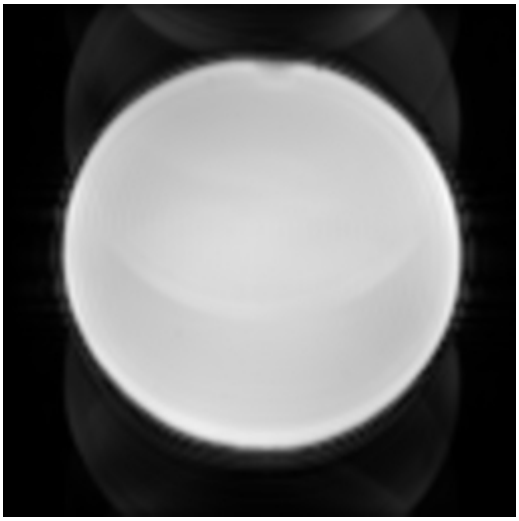

Standard Deviation image

0 15036.8


image min: 0, image max: 15037.4

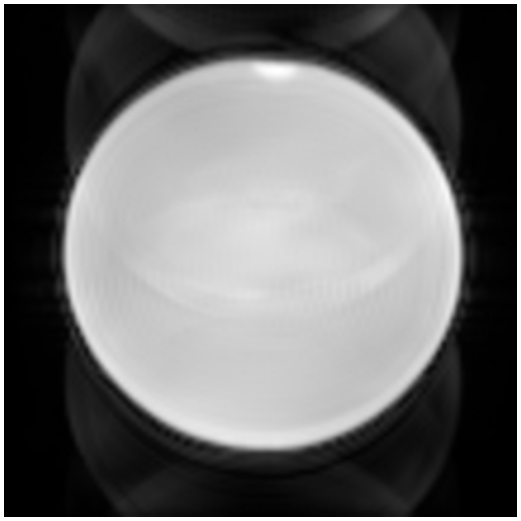

SFNR image



image min: 0, image max: 10.766

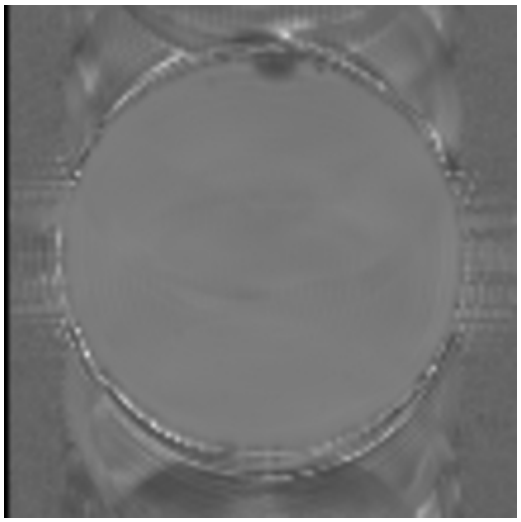

Acquisition parameters

dimensions	108x108x72x300
spacing	2.03704mmx2.03704mmx2mmx0ms
gap	0mmx0mmx0mmx0ms
scanner	AWP213018
psdname	
examnumber	a0f8a673-da21-44
studyid	Stability_20261019
seriesnumber	13
runnumber	1
magneticfield	3

description	ses-64ch_func-bold_acq-cmrrme_task-tsnrxacpc
scandate	2026-10-19
scantime	11:57:34
tr	1720
te	13.4 37.84 62.28 13.4 37.84 62.28 13.4 37.84 62.28

operator	
flipangle	70
prescribedslicespacing	2
frequencydirection	1
receivecoilname	HeadNeck_64_CS
transmitcoilname	Body
institution	THE UNIVERSITY OF PENNSYLVANIA
examdescription	ACTIVE KIRWAN
scanner	AWP213018
scannermanufacturer	Siemens Healthineers
scannermodelname	MAGNETOM Cima.X
protocolname	ses-64ch_func-bold_acq-cmrrme_task-tsnrxacpc
institutionaddress	Grays Ferry Ave. BLDG 250 STE 140 3401,Philadelphia,69 - KEYSTONE,US,19146
institutionaldepartmentname	MindCORE Neuroimaging Suite 140
acquisitiondatetime	20261019115717.422500
frametype	ORIGINAL
pixelpresentation	MONOCHROME
volumetricproperties	DISTORTED
volumebasedcalculationtechnique	NONE
complexiimagecomponent	MAGNITUDE
acquisitioncontrast	UNKNOWN
mracquisitiontype	2D
numaverages	1
spacingbetweenslices	2
echotrainlength	40
percentsampling	100
percentphasefieldofview	100
scannerserialnumber	213018
softwareversions	syngo MR XA61
inplanephaseencodingdirection	COLUMN
variableflipangleflag	N
contentqualification	RESEARCH
acquisitionduration	204.60500000000002
resonantnucleus	1H
applicablesafetystandardagency	IEC
acquisitionnumber	1
instancenumber	1
numtemporalpositions	100
imagecomments	

	Not for diagnostic use, Unaliased MB4/ PE4/LB SENSE1
samplesperpixel	1
photometricinterpretation	MONOCHROME2
numberofframes	72
rows	108
columns	108
bitsallocated	16
bitsstored	16
highbit	15
lossyimagecompression	00