




Phantom QA results for / fbirn_out/ses-64ch_func-bold_acq-siemensstd_task-tsnr.xml, slice 17

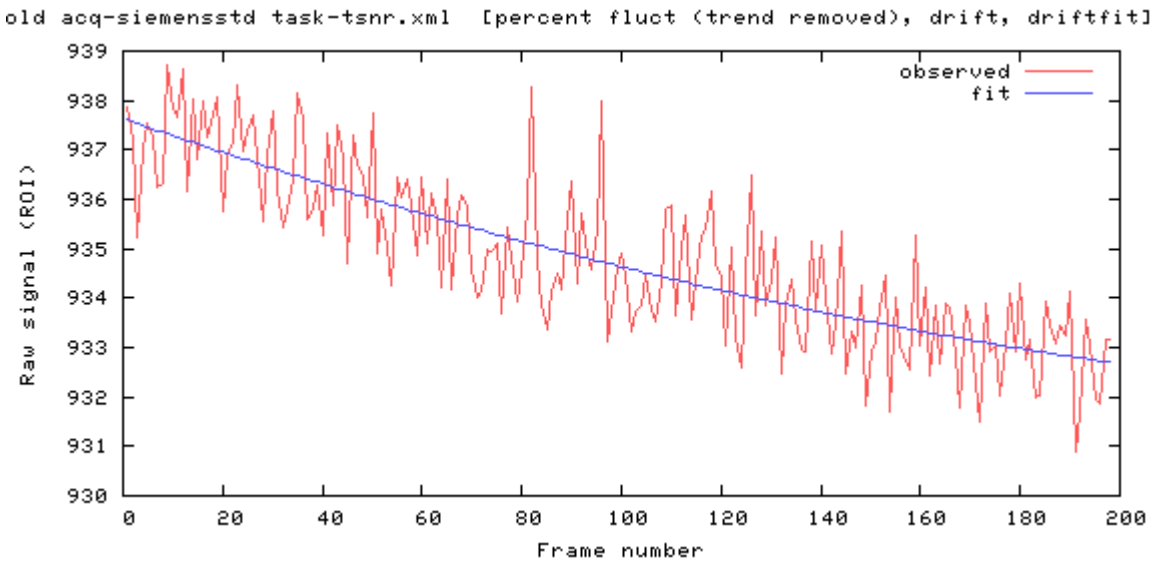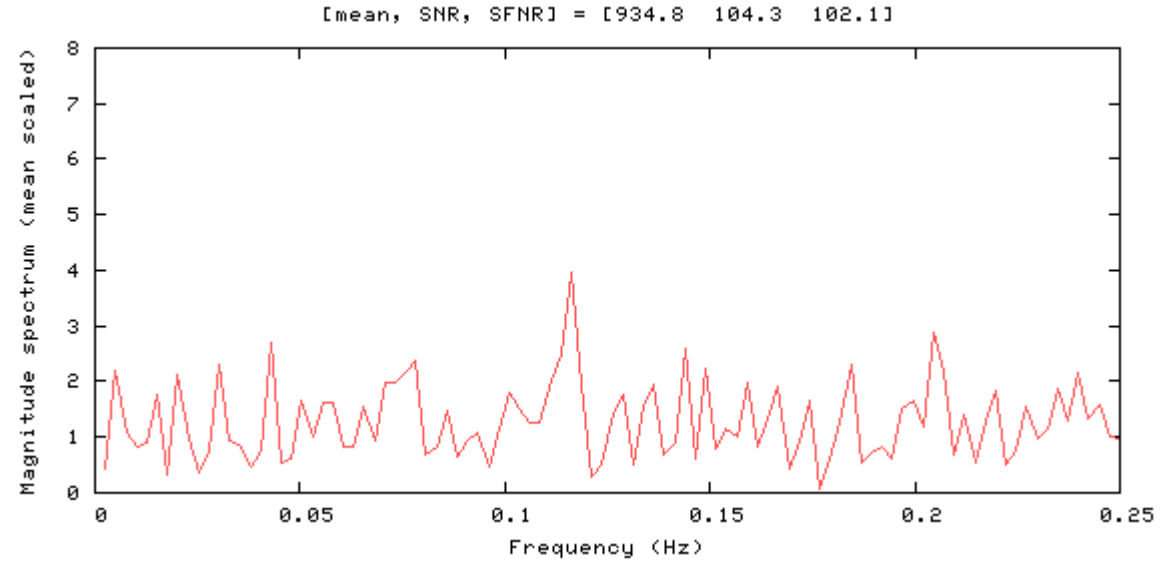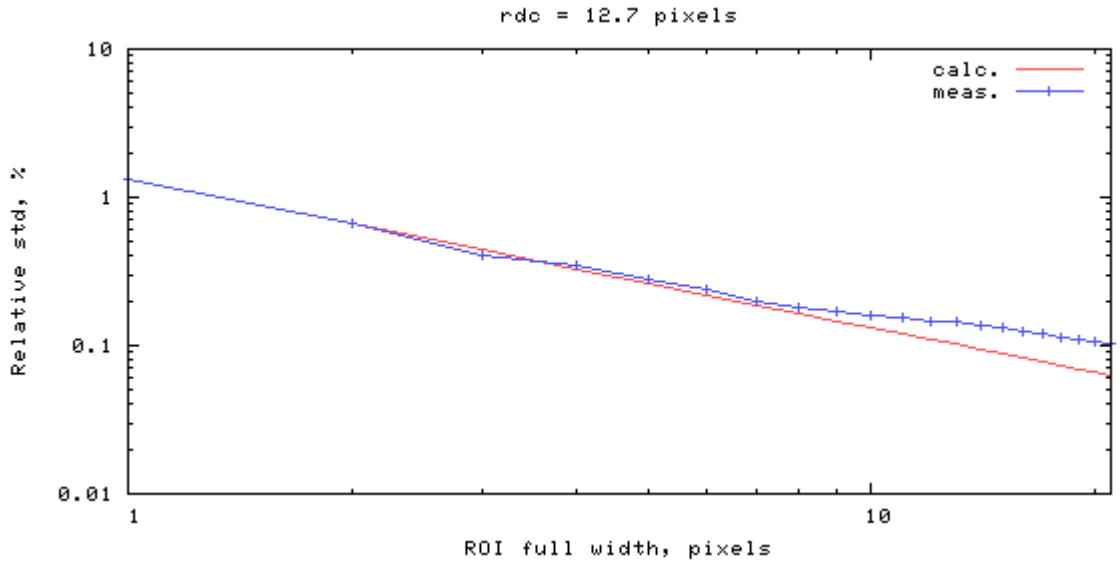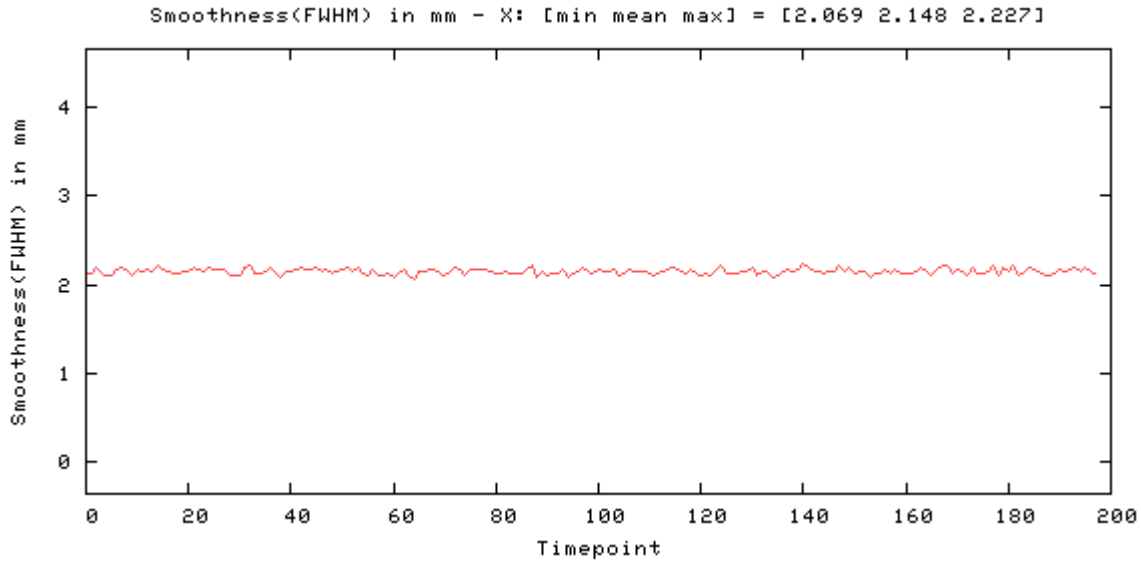


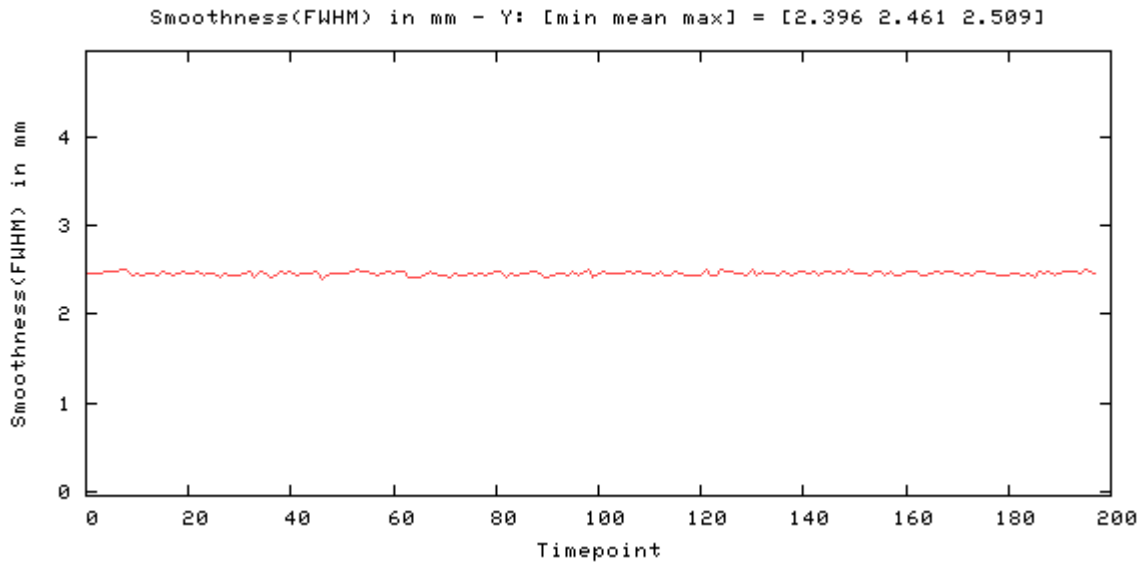




rdc = 12.7 pixels
calc.
meas.
Relative std, %
10
1
0.1
0.01
1
10
ROI full width, pixels



Smoothness(FWHM) in mm - X: [min mean max] = [2.069 2.148 2.227]
Smoothness(FWHM) in mm
4
3
2
1
0
0
20
40
60
80
100
120
140
160
180
200
Timepoint



Smoothness(FWHM) in mm - Y: [min mean max] = [2.396 2.461 2.509]
Smoothness(FWHM) in mm
4
3
2
1
0
0
20
40
60
80
100
120
140
160
180
200
Timepoint

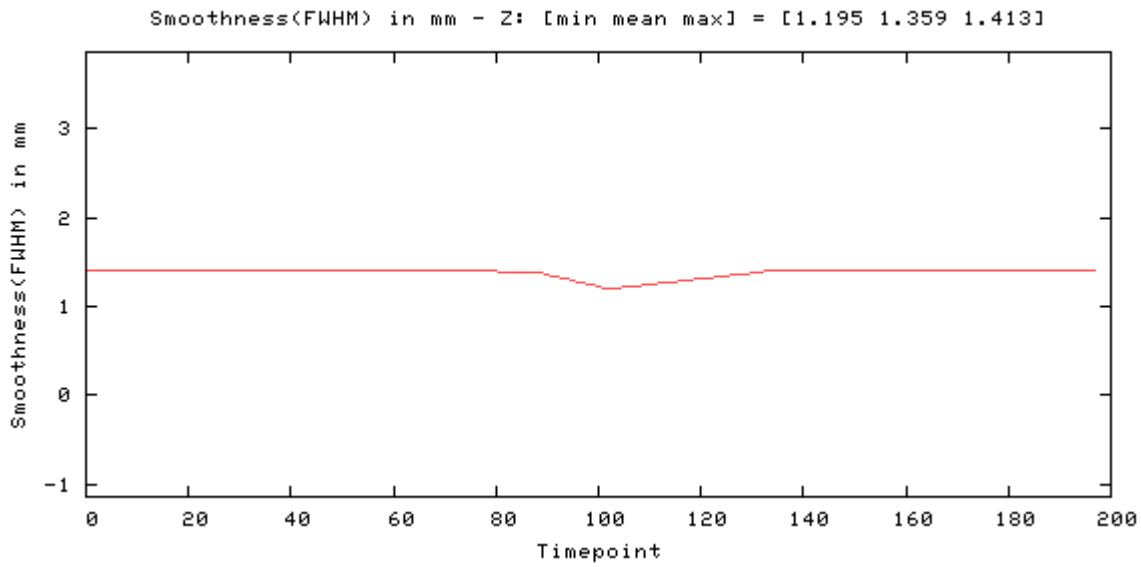
Smoothness(FWHM) in mm - Z: [min mean max] = [1.195 1.359 1.413]
Smoothness(FWHM) in mm
3
2
1
0
-1
0
20
40
60
80
100
120
140
160
180
200
Timepoint

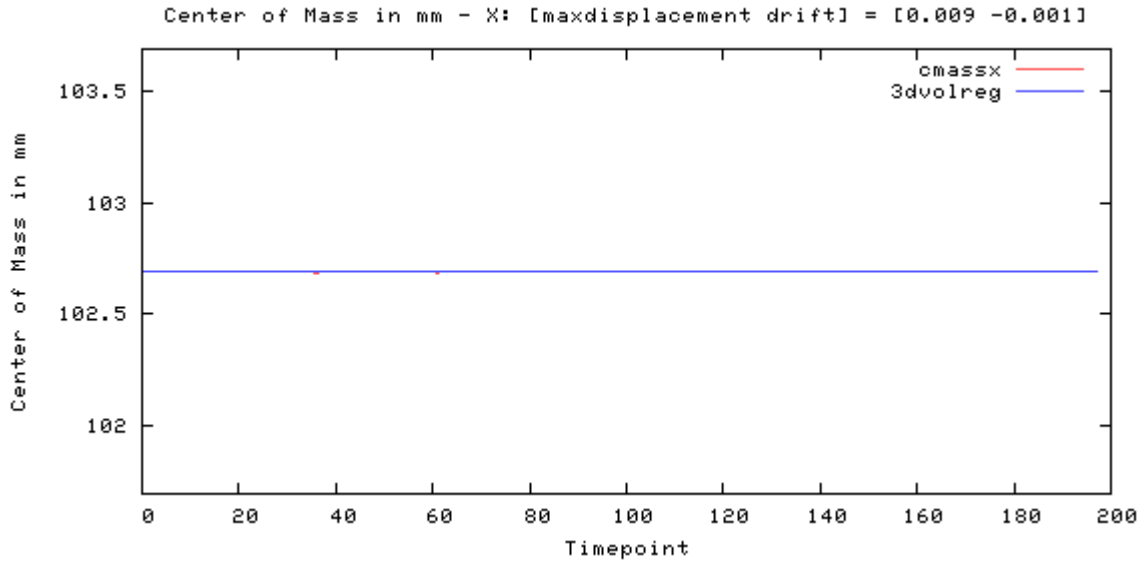
Center of Mass in mm - X: [maxdisplacement drift] = [0.009 -0.001]
cmassx
3dvolreg
Center of Mass in mm
103.5
103
102.5
102
0
20
40
60
80
100
120
140
160
180
200
Timepoint

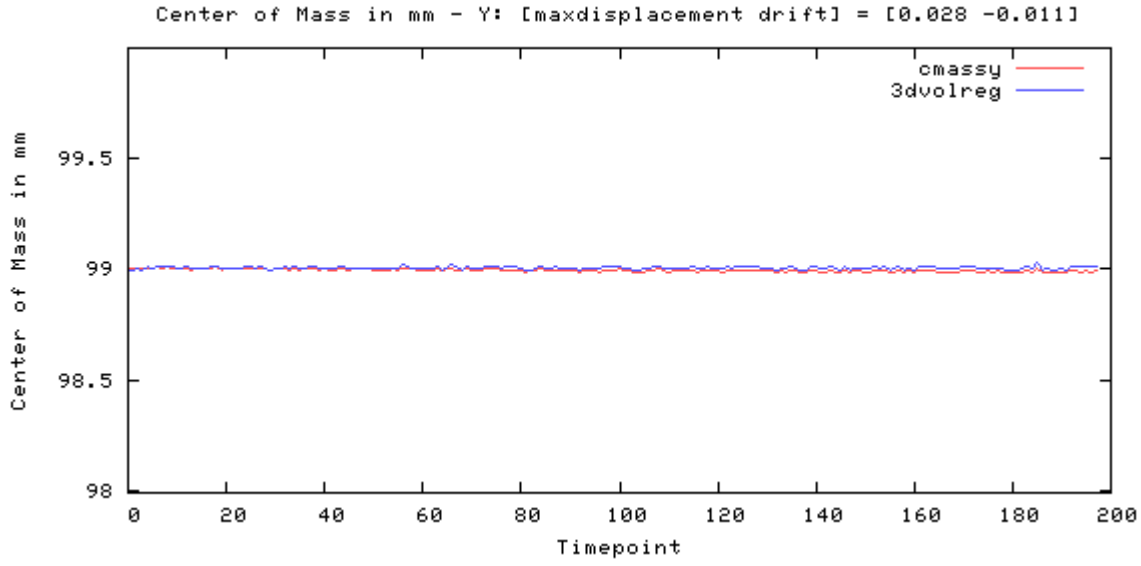
Center of Mass in mm - Y: [maxdisplacement drift] = [0.028 -0.011]
cmassy
3dvolreg
Center of Mass in mm
99.5
99
98.5
98
0
20
40
60
80
100
120
140
160
180
200
Timepoint

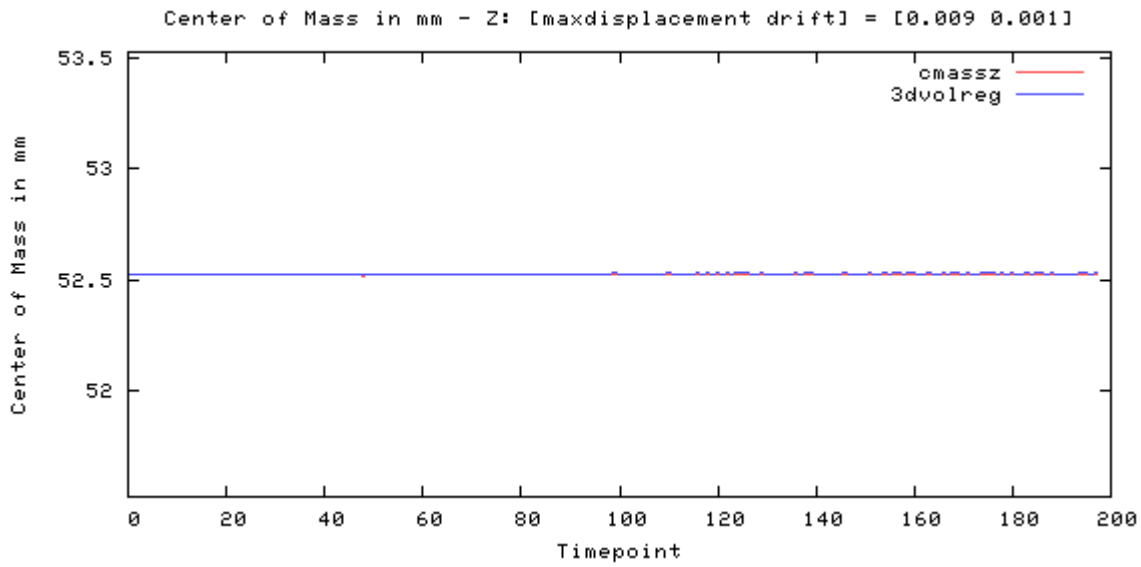


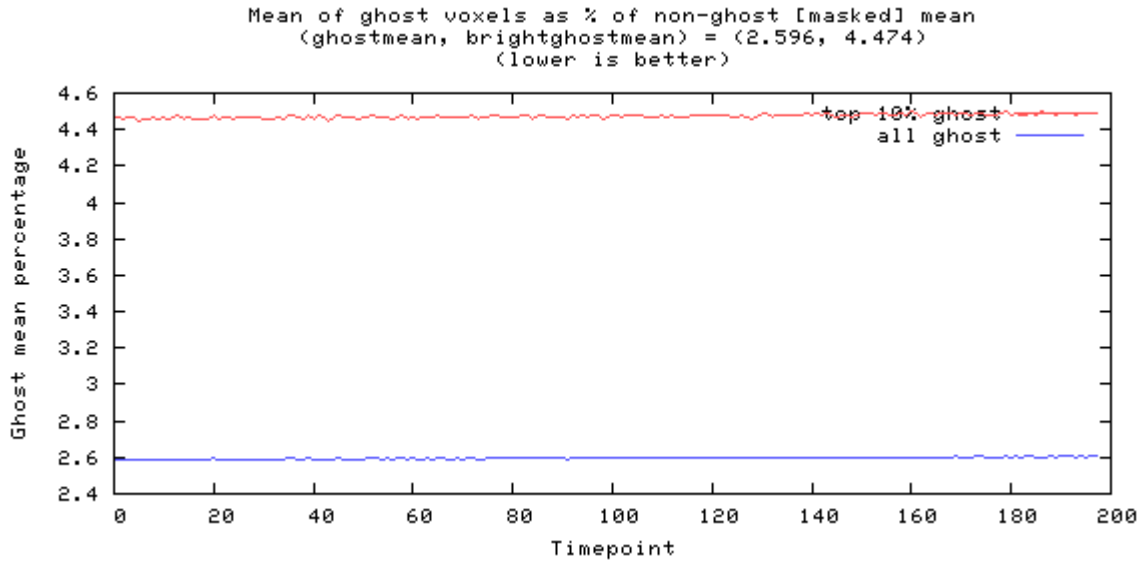

Odd-even difference image

-516 374

image min: -516, image max: 374

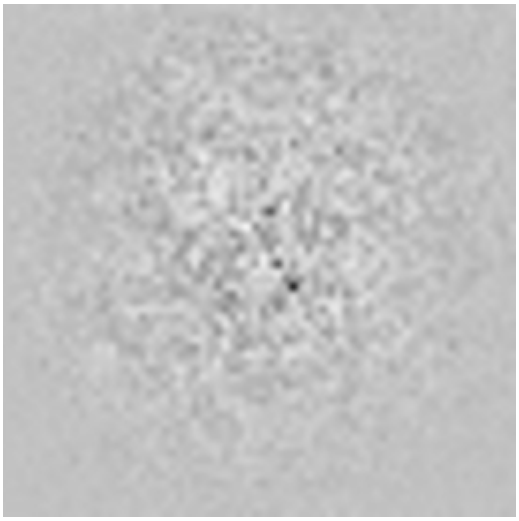

Mean image

0 1339.53


image min: 0, image max: 1339.53



Standard Deviation image

0 12.6419


image min: 0, image max: 12.8246

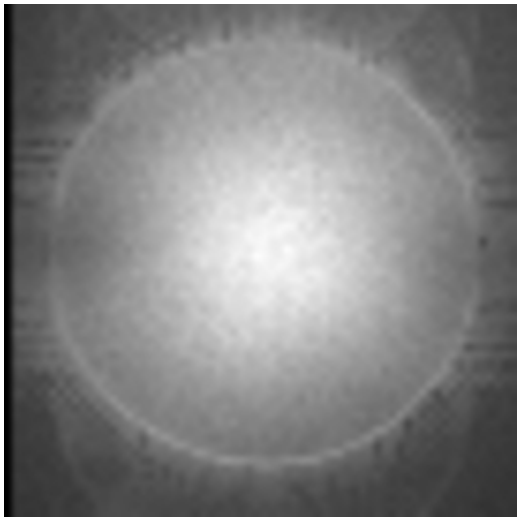

SFNR image

0 499.682

image min: 0, image max: 544.283

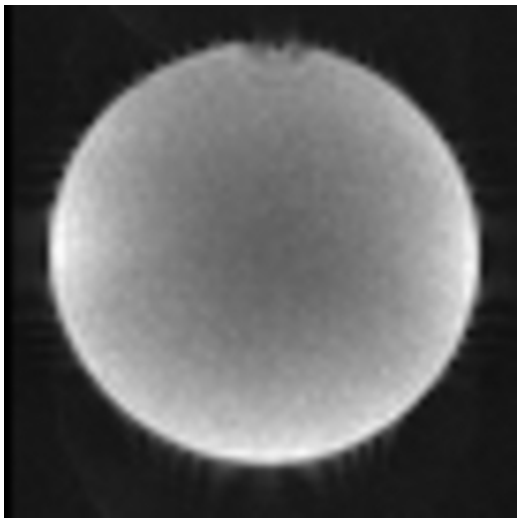

Acquisition parameters

dimensions	68x68x36x200
spacing	3mmx3mmx3mmx2000ms
gap	0mmx0mmx0mmx0ms
scanner	AWP213018
psdname	
examnumber	a0f8a673-da21-44
studyid	Stability_20261019
seriesnumber	4
runnumber	1
magneticfield	3

description	ses-64ch_func-bold_acq-siemensstd_task-tsnr
scandate	2026-10-19
scantime	11:31:31
tr	2000
te	30
operator	
flipangle	79
prescribedslicespacing	3
frequencydirection	1
receivecoilname	HeadNeck_64_CS
transmitcoilname	Body
institution	THE UNIVERSITY OF PENNSYLVANIA
examdescription	ACTIVE KIRWAN
scanner	AWP213018
scannermanufacturer	Siemens Healthineers
scannermodelname	MAGNETOM Cima.X
protocolname	ses-64ch_func-bold_acq-siemensstd_task-tsnr
institutionaddress	Grays Ferry Ave. BLDG 250 STE 140 3401,Philadelphia,69 - KEYSTONE,US,19146
institutionaldepartmentname	MindCORE Neuroimaging Suite 140
acquisitiondatetime	20261019113129.562500
frametype	ORIGINAL
pixelpresentation	MONOCHROME
volumetricproperties	DISTORTED
volumebasedcalculationtechnique	NONE
complexiimagecomponent	MAGNITUDE
acquisitioncontrast	UNKNOWN
mracquisitiontype	2D
numaverages	1
spacingbetweenslices	3
echotrainlength	33
percentsampling	100
percentphasefieldofview	100
scannerserialnumber	213018
softwareversions	syngo MR XA61
inplanephaseencodingdirection	COLUMN
variableflipangleflag	N
contentqualification	PRODUCT
acquisitionduration	407.92500000000001

resonantnucleus	1H
applicablesafetystandardagency	IEC
acquisitionnumber	1
instancenumber	1
numtemporalpositions	200
samplesperpixel	1
photometricinterpretation	MONOCHROME2
numberofframes	36
rows	68
columns	68
bitsallocated	16
bitsstored	12
highbit	11
lossyimagecompression	00