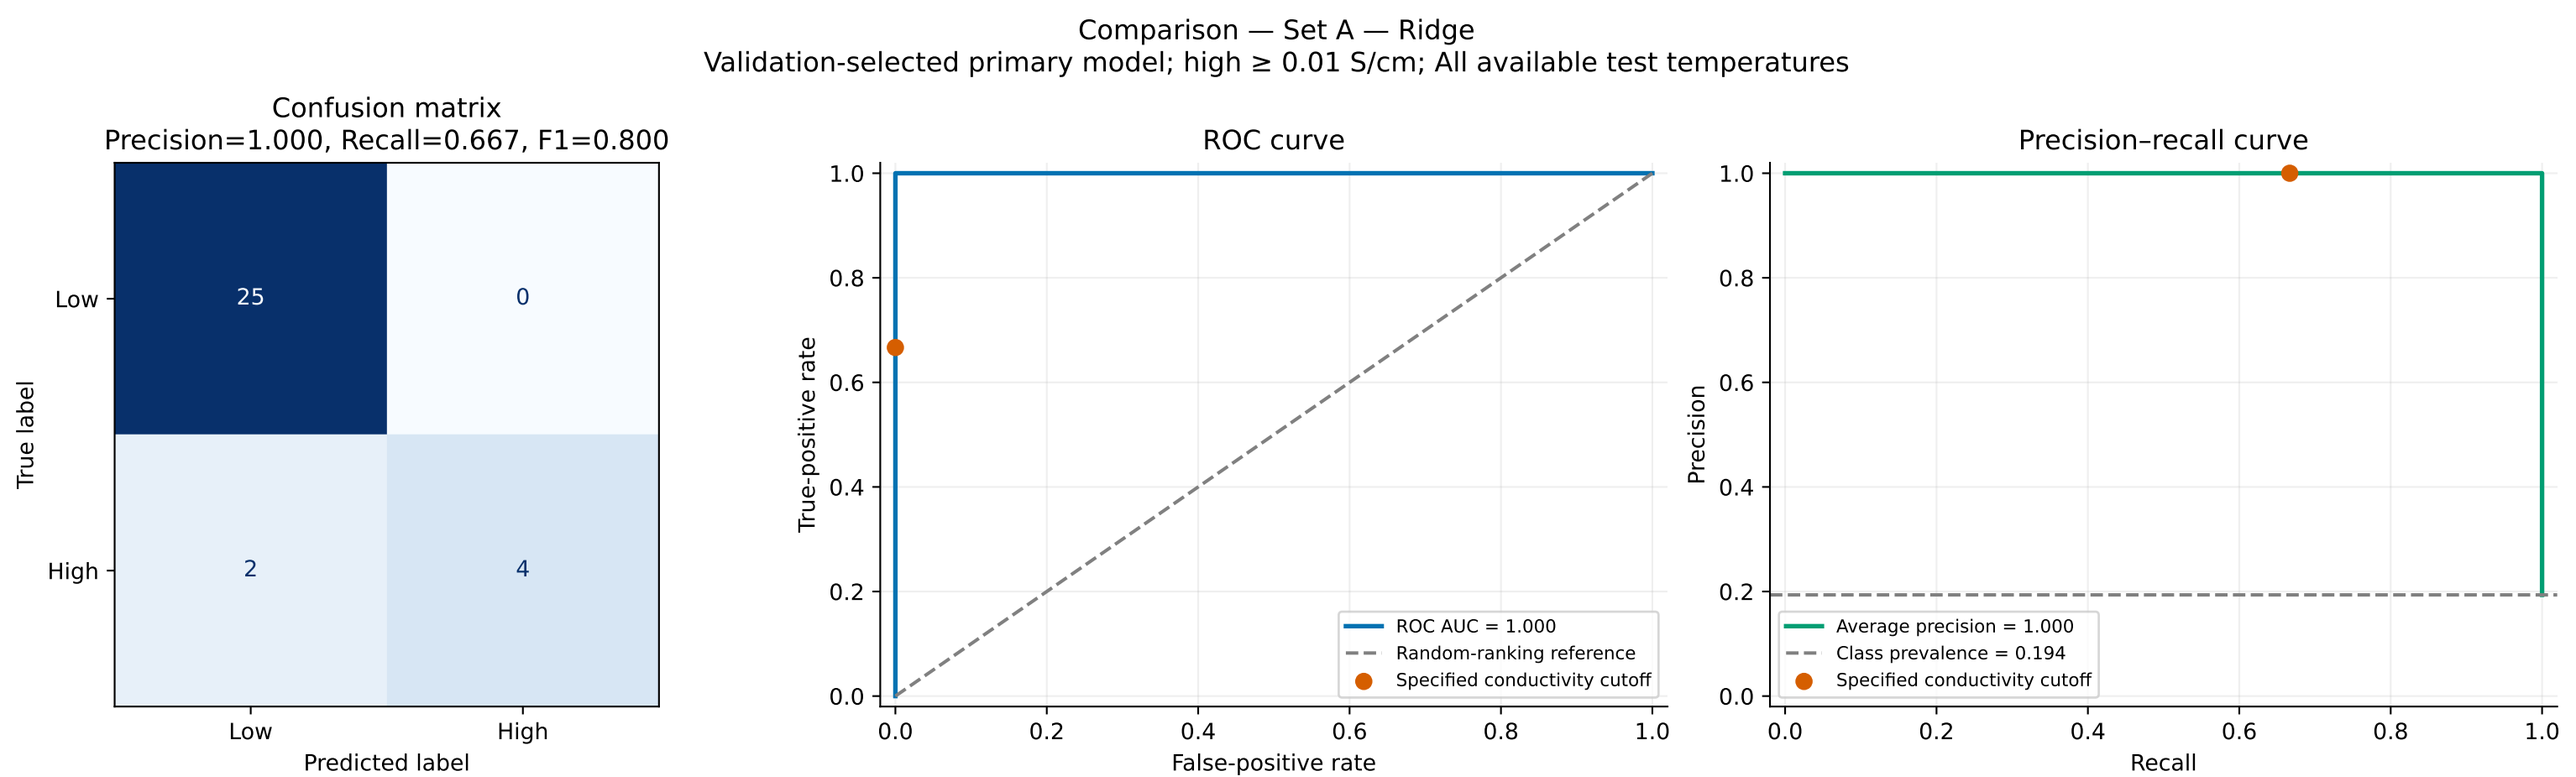
Comparison — Set A — Ridge
Validation-selected primary model; high ≥ 0.01 S/cm; All available test temperatures
Confusion matrix
Precision=1.000, Recall=0.667, F1=0.800
25
0
2
4
Low
High
True label
Low
High
Predicted label
ROC curve
True-positive rate
False-positive rate
ROC AUC = 1.000
Random-ranking reference
Specified conductivity cutoff
Precision–recall curve
Precision
Recall
Average precision = 1.000
Class prevalence = 0.194
Specified conductivity cutoff