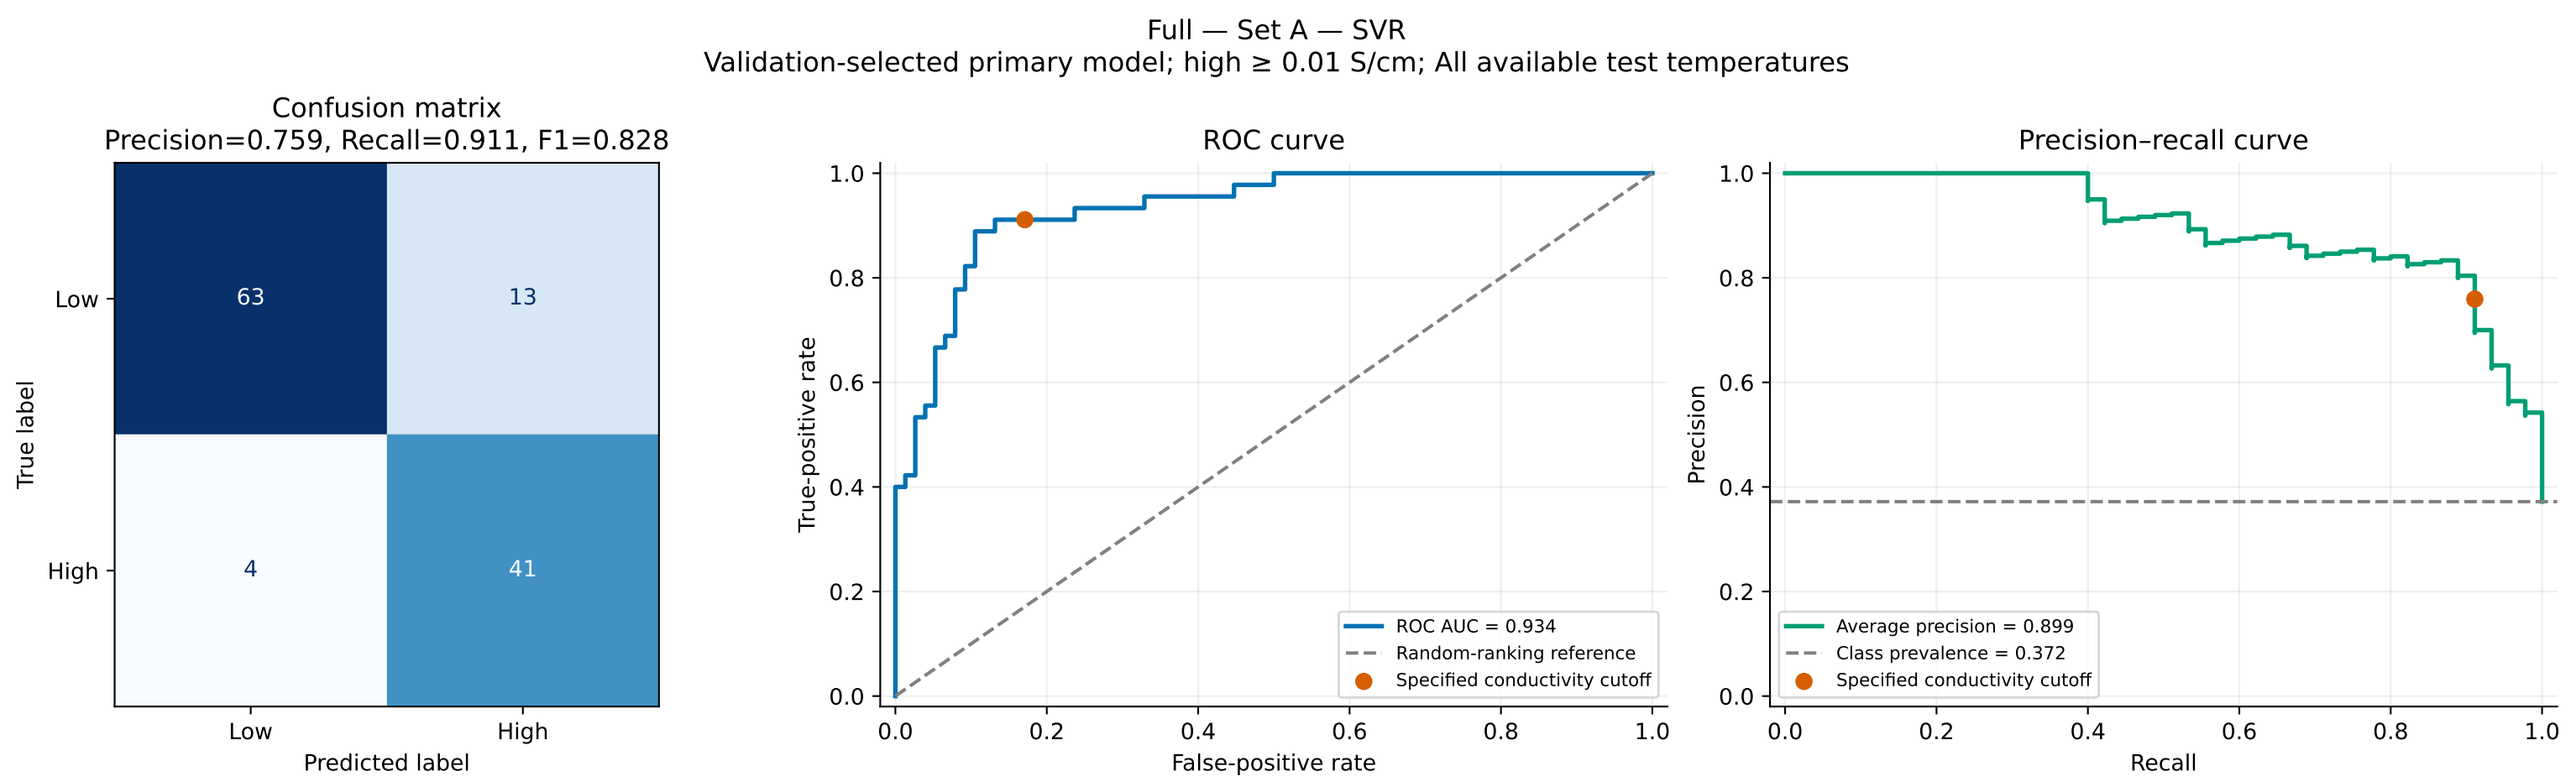
Full — Set A — SVR
Validation-selected primary model; high ≥ 0.01 S/cm; All available test temperatures
Confusion matrix
Precision=0.759, Recall=0.911, F1=0.828
63
13
4
41
Low
High
True label
Low
High
Predicted label
ROC curve
True-positive rate
False-positive rate
ROC AUC = 0.934
Random-ranking reference
Specified conductivity cutoff
Precision–recall curve
Precision
Recall
Average precision = 0.899
Class prevalence = 0.372
Specified conductivity cutoff