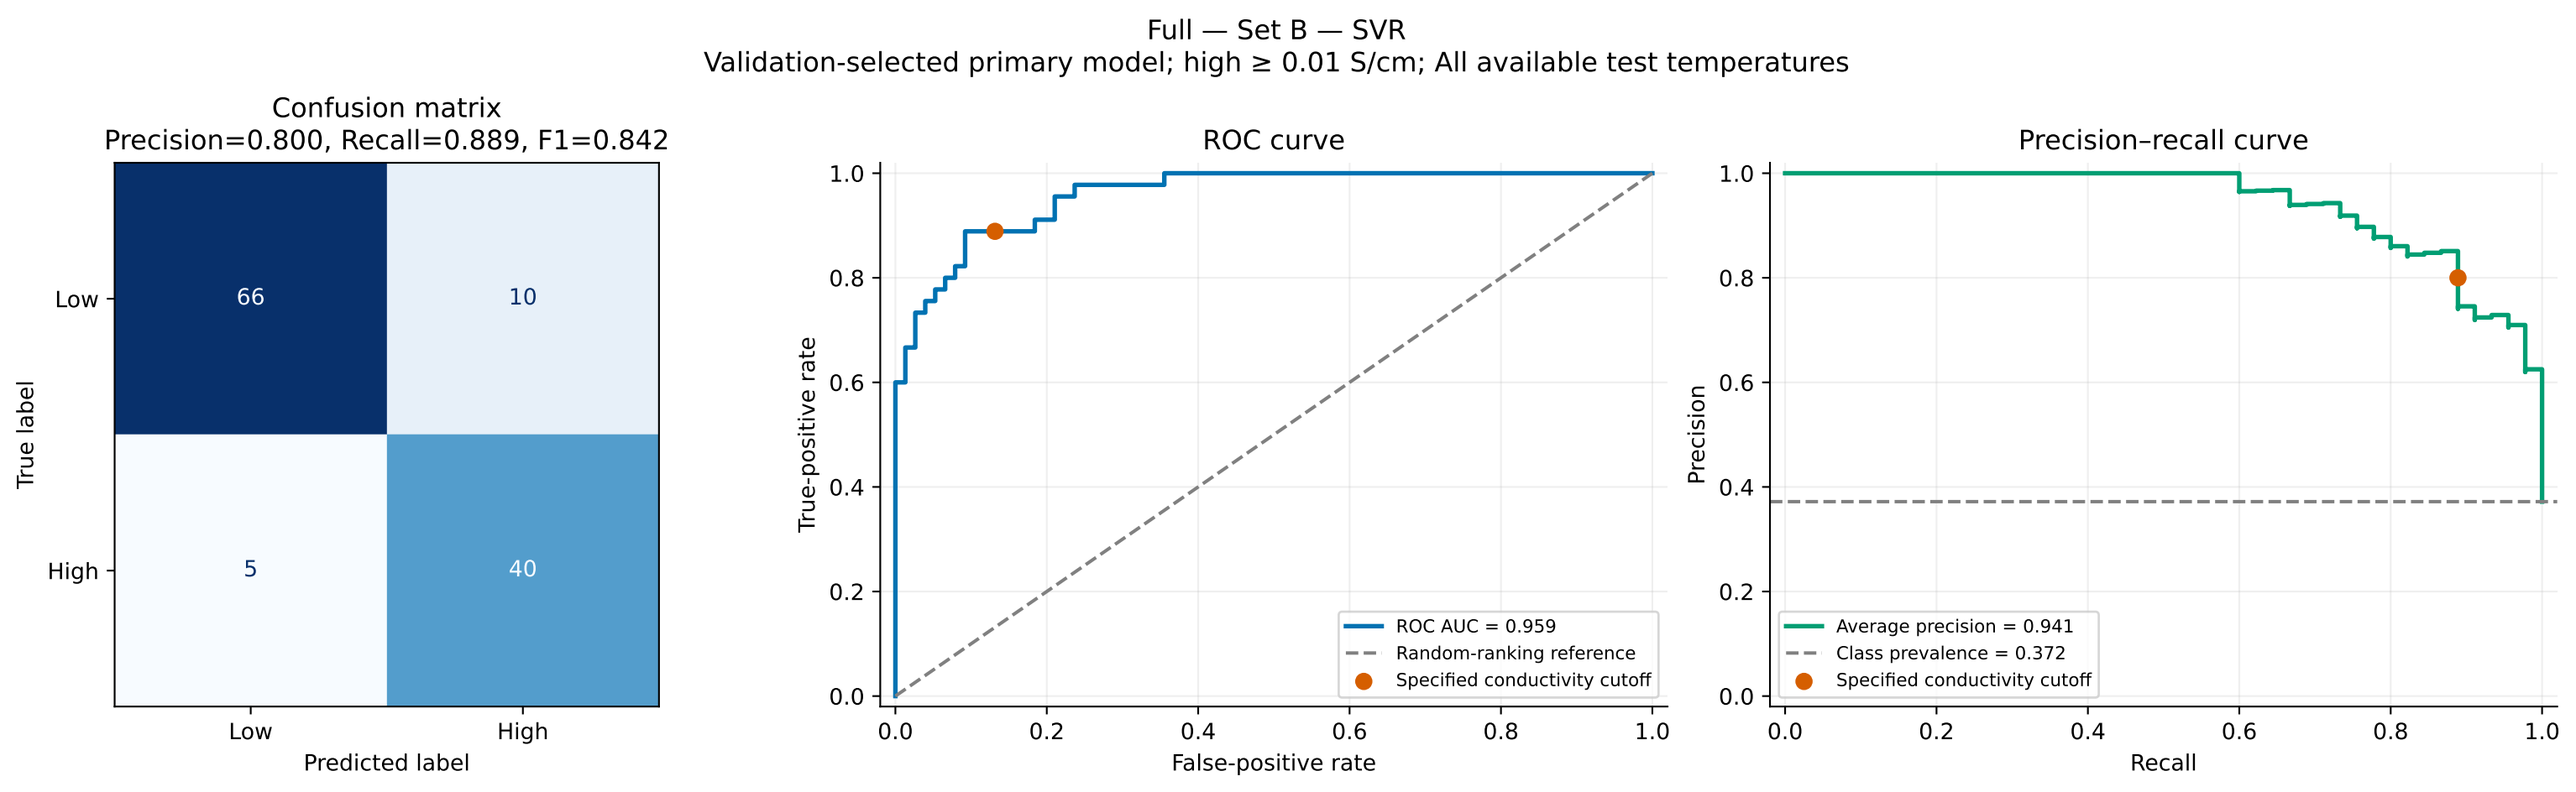
Full — Set B — SVR
Validation-selected primary model; high ≥ 0.01 S/cm; All available test temperatures
Confusion matrix
Precision=0.800, Recall=0.889, F1=0.842
66
10
5
40
Low
High
True label
Low
High
Predicted label
ROC curve
True-positive rate
False-positive rate
ROC AUC = 0.959
Random-ranking reference
Specified conductivity cutoff
Precision–recall curve
Precision
Recall
Average precision = 0.941
Class prevalence = 0.372
Specified conductivity cutoff