



Predictive Maintenance- POC

Case Study

May 25, 2026

Predictive Maintenance for Medical Equipment Failures and Alert Management

Problem Statement

Objective:

- Build a predictive maintenance system that empowers dashboards with medical equipment failure predictions and fault alert management, enabling proactive biomedical maintenance planning.

Challenges addressed:

- Unplanned downtime due to sudden medical device failures
- Lack of early visibility into equipment fault triggers and calibration drift
- Inconsistent telemetry data quality across device models and hospital sites
- Difficulty in scaling predictive models across diverse equipment fleets and modalities


Solution

- Data preparation and cleaning of device telemetry, usage logs, fault codes, and service records
- Exploratory data analysis to identify device failure patterns and critical signal features
- Iterative QA with validation metrics (WAPE, MAPE, FA) and back-testing (predicted vs actual failures)
- Deployment of the best-fit model integrated into maintenance dashboards for real-time predictive alerts


Outcome and Impact

- **Outcome:**
 - Early detection of potential device failures and fault code occurrences
 - Reduced equipment downtime and improved hospital operational continuity
- **Impact:**
 - Enhanced biomedical decision-making through predictive dashboards
 - Scalable framework that can adapt to weekly and monthly forecast horizons

Proposed Predictive Maintenance for POC - illustration

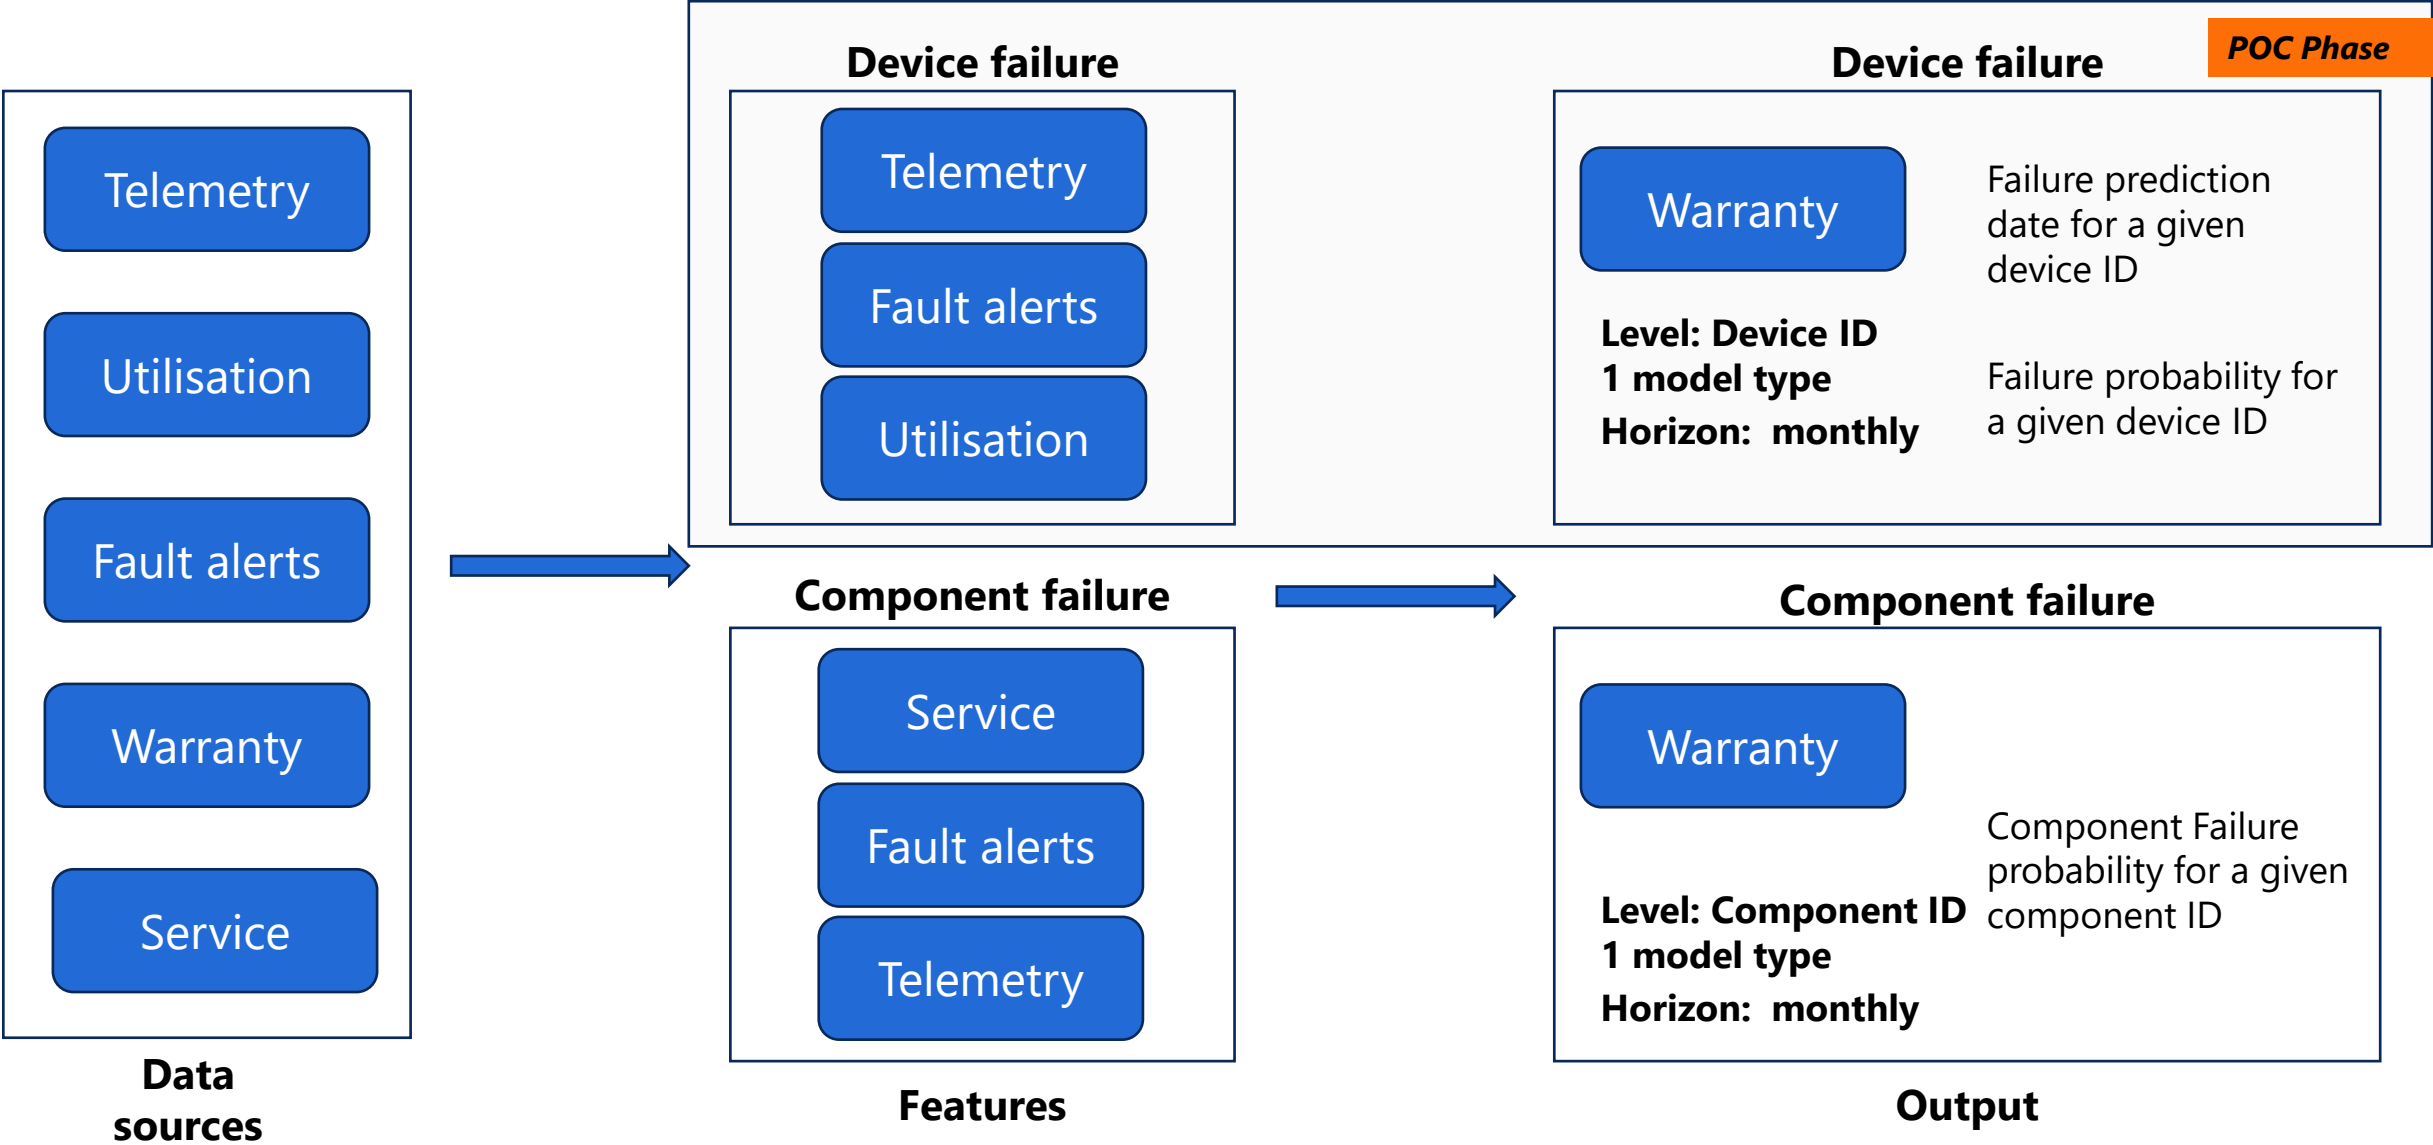

Predictive Maintenance process is devised while constantly assessing results, measuring impact, making clinical changes and providing feedback loop for improvement

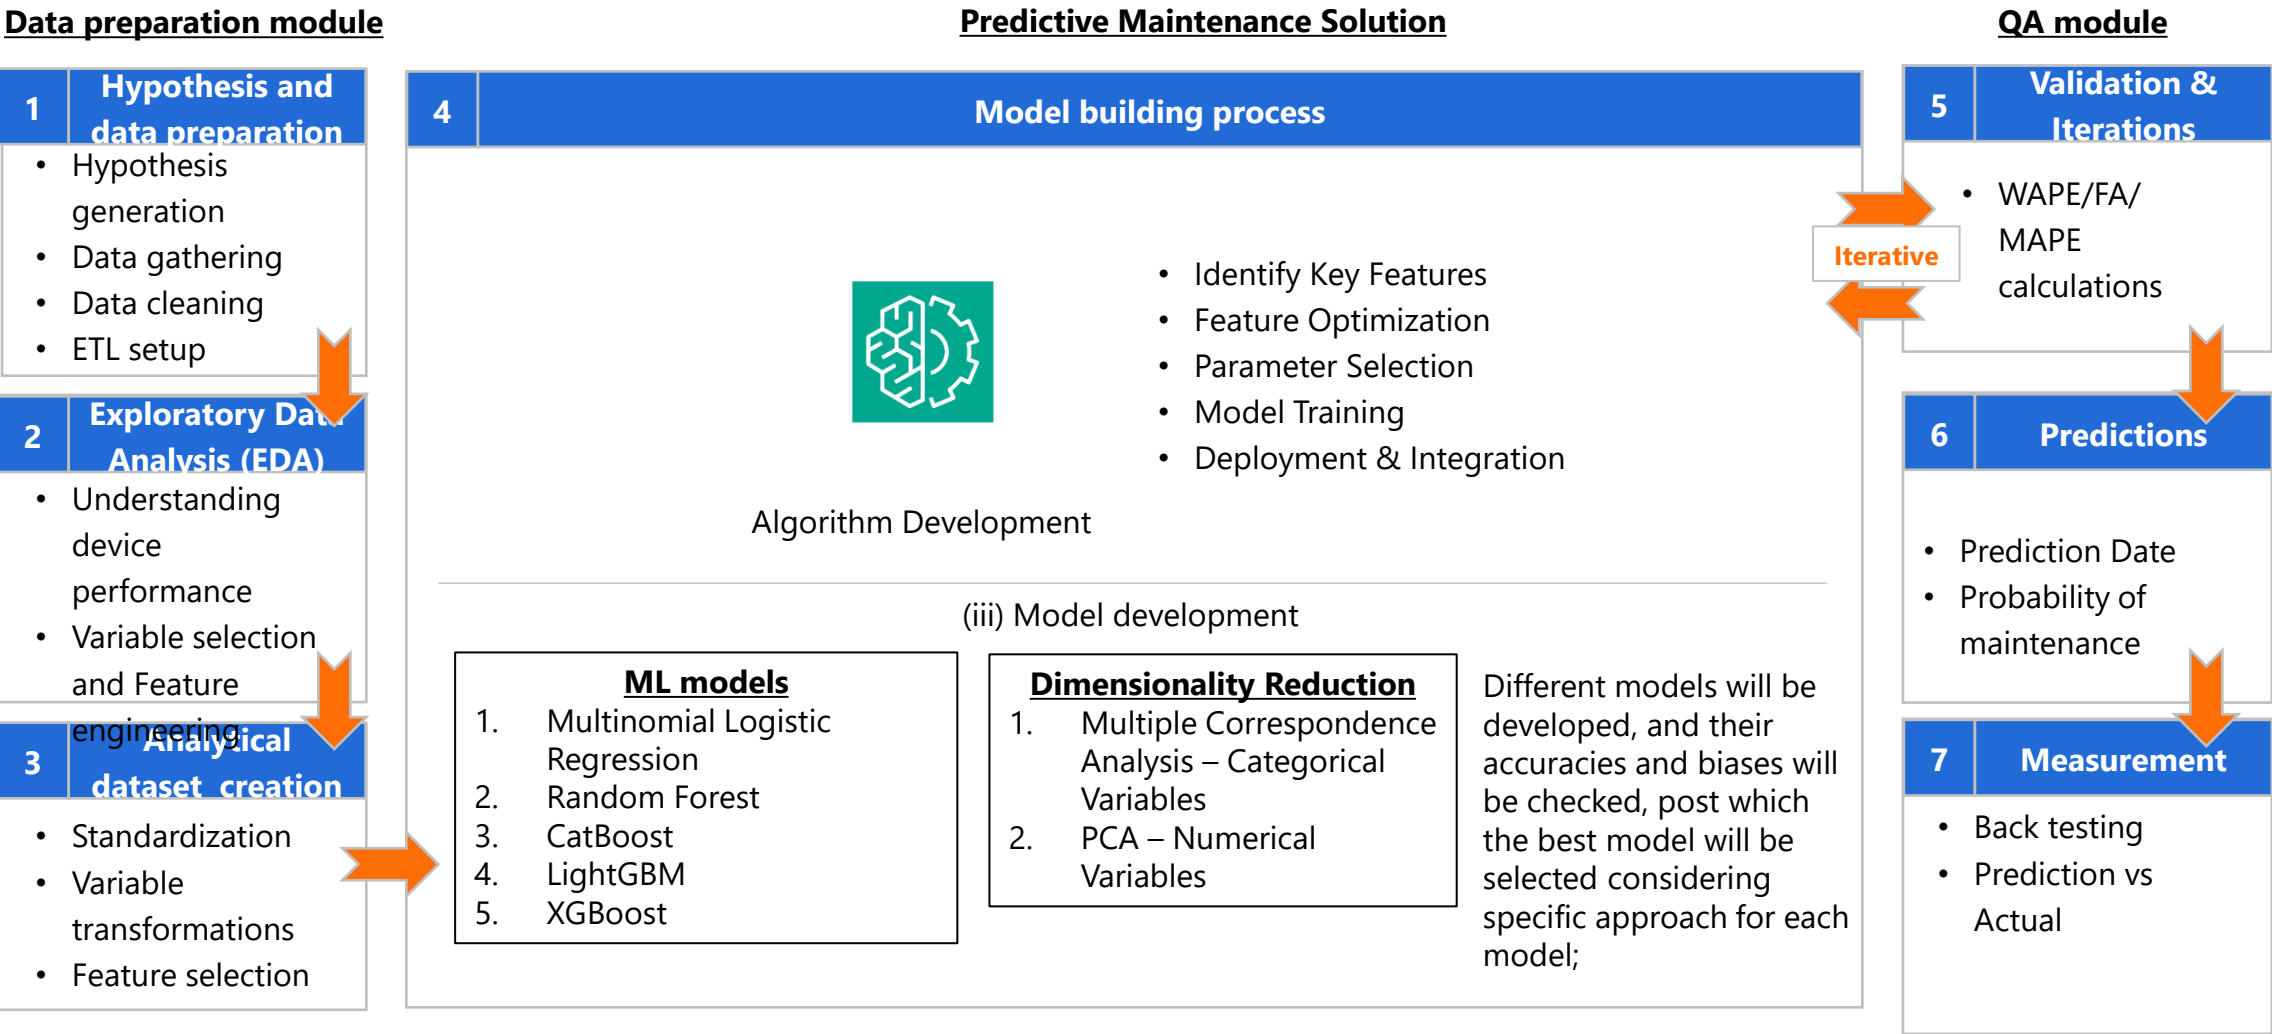

Please note: this is the generic procedure followed for Predictive Maintenance, and selective steps will be followed as applicable

The process for building weekly and monthly models remains the same while nuances, based on forecast horizon, will be captured by the algorithms

Level of predictive maintenance and the features considered for Device failure

Medical device x model (5 types) x device id	MRI Scanner
	CT Scanner
	Ultrasound System
	Patient Monitor
	Ventilator

Features

Performance	Operating Hours (Period Hrs) from utilisation data	numeric
	Scan/Procedure Time (Period in hrs)	numeric
	Idle Time Band (Period in hrs)	numeric
	Active Use Band (Period in hrs)	numeric
	Peak Load Band (Period in hrs)	numeric
	Imaging Job (Hrs.)	numeric
	Calibration Job (Hrs.)	numeric
	Maintenance Job (Hrs.)	numeric
	Emergency Job (Hrs.)	numeric

Utilization	Device Model	Categoric
	Hospital / Site	Categoric
	Modality	Categoric
	Runtime Hours (Period Hrs)	numeric

Fault Alerts	Device_Runtime_Hours	numeric
	FaultAlertGenerationTime	convert to numeric
	FaultAlertClosureTime	convert to numeric
	FaultErrorCode	Categoric

Service	Count of PM services before failure date	numeric
---------	--	---------

Thank You

Ganit provides cutting edge solutions at the intersection of hypotheses-based analytics, ML-driven AI, and new-data insights from smart devices



We have delivered tangible benefits to leading brands in the North America, Europe, MENA and APAC

info@ganitinc.com

www.ganitinc.com

Our Offices

US

Halsey Corporate Center,
90 East Halsey Road, Suite 320,
Parsippany NJ 07054

INDIA

3rd floor, Geeyam Tech Square,
No 57, Estate Main Rd, Industrial Estate,
Perungudi, Chennai, Tamil Nadu 600096

DISCLAIMER: Information contained in this document is proprietary or legally privileged information to Ganit Inc. (the Company). It is intended for the designated recipient(s) and purpose, and may contain information that is privileged, confidential or exempt from disclosure under applicable law. Access to information by anyone else is unauthorized. If you are not the intended recipient, an agent of the intended recipient or a person responsible for delivering the information to the intended recipient, you are notified that any use, copying, reproduction, dissemination, disclosure, modification, publication of this document or any information contained therein in any way or in any manner is strictly prohibited or may be unlawful. Further, if you are not the intended recipient, please notify the company immediately about mis-delivery and permanently delete this document. The recipient acknowledges that the views expressed in this document are those of sender and may not necessarily reflect those of the Company. There is no guarantee that the integrity of this document has been maintained and nor is this document free of viruses, interceptions or interference. The Company accepts no liability for damage caused by any virus transmitted in this document or error or omissions.