Turning-point refinement: comparison screens

108 stimuli per method. Green = passes every applicable screen; orange = one or more misses.

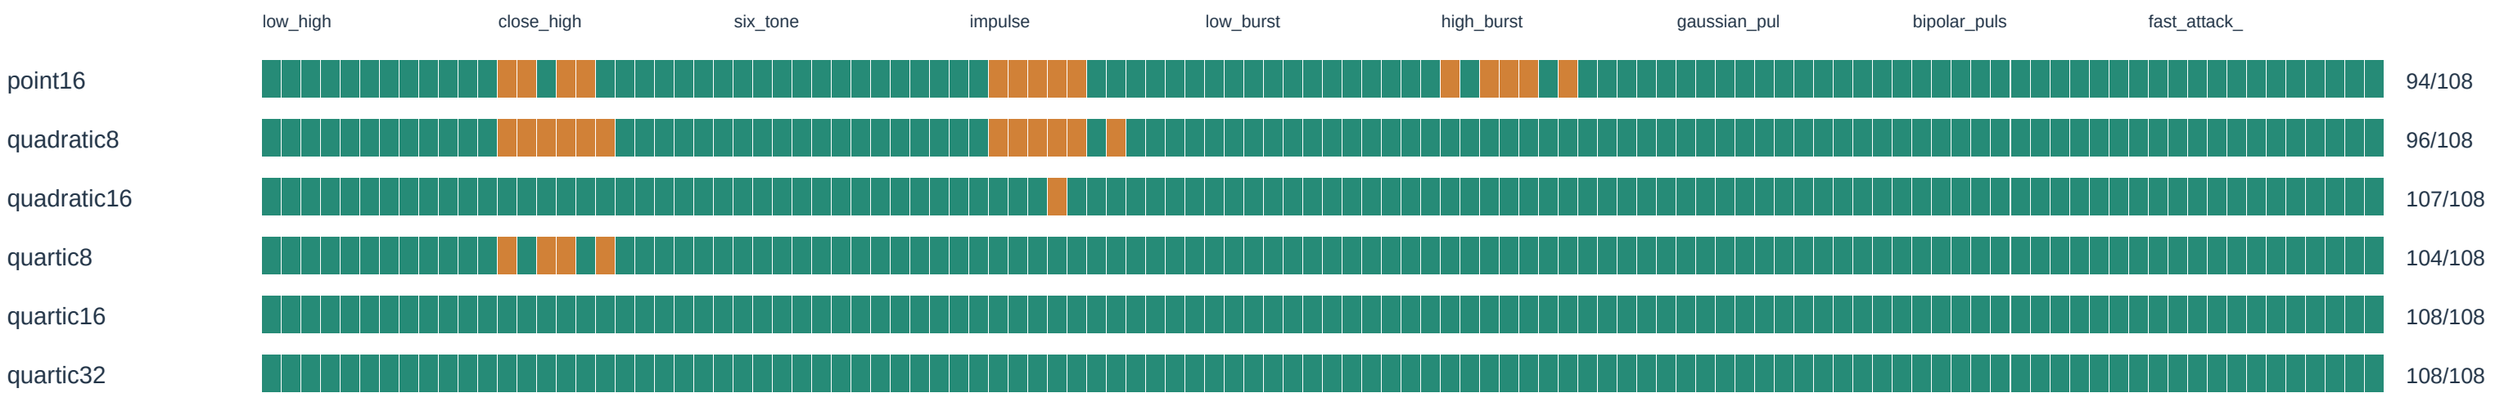

Within each signal: 44.1/48/96/192 kHz; H scales 0.05/1/4. Same independent reference and screens as validation v1.

Offline research only. A pass is numerical reference agreement over DC-20 kHz, not a calibrated transformer or audibility claim.