ElderCareAI User Guide

Installation caregiver phone app Galaxy Watch6 and administrator portal

Use this guide to install ElderCareAI, connect the patient watch, monitor recorded health information and manage everyday care. Each section identifies the screen to capture for the project report and gives operating instructions. Replace the figure spaces with screenshots from the installed system.

Install the Android app

Visit https://eldercareai-capstone.vercel.app/ and choose Install or try the app. Best with Galaxy Watch6 and the separate watch companion.

Before taking screenshots

- Use one intended caregiver and patient account throughout the demonstration.
- Hide personal names, phone numbers, prescriptions and exact home coordinates.
- Use real demonstration records and show their original timestamps.
- Wearable readings and Elle suggestions support care review and do not provide medical diagnoses.

1 Download ElderCareAI

Screen: Android phone browser

What to screenshot: Capture the website installation section and Google Drive APK download.

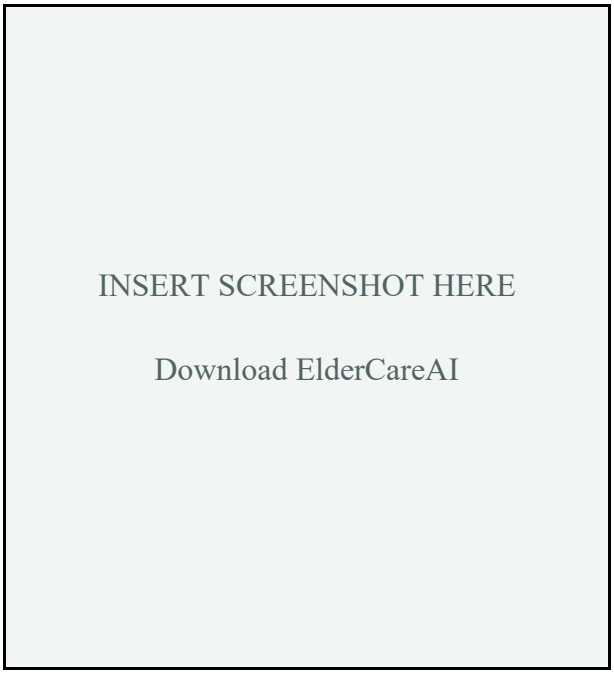


Figure 1: Download ElderCareAI

1. On the Android phone, open https://eldercareai-capstone.vercel.app/ and select Install or try the app.
2. Choose Download Android APK. The supplied APK is shared through Google Drive; use its Download action and wait for the file to finish downloading.
3. If Drive requests access, contact the project team to enable link access. Do not substitute an APK from an unrelated source.
4. ElderCareAI is designed for an Android phone and works best with Galaxy Watch6. The caregiver website and administrator portal do not replace the phone or watch app.
5. Keep the phone connected to the internet for Google sign-in, shared records and notifications.

2 Install or update the phone app

Screen: Android Downloads and installer

What to screenshot: Capture the APK Install or Update screen and the ElderCareAI launcher icon.

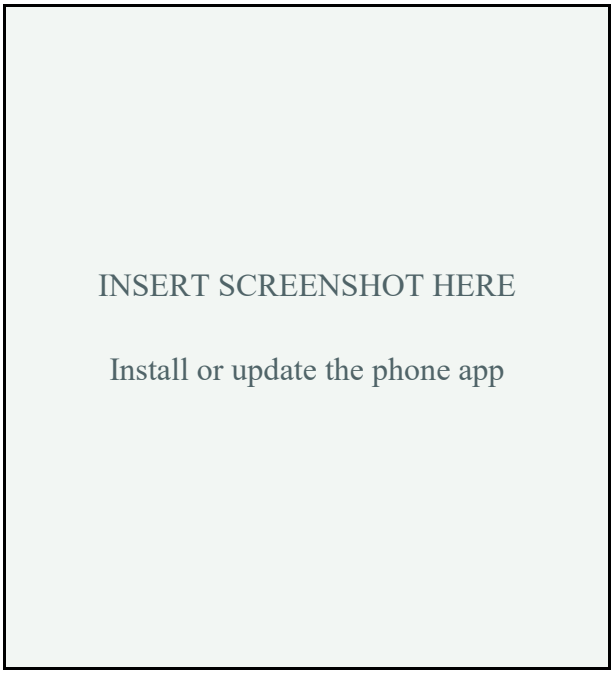


Figure 2: Install or update the phone app

1. Open the downloaded APK from the browser downloads or the phone Files app.
2. If Android blocks installation from that source, open the displayed Settings link and temporarily allow that browser or file manager to install unknown apps.
3. Return to the installer and choose Install, or Update when a compatible ElderCareAI installation already exists. Open the app after completion.
4. If an update reports incompatible signatures, contact the project team for an APK signed with the original key. Keep the existing app until the mismatch is resolved.
5. After installation, turn off the temporary install permission if it is no longer needed. Allow requested app notifications when setting up alerts.

3 Prepare the Galaxy Watch6

Screen: Galaxy Wearable and watch settings

What to screenshot: Capture Galaxy Watch6 pairing and the watch app launcher.

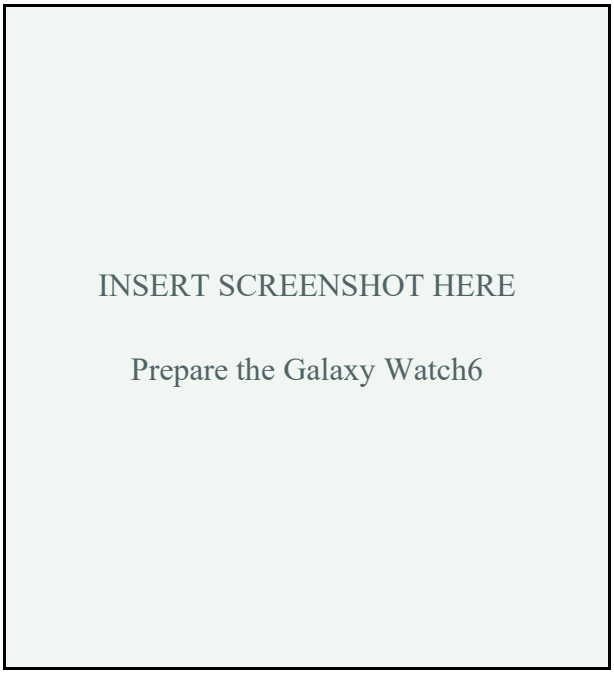


Figure 3: Prepare the Galaxy Watch6

1. Pair Galaxy Watch6 to the Android phone using Galaxy Wearable. For sleep history, use this same patient watch and Samsung Health on this phone.
2. Install the separate ElderCareAI Wear OS companion. The Android phone APK cannot be installed as the watch companion; obtain the watch APK from the project team.
3. For developer installation, enable watch Developer options and Wireless debugging. On the computer use Android platform-tools: adb pair WATCH_IP:PAIRING_PORT and enter the watch pairing code.
4. Then run adb connect WATCH_IP:CONNECTION_PORT and adb -s WATCH_IP:CONNECTION_PORT install -r WATCH_APK_PATH. Use the main debugging screen connection port and the actual Wear OS APK path.
5. After installation, open ElderCareAI on the watch. Wireless debugging can be disabled; normal use requires app permissions and internet, not debugging.

4 Allow monitoring and notifications

Screen: Phone and watch permission settings

What to screenshot: Capture granted watch permissions and phone background notification status.

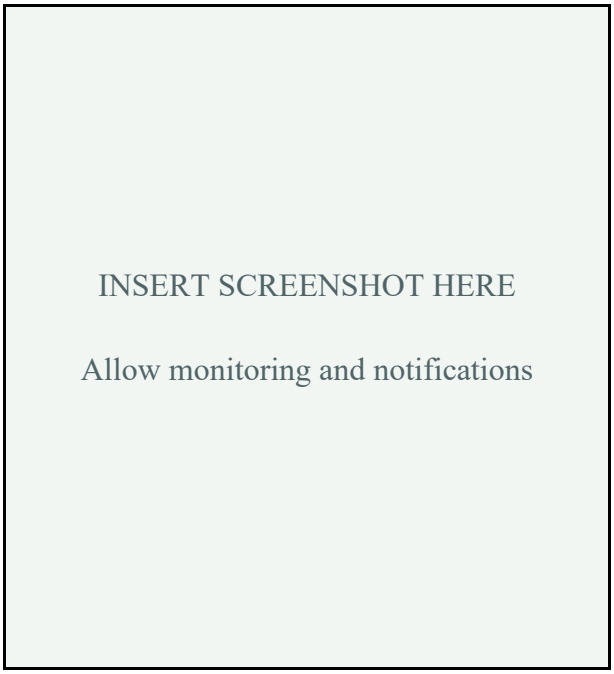


Figure 4: Allow monitoring and notifications

1. On the watch enable Location and grant ElderCareAI its requested sensor, physical activity, precise location and notification permissions.
2. Keep Wi-Fi or supported LTE available when the watch wearer leaves the paired phone. Bluetooth alone does not provide standalone internet outside phone range.
3. In the phone app open Alerts, tap Enable background notifications and allow Android notifications. Confirm alert channels have sound enabled and notification volume is audible.
4. For watch medication reminders, allow alarms and reminders through the watch reminder-timing settings when requested. Keep device time and timezone automatic.
5. For developer sensor builds, follow the supplied Samsung Health Sensor SDK test-mode setup if sensor access is denied. Pair the app and tap Start monitoring to verify real values.

5 Sign in

Screen: Phone app opening screen

What to screenshot: Capture the Google sign-in button and app name.

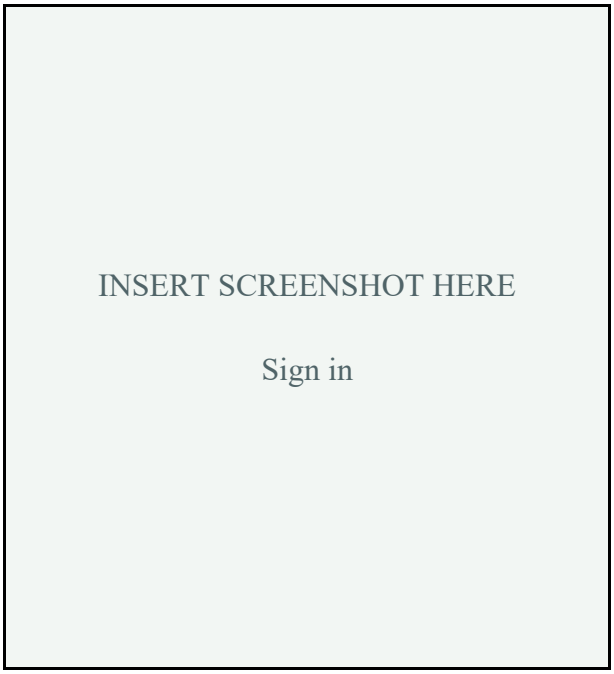


Figure 5: Sign in

1. Open ElderCareAI and tap Sign in with Google. Choose the caregiver account responsible for this patient.
2. Complete Google's account selection. If cancelled or unsuccessful, return to sign in and retry with internet available.
3. On first use, follow caregiver and patient setup. A returning account restores its saved setup and patient context.
4. Check the patient name on Home before viewing or recording care. Sign out through Profile before using another account.
5. Conceal the account email in screenshots. A saved session may bypass sign in on subsequent launches.

6 Caregiver and patient setup

Screen: First sign-in onboarding

What to screenshot: Capture the caregiver profile and patient profile screens separately.

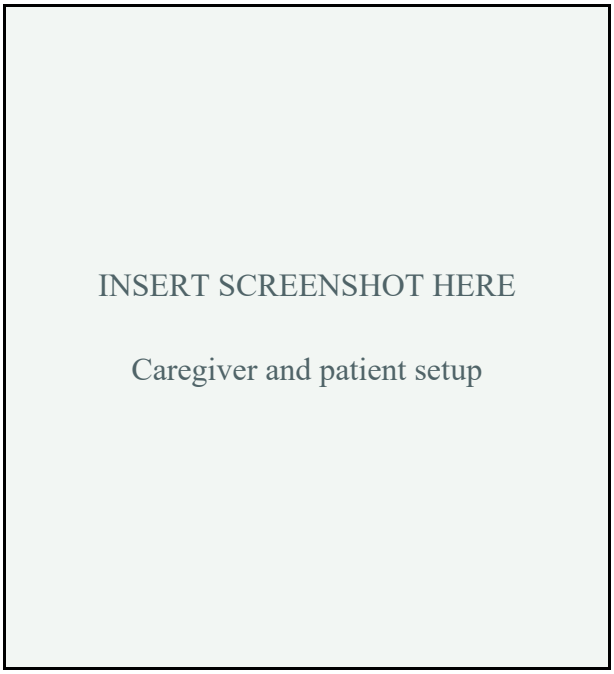


Figure 6: Caregiver and patient setup

1. Enter the caregiver name, contact number, age and gender; the signed-in email identifies the account. Add a photo if desired.
2. Continue to the patient form and enter the older adult's name, birth date or age, gender, and the requested health details.
3. Add weight, height, blood type, known conditions and current medications when available. Use the displayed units.
4. Enter the emergency contact details and save. Correct any highlighted invalid field before continuing.
5. Patient selection controls the vitals, sleep, care plan, location and alerts displayed. Confirm the correct patient after changing accounts.

7 Connect Galaxy Watch6

Screen: Profile or setup watch integration

What to screenshot: Capture Connect or change watch and the paired device status.

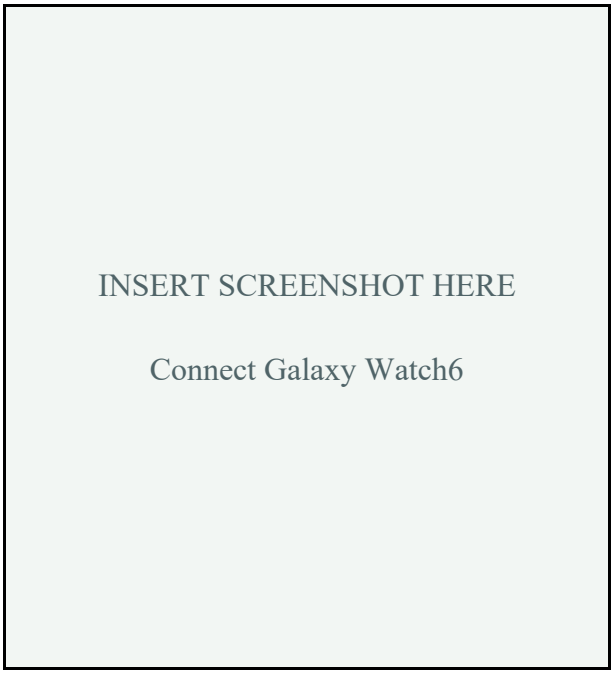


Figure 7: Connect Galaxy Watch6

1. Open Profile and choose Connect or change watch, or continue from watch setup during onboarding.
2. Generate the eight-digit pairing code for the intended patient. Open ElderCareAI on the watch and enter that code.
3. Tap Pair watch and wait for confirmation. An invalid or expired code requires a new code; network errors require a working connection.
4. Confirm the phone shows Galaxy Watch6 connected. This app pairing is separate from Galaxy Wearable's Bluetooth pairing.
5. Allow watch sensor, activity, location and notification permissions, then start monitoring. Pair the watch again when intentionally assigning it to a different patient.

8 Watch monitoring

Screen: ElderCareAI on the watch

What to screenshot: Capture Start monitoring or Stop monitoring, current readings, Location and sharing status.

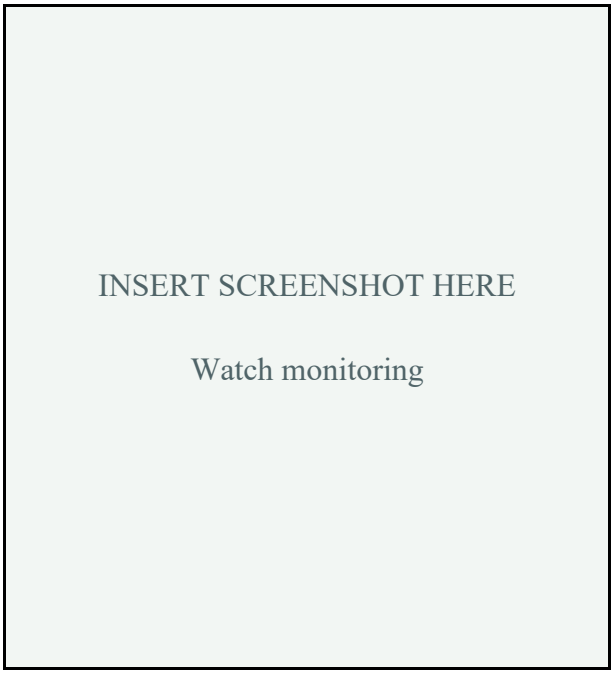


Figure 8: Watch monitoring

1. Open ElderCareAI on the paired Galaxy Watch6 and tap Start monitoring. Allow requested permissions and keep the watch snug on the wrist.
2. Heart rate, skin temperature, steps and HRV update when usable sensor events arrive. HRV needs a sustained interval of valid beat data and may restart after poor contact.
3. Location starts with monitoring. Enable Location and internet; move outdoors for better satellite reception. GPS, fused and network estimates retain source and accuracy labels.
4. Open Measure blood oxygen for a manual spot check. Keep the arm still. Optional five-minute auto checks work only while that screen stays open.
5. Inspect sharing status and queued samples. Offline vital measurements retry when connected. Tap Stop monitoring to end monitoring; restart it after a watch reboot or force stop.

9 Caregiver dashboard

Screen: Home tab

What to screenshot: Capture live vital cards with visible values, labels and measurement times.

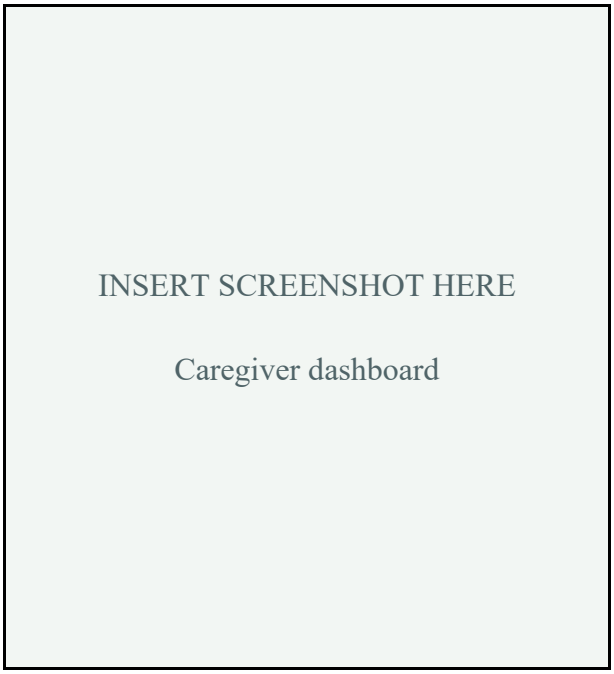


Figure 9: Caregiver dashboard

1. The dashboard summarizes the selected patient. Each vital displays its latest available reading and a text status.
2. A fresh heart-rate update can change the display label without reopening the screen. The alert rule remains above 110 BPM.
3. A waiting or stale label means a fresh measurement is unavailable; it is not a normal reading.
4. Tap Sync now or pull to refresh when needed. A failed refresh should not be mistaken for a new measurement.
5. Tap a vital card for detail or a care task to open its relevant Care plan screen.

10 Vital signs

Screen: Health tab Vitals

What to screenshot: Capture heart rate, oxygen, sleep, steps, skin temperature and stress if present.

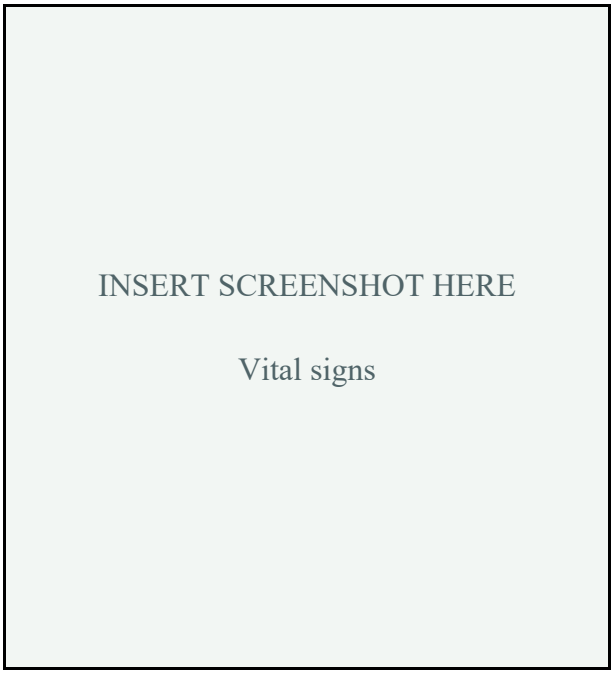


Figure 10: Vital signs

1. Open Health and select Vitals. Review Heart Rate, Blood Oxygen, Skin Temperature, Stress level, Sleep and Steps.
2. Each available card shows a value, unit, status and measurement time. A status can change with a new reading; missing or stale values are not normal readings.
3. Heart rate, wrist temperature and valid HRV come from watch monitoring. Steps count the increments collected during monitoring on that watch day.
4. Blood oxygen uses spot measurements or available imported history. Sleep appears after Samsung Health records and synchronizes the patient's session.
5. Stress is an experimental HRV-based index. It needs a personal reference before a score is available and is not a medical diagnosis.

11 Vital detail and history

Screen: Tap a vital card

What to screenshot: Capture one vital detail with its dated reading and status explanation.

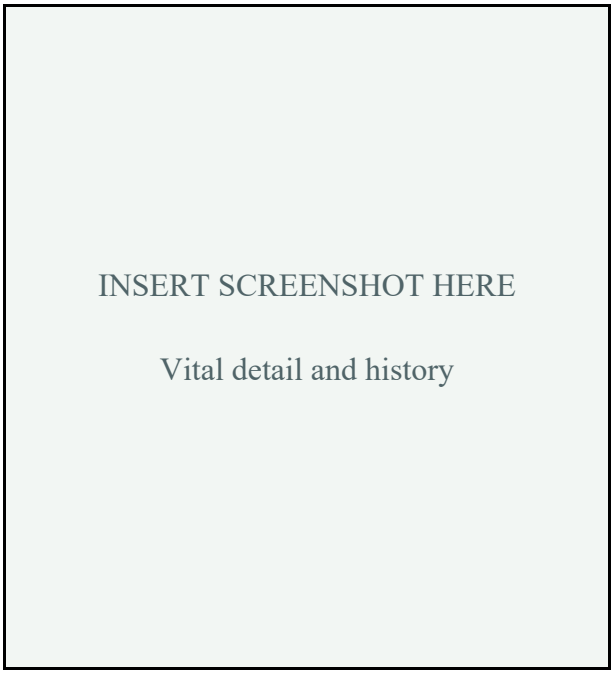


Figure 11: Vital detail and history

1. Tap any vital card to open its details. Read the latest value, status and original measurement time.
2. Scroll to Elle insight. Its observation remains steady while the live value above continues updating.
3. When New readings available appears, tap Refresh insight when ready. The Reading reviewed timestamp identifies the observation's reference reading.
4. Review recent measured history or nightly sleep entries, source details and the explanation below the card.
5. If the insight request fails, use Retry insight. Interpret status labels and wellness suggestions as review guidance; confirm concerns with an appropriate professional.

12 Health analytics

Screen: Health tab Analytics

What to screenshot: Capture the date filter, line chart, bar chart and a selected timestamp.

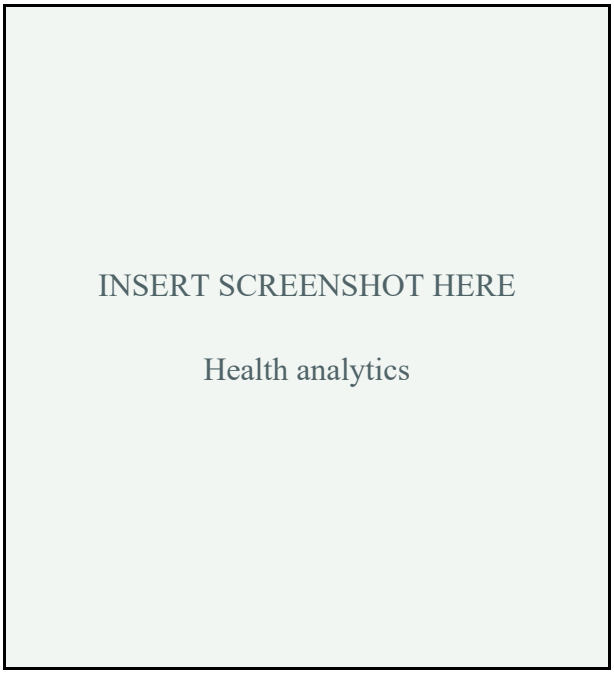


Figure 12: Health analytics

1. Choose a metric and date range. The chart uses saved database readings for the selected patient.
2. Switch between line and thin bar views. Inspect a point to see its original value and measurement time.
3. Daily steps show a day total rather than adding cumulative samples together.
4. Use actual measurement timestamps to distinguish delayed uploads from newly measured values.
5. If the range is empty, choose a date with saved readings. Retry a failed load instead of assuming a zero value.

13 Health history sync

Screen: Profile or Settings Health History

What to screenshot: Capture the sync status and one saved sleep history entry.

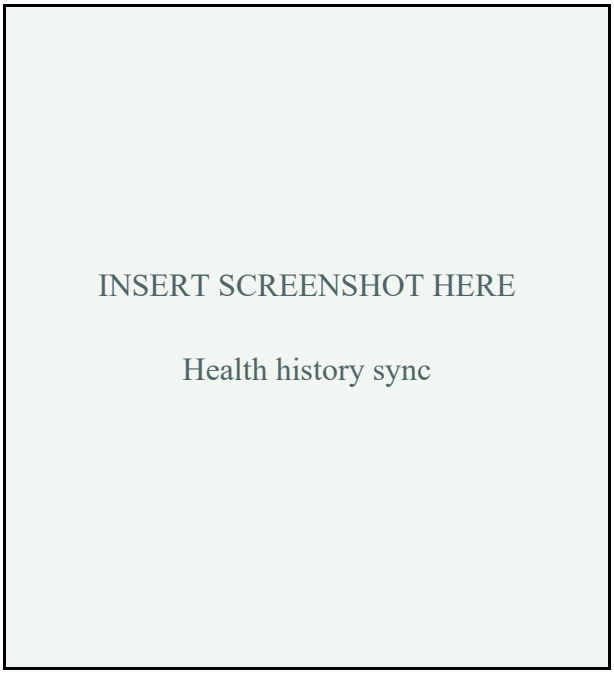


Figure 13: Health history sync

1. On the same Android phone paired to the patient's watch, install and open Samsung Health and allow its watch synchronization.
2. In ElderCareAI Profile, open Health History and connect the history import. Grant the requested access when prompted.
3. Tap Sync health history after a recorded sleep session is available. Importing sleep is different from live watch sensor monitoring.
4. Check the sync result and Sleep card history. No new data means no additional source records; previously saved patient history should remain available.
5. If access or upload fails, check internet and Samsung Health permissions and retry. Developer installations may need Samsung Health Data SDK developer access. Background checks depend on Android scheduling; wake-up delivery is not immediate.

14 Live location and safe zone

Screen: Live location tracking

What to screenshot: Capture the watch marker, accuracy or source label, and safe-zone circle.



Figure 14: Live location and safe zone

1. On the watch, tap Start monitoring with Location and internet enabled. Open Live location tracking on the phone; no separate walking mode is needed.
2. Read the marker's source, measurement age and accuracy. The displayed stream can contain watch GPS, fused and network estimates; fused location may represent the paired phone.
3. Open Set up safe zone or Edit safe zone. Enter a place name, tap Choose on map and tap the actual home center, including inside the circle or on the marker.
4. Choose a radius from 10 to 5,000 meters, then Save and enable safe zone. Use current location can copy a fresh usable estimate; the saved center stays fixed.
5. An estimated exit uses 3 qualifying outside updates spanning at least 20 seconds. For a 10 or 20 m zone, reported accuracy must be 50 m or better. Larger-zone limits rise to at most 100 m.
6. GPS, fused and network can all confirm the marker-based crossing. Very inaccurate or stale estimates cannot. Read confirmation progress and the source-labelled alert; small-zone false alarms are possible.
7. Keep the zone enabled and allow background notifications. Walk outside within internet coverage and inspect Alerts. Pan to explore or tap Follow location to return; Pause alerts disables boundary checks.

15 Medication list

Screen: Care plan Medications

What to screenshot: Capture one medication card showing image, 12-hour time and Taken status.

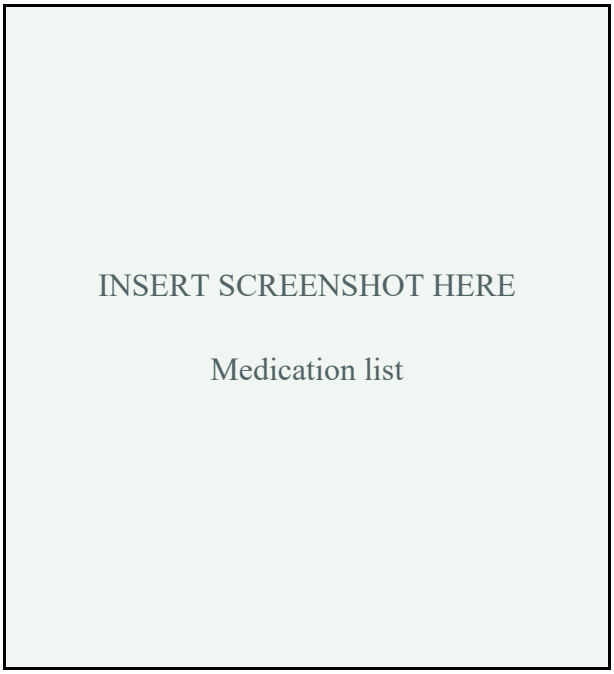


Figure 15: Medication list

1. Open Care plan then Medications. Tap Add to enter name, dosage, frequency and instructions from the verified prescription.
2. Choose an optional medication photo and review its preview. Without a photo the card uses its placeholder.
3. Select start and end dates and each reminder time. Displayed times use AM or PM; verify the device's local date and timezone before saving.
4. Save and check the medication card. Use Edit to correct the schedule; confirm Delete to remove it and cancel applicable reminders.
5. Tap Taken only after the dose was taken, and select the corresponding dose when asked. Watch confirmations also update the phone after successful sync; pending offline confirmations are not yet saved.

16 Prescription draft with Elle

Screen: Care plan Scan or upload prescription

What to screenshot: Capture the Elle entry card and the editable extracted draft.

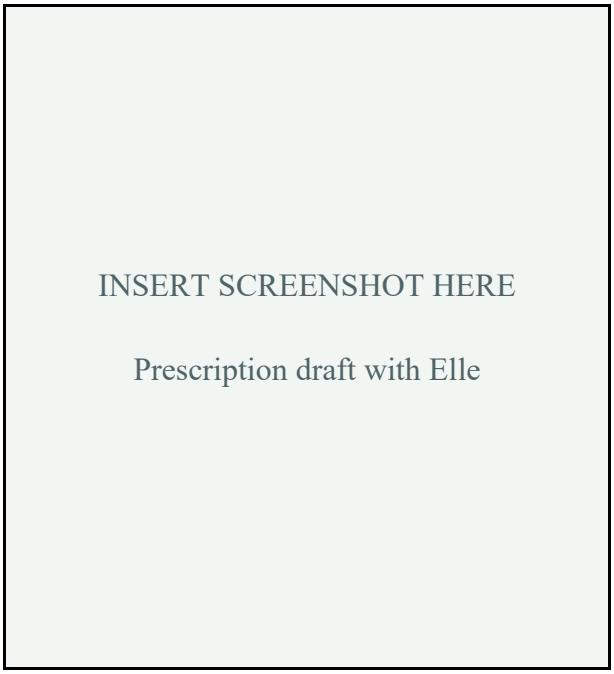


Figure 16: Prescription draft with Elle

1. Tap Scan or upload a prescription in Care plan. Choose a clear image or capture the original with the camera.
2. Wait for Elle to prepare an editable draft. If extraction fails or handwriting is unclear, retry with a clearer image or enter the medication manually.
3. Compare every extracted name, dosage, frequency, time, instruction, date and prescriber against the original. Correct mistakes and complete missing information.
4. Check the review confirmation only after verification. AI extraction does not prescribe medication or verify the doctor's instruction.
5. Confirm and save medication. Check the resulting medication card, schedule and reminder times; unconfirmed drafts do not activate a schedule.

17 Appointments

Screen: Care plan Appointments

What to screenshot: Capture a saved upcoming appointment showing patient, purpose, date and time.

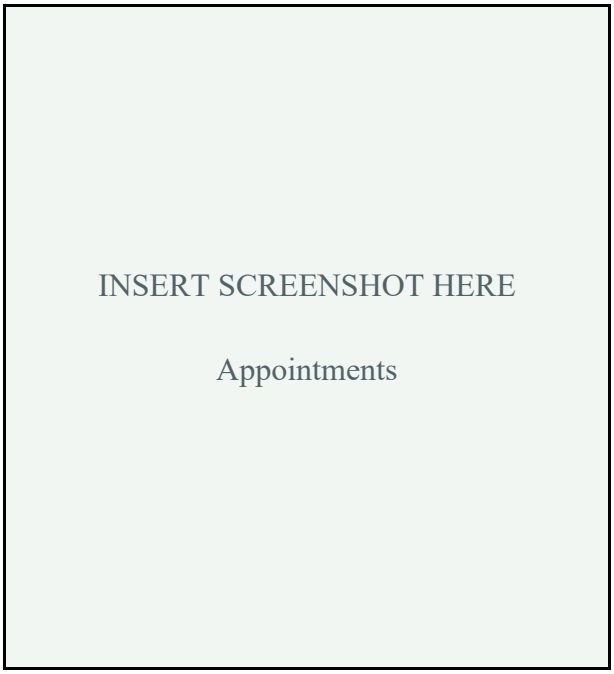


Figure 17: Appointments

1. Open Care plan then Appointments. Tap Add and enter the purpose or title, appointment date and local time.
2. Add doctor name, location and notes if known. Save, correcting any invalid field while keeping the draft available.
3. Review the saved visit. Appointment reminders are prepared ahead of the visit; the server schedule uses a 15-minute advance, so create a test visit at least 20 minutes ahead.
4. Enable background notifications and check phone time and internet. A reminder is not proof the appointment has started or been attended.
5. Use Edit to reschedule, Complete after attendance, or confirm Delete when cancelled. The list and combined schedule refresh after the change.

18 Care schedule

Screen: Care plan Schedule

What to screenshot: Capture two scheduled items in chronological order.

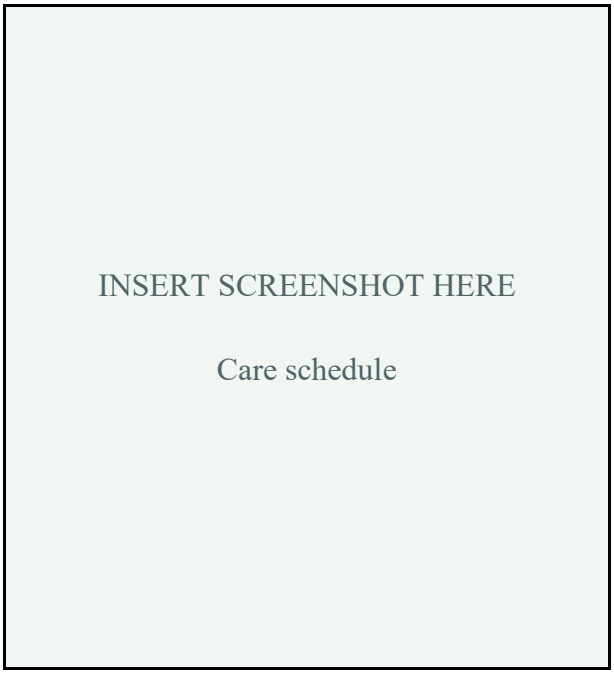


Figure 18: Care schedule

1. Open Schedule to review medications and appointments together. Items on the same day sort by their actual time.
2. Completed activities have a different status from upcoming activities.
3. When two reminders share one time, dismiss the first popup and capture the second popup separately.
4. Reschedule a visit or edit a dose time and reopen Schedule to check its new chronological position.
5. For simultaneous reminders, verify both separate items remain visible and capture both popups after dismissing each in turn.

19 Alerts and notifications

Screen: Alerts tab

What to screenshot: Capture collapsed Automatic vital alerts, SOS action, and one dated notification.

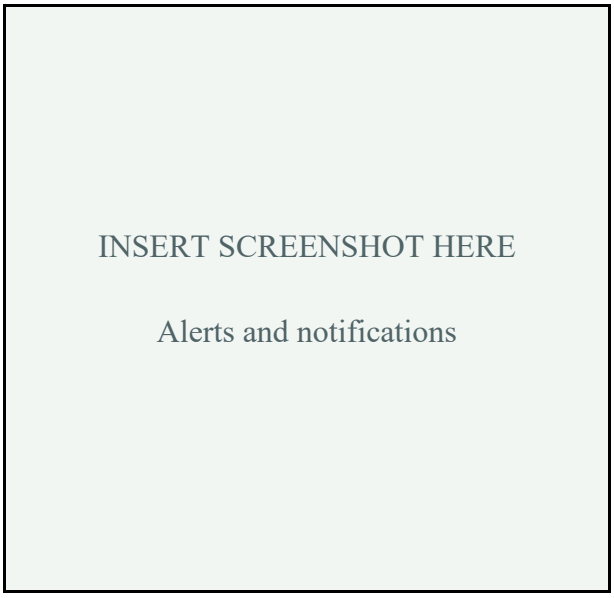


Figure 19: Alerts and notifications

1. Open Alerts and expand Automatic vital alerts to review the configured rules; collapse it to leave emergency actions visible.
2. A qualifying measured crossing saves a patient alert. The high-heart-rate warning starts above 110 BPM, rather than at 100 or exactly 110 BPM.
3. Open Notifications for medication, appointment and other notices. Review the timestamp and related details before acting.
4. Tap Enable background notifications and allow Android permission. Sound also needs the relevant channel enabled, audible volume and suitable Do Not Disturb settings.
5. When multiple alerts arrive together, dismiss or open the current popup to review the next queued popup. A linked-medication action is shown only when a relevant medication is associated.
6. Push can work when the app is backgrounded or normally closed; Android force-stop and device restrictions can prevent delivery until the app is opened again.

20 Emergency contacts and SOS

Screen: Alerts and Settings

What to screenshot: Capture contact order with numbers covered, plus the emergency action.

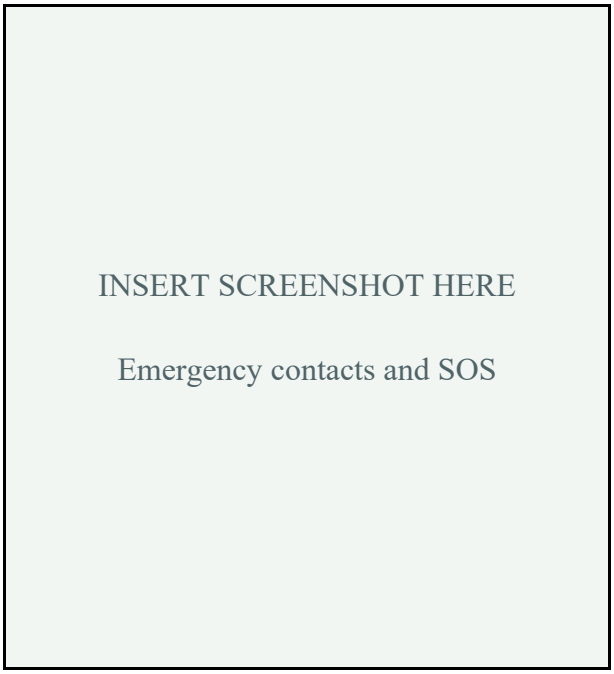


Figure 20: Emergency contacts and SOS

1. Save the caregiver, family member and doctor names and telephone numbers in Settings or the emergency-contact editor.
2. Open the emergency contact list. The order is caregiver first, family member second and doctor third.
3. Select a contact to open the supported phone dial action. Confirm the number before making the call.
4. On the watch, open SOS and tap Send SOS deliberately. Check for a successful send or a pending/error message; merely opening the screen does not send it.
5. Review the saved SOS in the phone Emergency tab, then acknowledge or respond through the alert actions. An SOS does not automatically call emergency services.

21 Elle assistant

Screen: Elle tab

What to screenshot: Capture a non-identifying question and its answer.

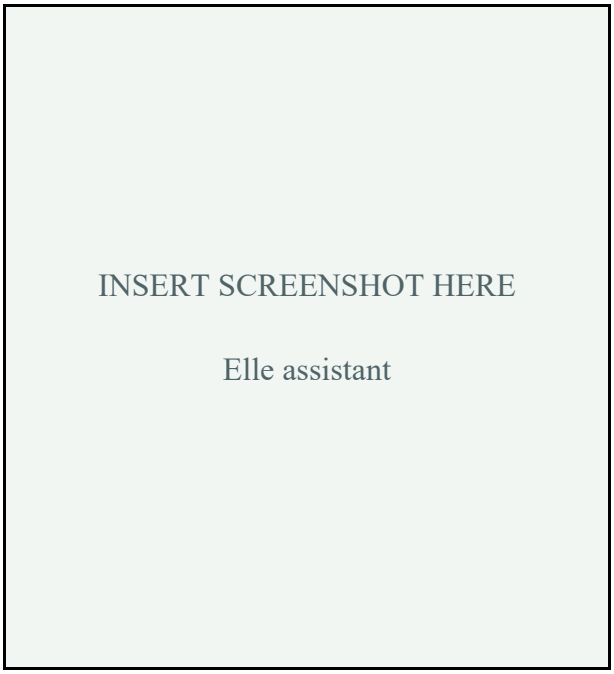


Figure 21: Elle assistant

1. Ask Elle about an existing saved record, such as a dated heart-rate reading, medication or health trend.
2. Check that the response is grounded in available patient data. Elle should not invent readings or diagnose illness.
3. For a report screenshot, use a demonstration question without private patient details.
4. Wait for the thinking indicator to finish. If a service error appears, retry while connected.
5. Use related-screen actions or evidence links when offered. Start New Chat for a separate question.

22 Settings and exports

Screen: Profile or Settings

What to screenshot: Capture watch integration, background notifications and PDF export options.

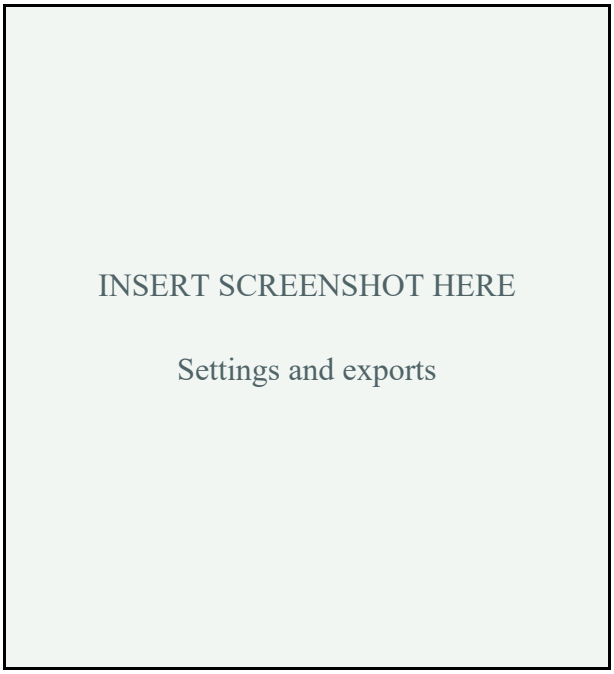


Figure 22: Settings and exports

1. Open Profile to review the active caregiver, patient and Galaxy Watch6 connection. Edit the relevant profile or emergency contacts as needed.
2. Use Health History to connect and import recorded sleep and supported overnight oxygen. Keep the patient's paired-watch identity correct.
3. Select Health vitals PDF or Medication schedule PDF. The export uses saved records for the selected patient and opens the supported sharing options.
4. If a required record is missing or an export fails, check patient selection, connectivity and the displayed message before retrying.
5. Enable background notifications from Alerts. Sign out before switching caregiver accounts and check the restored patient after the next sign-in.

23 Administrator overview and accounts

Screen: Web administrator portal

What to screenshot: Capture Overview, then Manage accounts with identifying fields covered.

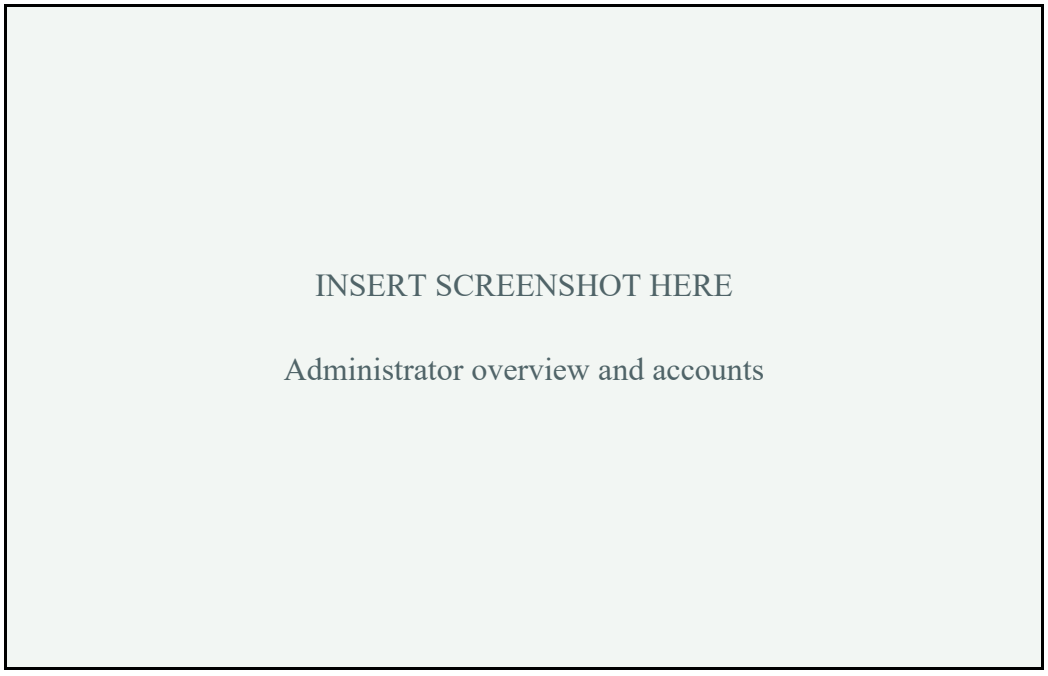


Figure 23: Administrator overview and accounts

1. Open the website's administrator portal and sign in with an authorized administrator username or email and password.
2. If sign-in fails, correct the credentials; use Forgot password and follow its verification steps when recovery is needed.
3. Overview displays saved system counts, recent alerts and emergency activity. Refresh to request updated administration data.
4. In Accounts select a caregiver and review the linked patients. Use permitted editing and access controls and read each confirmation before saving a change.
5. Use Install or try the app on the public landing page to open the Android APK and installation instructions. The caregiver phone app uses its own Google sign-in.

24 Administrator monitoring and reports

Screen: Web administrator portal

What to screenshot: Capture System monitor, Alerts and notifications, and Generate reports.

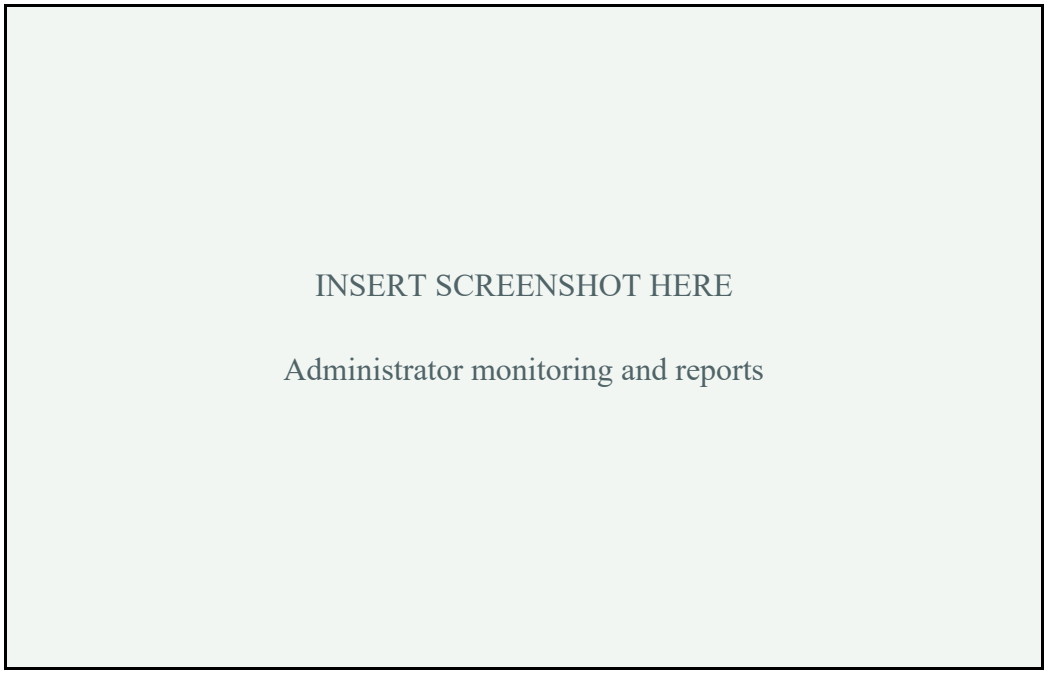


Figure 24: Administrator monitoring and reports

1. Open System monitor to inspect reported connection state and recent database health syncs. This is not a live watch sensor display.
2. Distinguish Saved at, the database write time, from Measured at, the original measurement time. Older saved readings do not establish current sensor activity.
3. Open Alerts and notifications to review saved warnings and emergency history, including status and delivery information.
4. Open Reports, choose report type and date range, then generate the available CSV. Review empty results and errors before retrying.
5. Use Security for supported administrator access and audit tasks. Sign out when finished, and hide personal identifiers in screenshots.