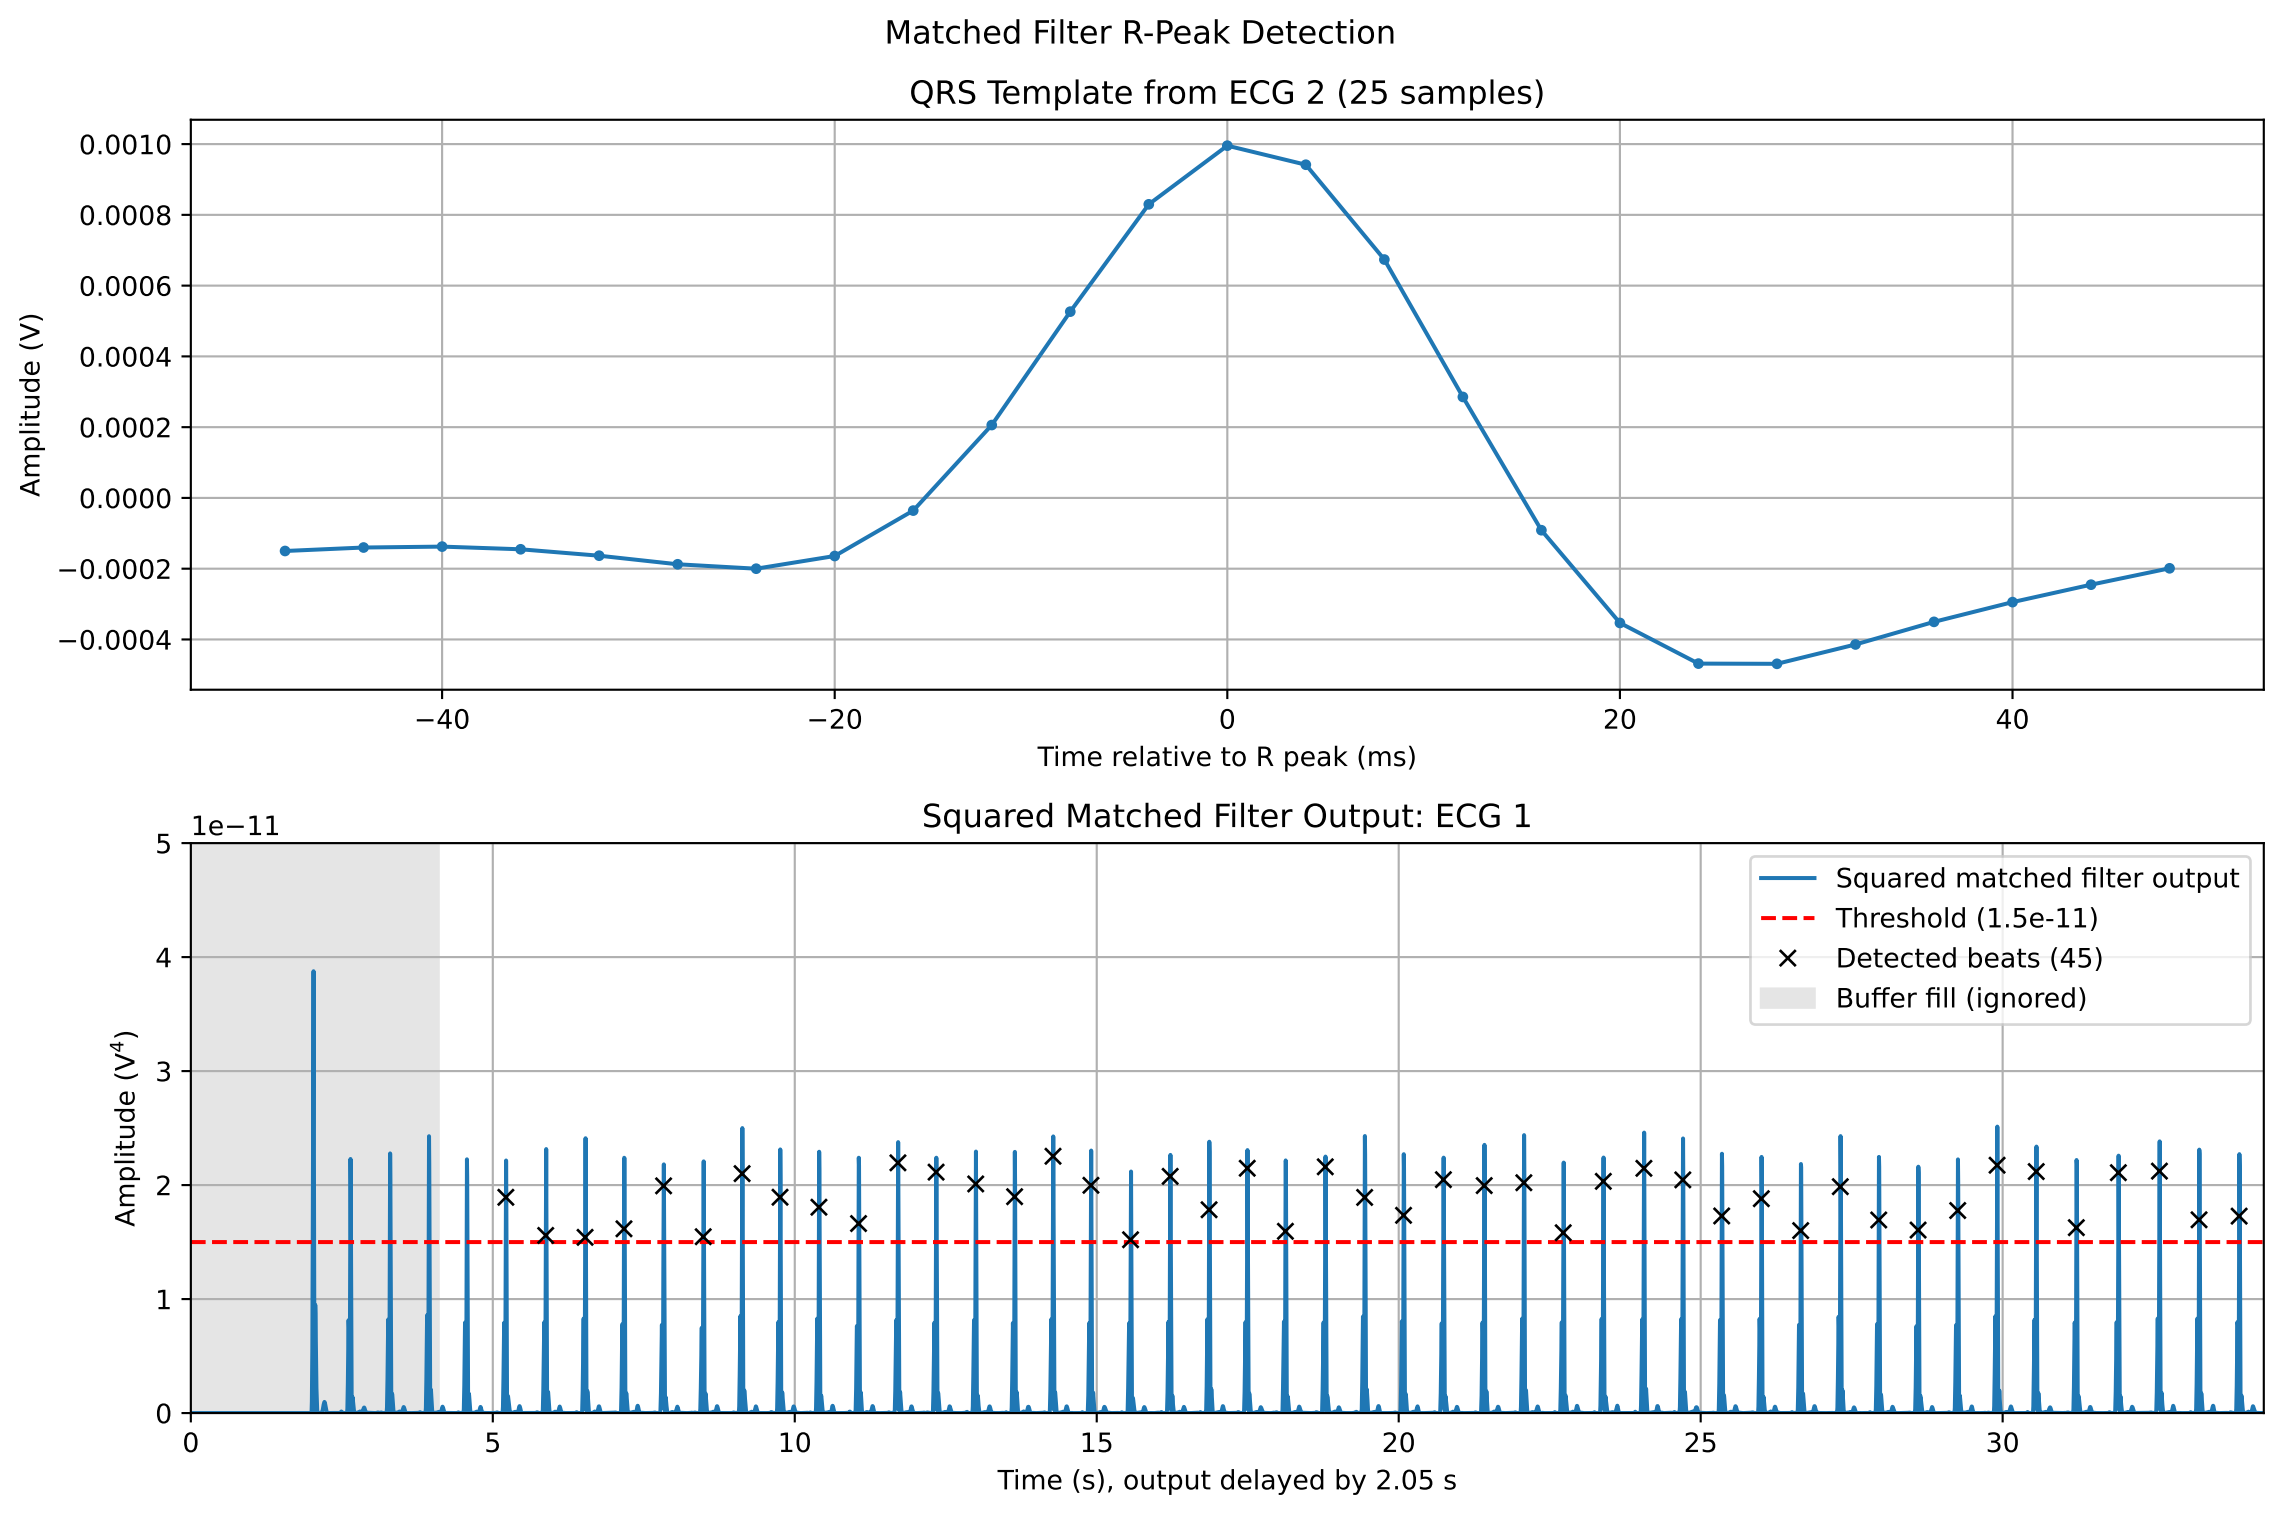
Matched Filter R-Peak Detection
QRS Template from ECG 2 (25 samples)
Amplitude (V)
0.0010
0.0008
0.0006
0.0004
0.0002
0.0000
−0.0002
−0.0004
−40
−20
0
20
40
Time relative to R peak (ms)
Squared Matched Filter Output: ECG 1
1e−11
Amplitude (V⁴)
Squared matched filter output
Threshold (1.5e-11)
Detected beats (45)
Buffer fill (ignored)
0
5
10
15
20
25
30
Time (s), output delayed by 2.05 s