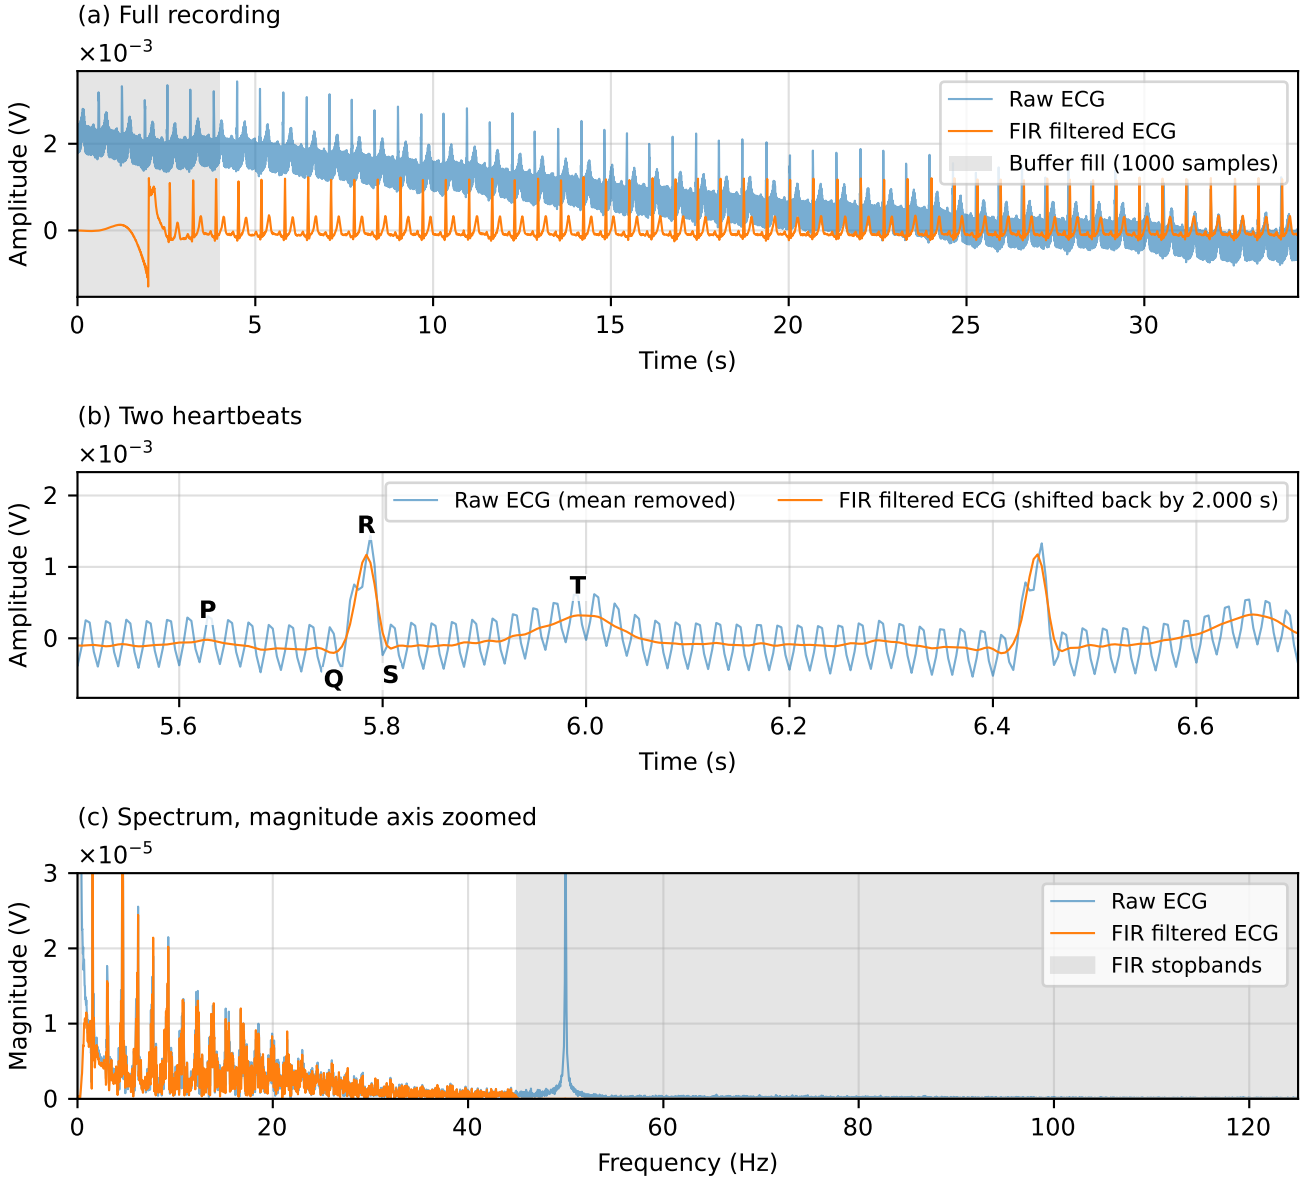

(a) Full recording
×10−3
Amplitude (V)
Raw ECG
FIR filtered ECG
Buffer fill (1000 samples)
Time (s)
(b) Two heartbeats
×10−3
Amplitude (V)
Raw ECG (mean removed)
FIR filtered ECG (shifted back by 2.000 s)
P
Q
R
S
T
Time (s)
(c) Spectrum, magnitude axis zoomed
×10−5
Magnitude (V)
Raw ECG
FIR filtered ECG
FIR stopbands
Frequency (Hz)