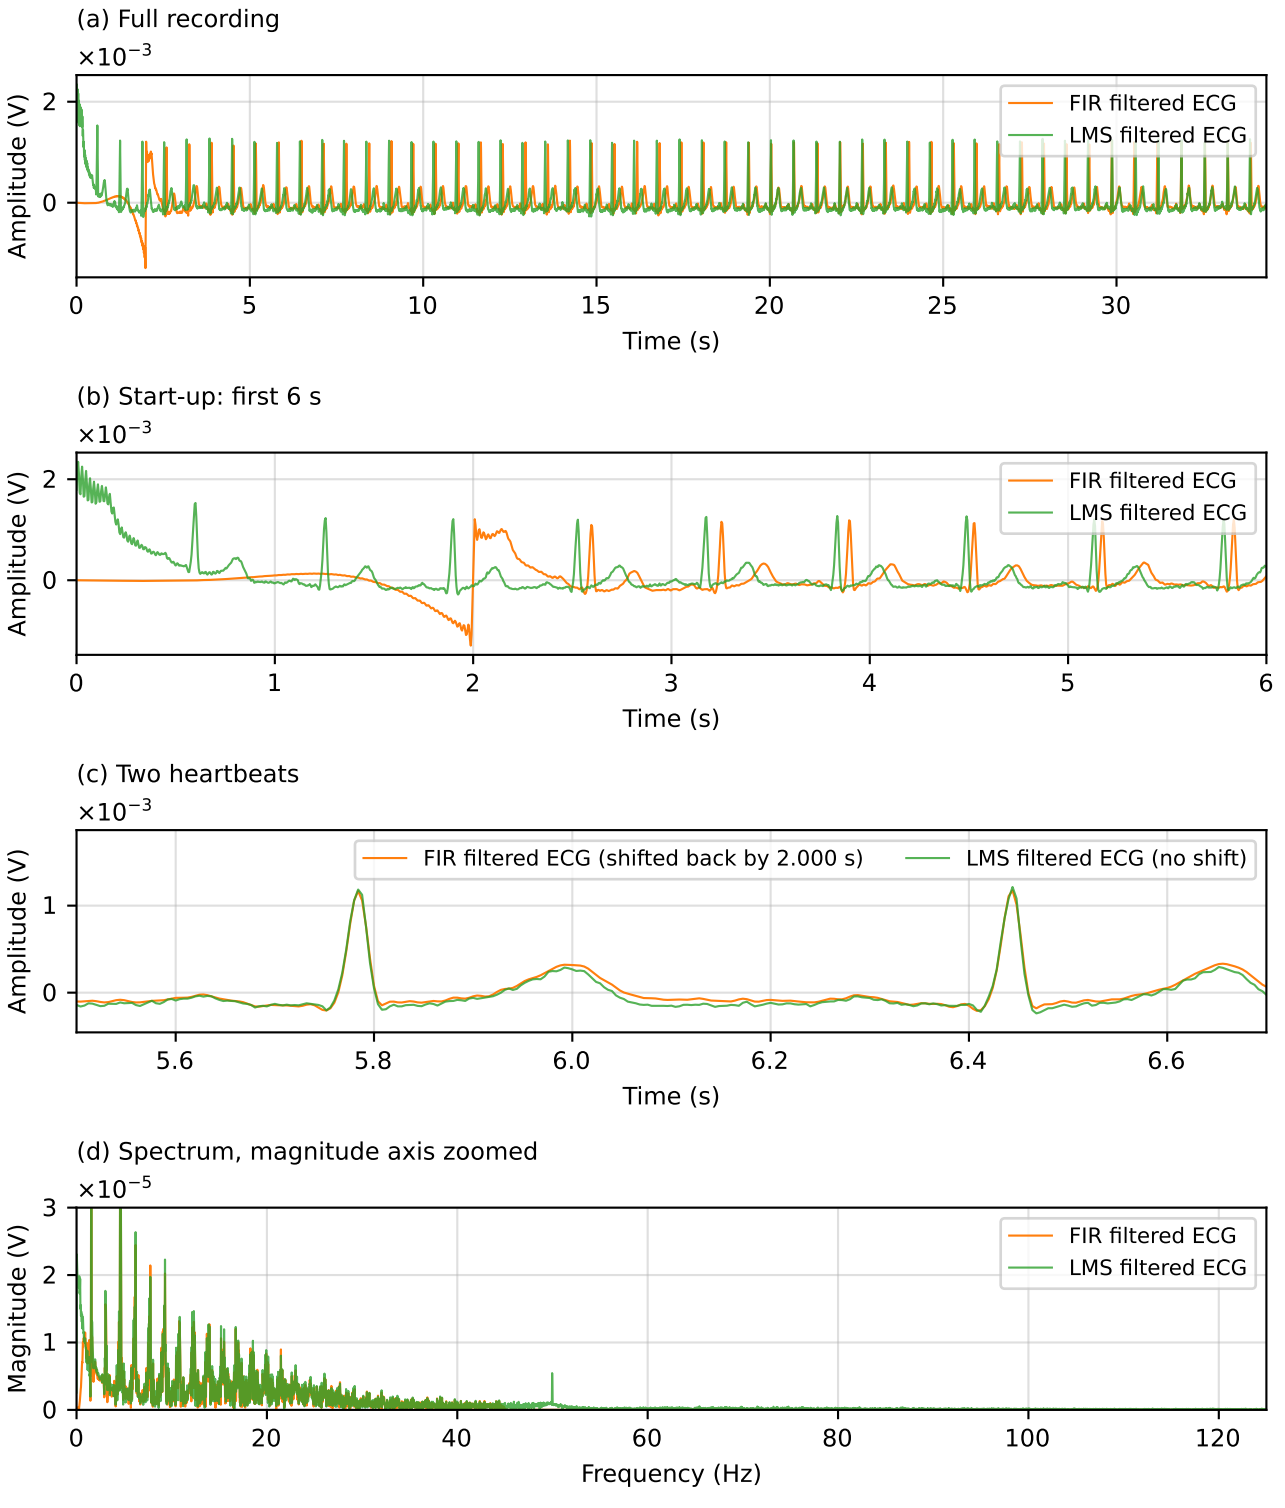

(a) Full recording
×10⁻³
Amplitude (V)
FIR filtered ECG
LMS filtered ECG
Time (s)
(b) Start-up: first 6 s
×10⁻³
Amplitude (V)
FIR filtered ECG
LMS filtered ECG
Time (s)
(c) Two heartbeats
×10⁻³
Amplitude (V)
FIR filtered ECG (shifted back by 2.000 s)
LMS filtered ECG (no shift)
Time (s)
(d) Spectrum, magnitude axis zoomed
×10⁻⁵
Magnitude (V)
FIR filtered ECG
LMS filtered ECG
Frequency (Hz)