



ALLANS

Your Satisfaction is our Technology



MENTOR-FP

ALLANS is showcasing an innovative, high-quality C-Arm tailored for diverse customer needs.

ALLANS FLAT PANEL C-ARM

About Allans


Welcome to Allans Medical Systems Pvt. Ltd. Founded in 1992, we are a leading manufacturer of X-ray equipment in the biomedical engineering sector. We are known for our high-quality, precisely crafted products. Our skilled team of engineers, with extensive field experience, designs a wide range of X-ray equipment, including dental machines. We offer systems with output capacities ranging from **15 mA to 500 mA, and high-frequency machines from 3.5 kW to 80 kW**. We recently introduced a **Flat-panel C-arm**, further expanding our product range.

MENTOR-FP




ALLANS Flat Panel C-Arm utilises advanced High Frequency Technology (**3.5/5 kW**) to minimise radiation exposure and enhance image quality compared to traditional image intensifier C-arms, and it has lots of benefits

- Flat panel detectors offer superior image resolution, producing clearer images than image intensifiers.
- Flat-panel C-arms capture a broader field of view in a single exposure.
- They typically require lower radiation doses for similar image quality, reducing patient exposure.
- Additionally, flat-panel C-arms enable faster image acquisition and processing, shortening operating time and improving workflow efficiency.
- Flat-panel C-arms produce more stable images, with no degradation in image quality over time.

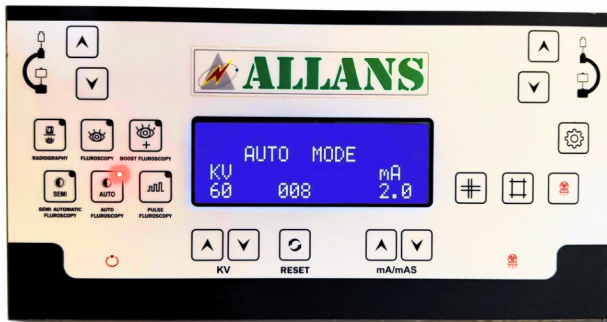


The **ALLANS** Medical C-arm's Console Board is designed as the **central, user-friendly interface** that empowers healthcare professionals with comprehensive control over its advanced imaging capabilities.


C-Arm Movements

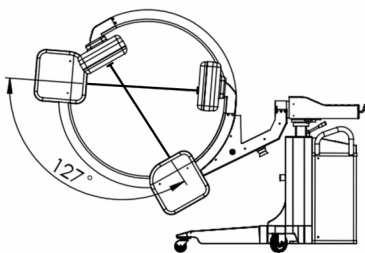


The C-arm can be rotated **orbitally by 127°**

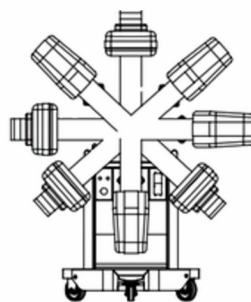


The C-arm can be rotated **$\pm 180^\circ$ in the vertical plane** around the horizontal axis

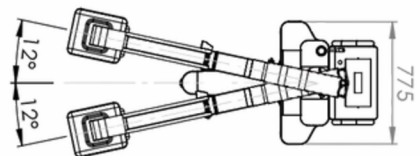

The C-arm can be **swiveled 12° to the left or right** around the vertical axis of the lifting column

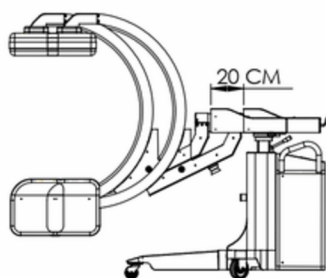

The C-arm can be moved forward and backwards by **20 cm in the horizontal plane** using the horizontal carriage



The C-arm can be **moved up and down by 40 cm**, and this movement is motorized.


Technical Specification

High Voltage Generator 40kHz		Electrical Characteristics	
Maximum Power	3.5 kW	Input Voltage (AC, Single Phase)	230V, 16A
Maximum Voltage to XRay Tube	110 kV	Frequency	50Hz
Cathode to Ground	55 kV	Max. Current Absorption	230V, 6A
Anode to Ground	55 kV	Anode to Ground	55 kV
Max Current to Xray Tube	80 mA	Power Chord	16A

Mechanical Characteristics		Software Characteristics	
Vertical Up/Down	420mm	Image	DICOM
Horizontal Movement	200mm	Post Processing	Yes
Wig-Wag	+/- 12°	Noise Reduction	Yes
Arc rotation around horizontal axis	360°	PACS	Yes
Arc movement	-130°	Print	Yes
SID	1000mm	Digital Image Rotation	Yes
Arc depth	700mm	Image Flip	Yes
Max Length	1803mm	Contrast/Brightness	Yes
Max Width	784mm	Horizontal/Vertical	Yes
Max Height	1733mm	Anatomical Preset	Standard
Weight	255 kg	Zoom & PAN	Yes
Movement	Manual steering, Handle for locking	Magnification Glass	Yes
		Annotation	Text/Angle
		Undo / Deletion	Yes

The company have right to make any change in design or specification without prior notice or obligation

QUALITY AND SAFETY CERTIFICATIONS

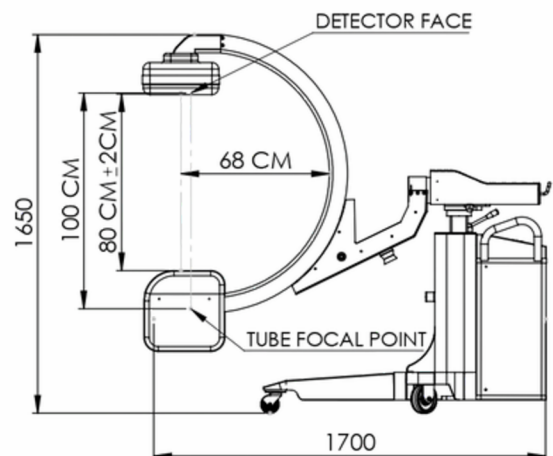

system drawing overview with component labelling

ALLANS MEDICAL SYSTEMS PVT. LTD.

No.1, Thakur Lane, Opp. Datta Mandir, Behind Disha Hospital, Asalpha Village, Ghatkopar (W),

Mumbai - 400084 INDIA Office:- 8879780695, Tel:- 022-2512 8274

Email:- allansmedisys@gmail.com Website:- www.allansmedisys.com