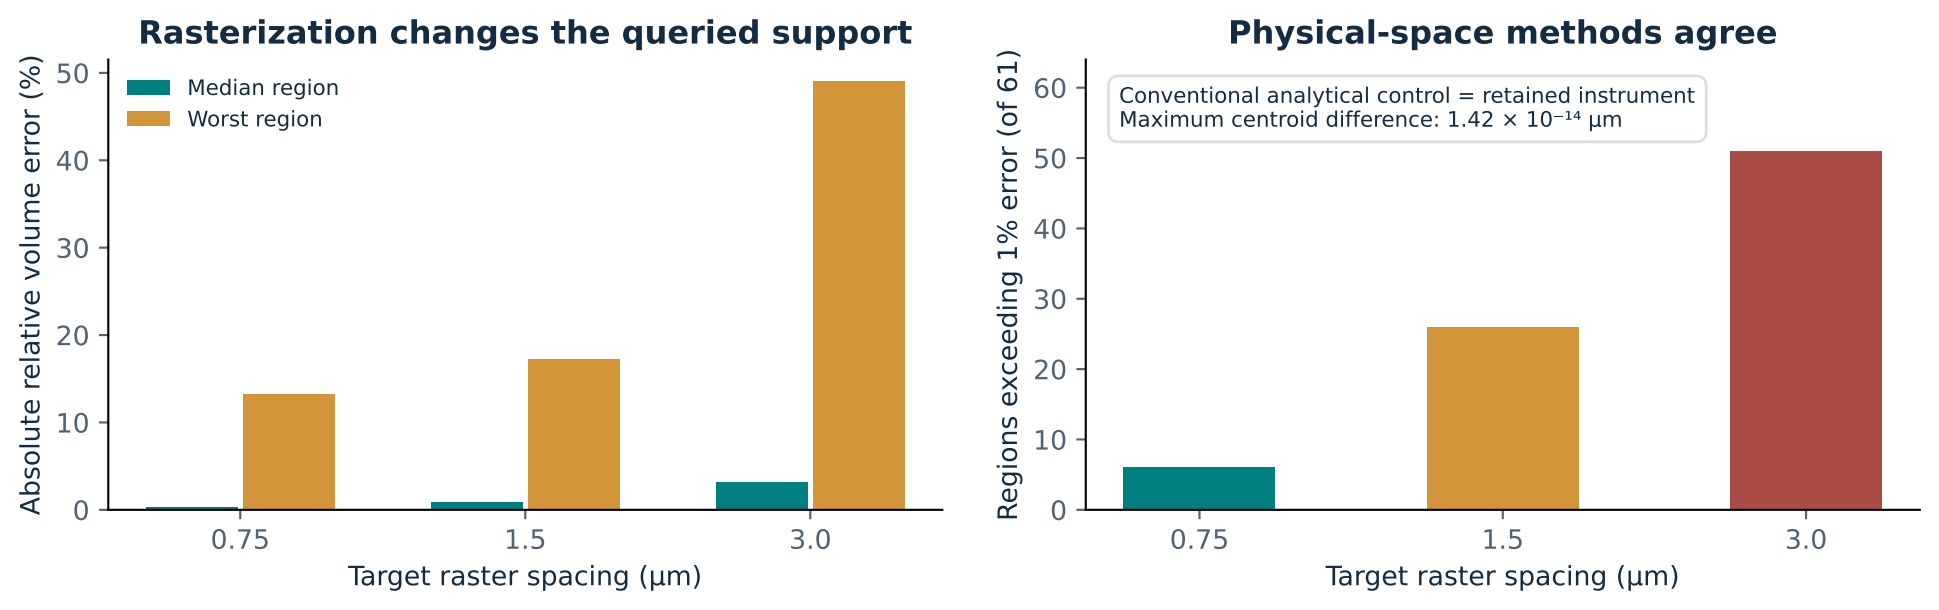
Rasterization changes the queried support
Median region
Worst region
Absolute relative volume error (%)
0
10
20
30
40
50
0.75
1.5
3.0
Target raster spacing (µm)
Physical-space methods agree
Conventional analytical control = retained instrument
Maximum centroid difference: 1.42 × 10⁻¹⁴ µm
Regions exceeding 1% error (of 61)
0
10
20
30
40
50
60
0.75
1.5
3.0
Target raster spacing (µm)