



Polygraph Lab — Automatic Experiment Report




Generated: 2025-10-26T10:34:03.776553 UTC



Experiment Objective: How do physical factors—in particular contact pressure and moisture—affect the measurement accuracy of a lie detector based on galvanic skin response (GSR)?

Device: device_4

GSR Baseline: 6.226 ± 2.733
Baseline Pressure: 100.0 g | Baseline Humidity: 50.0 %

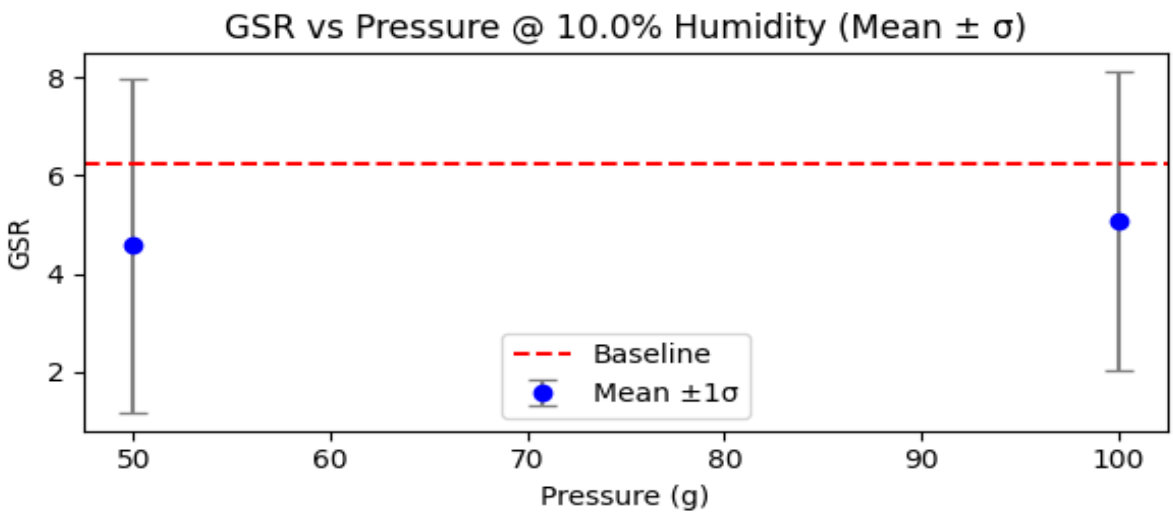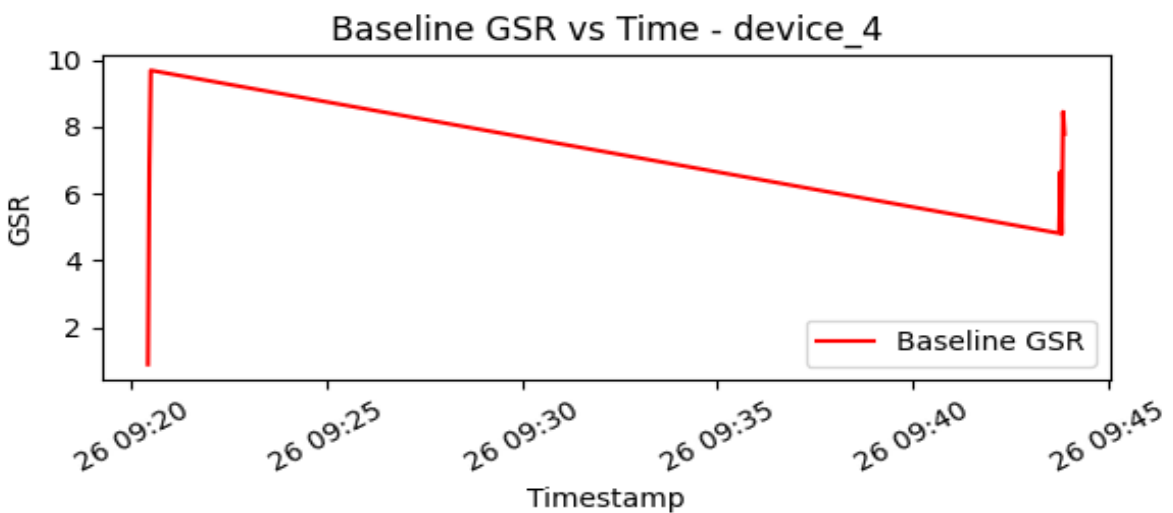

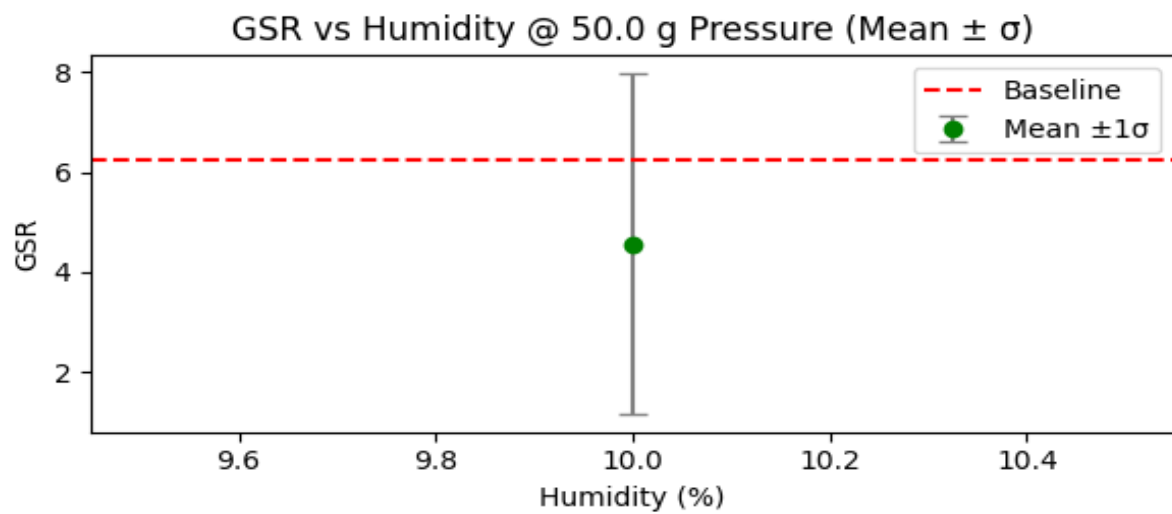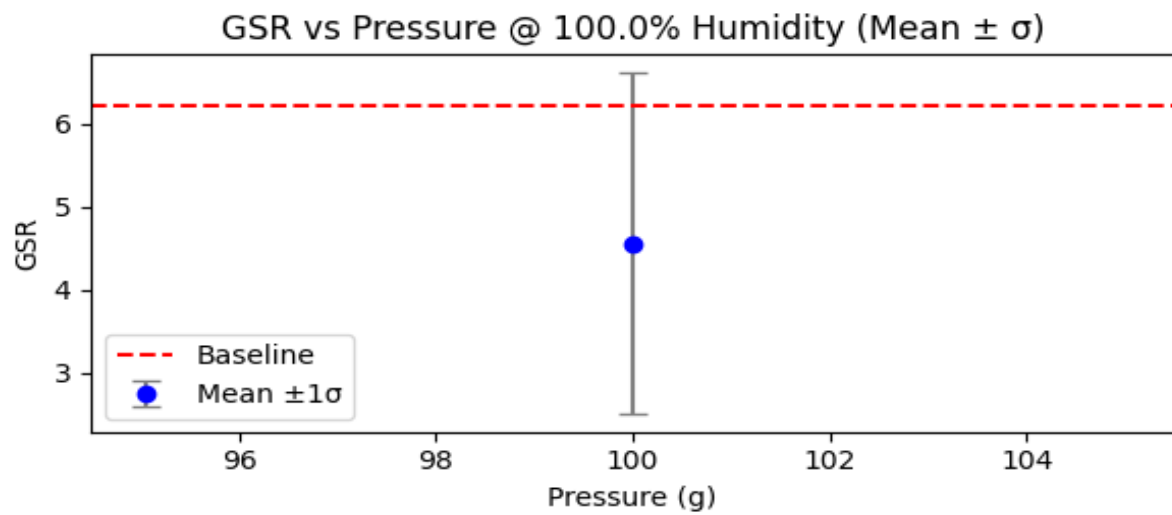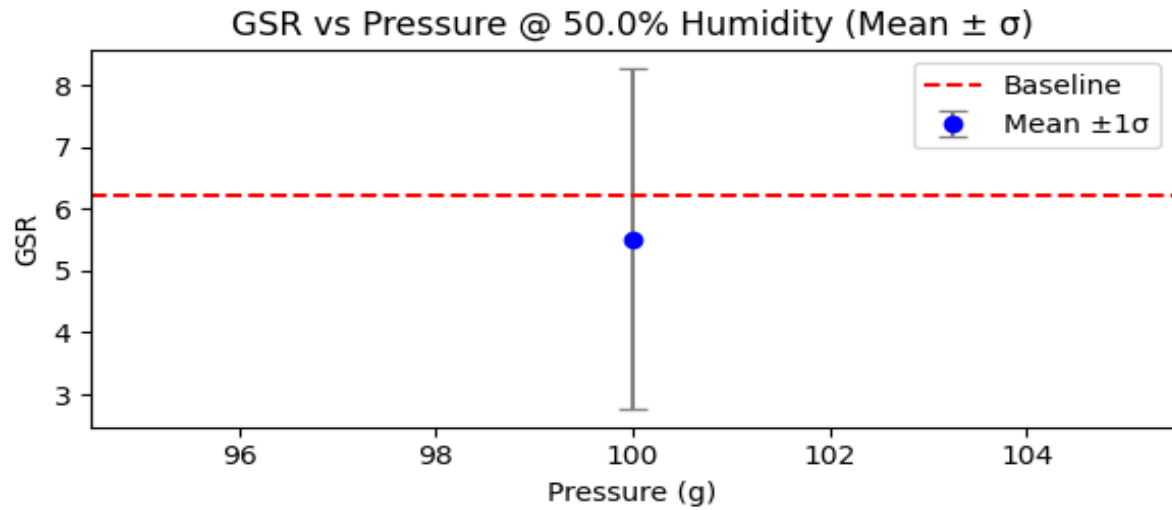

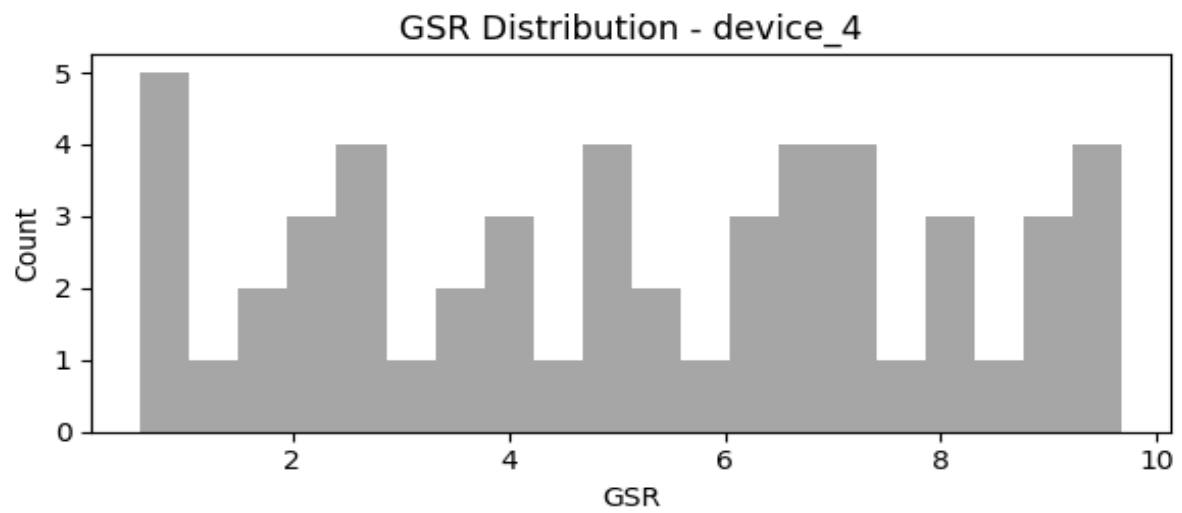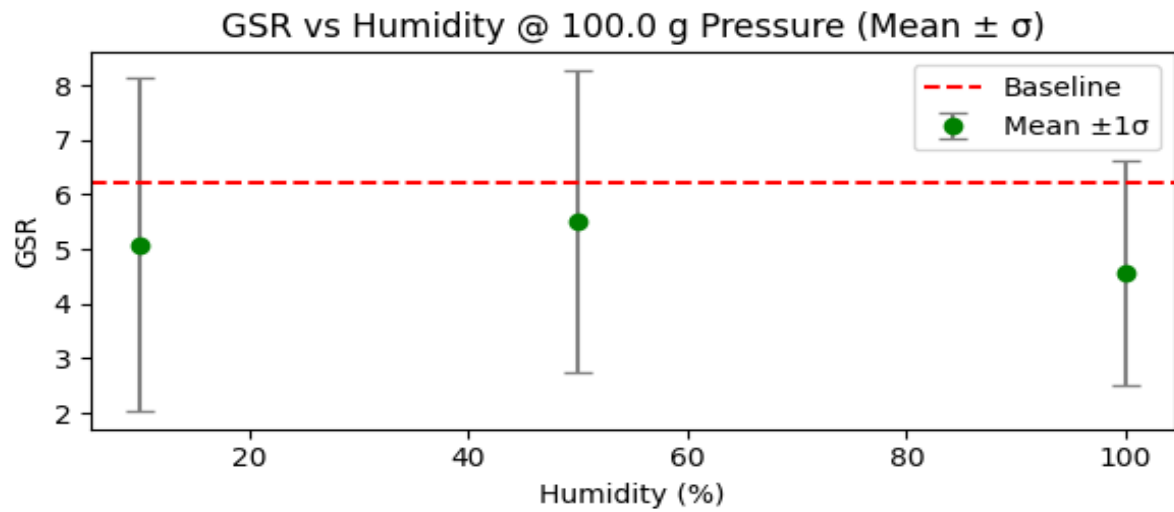

Overall optimal pressure: 100.0 g