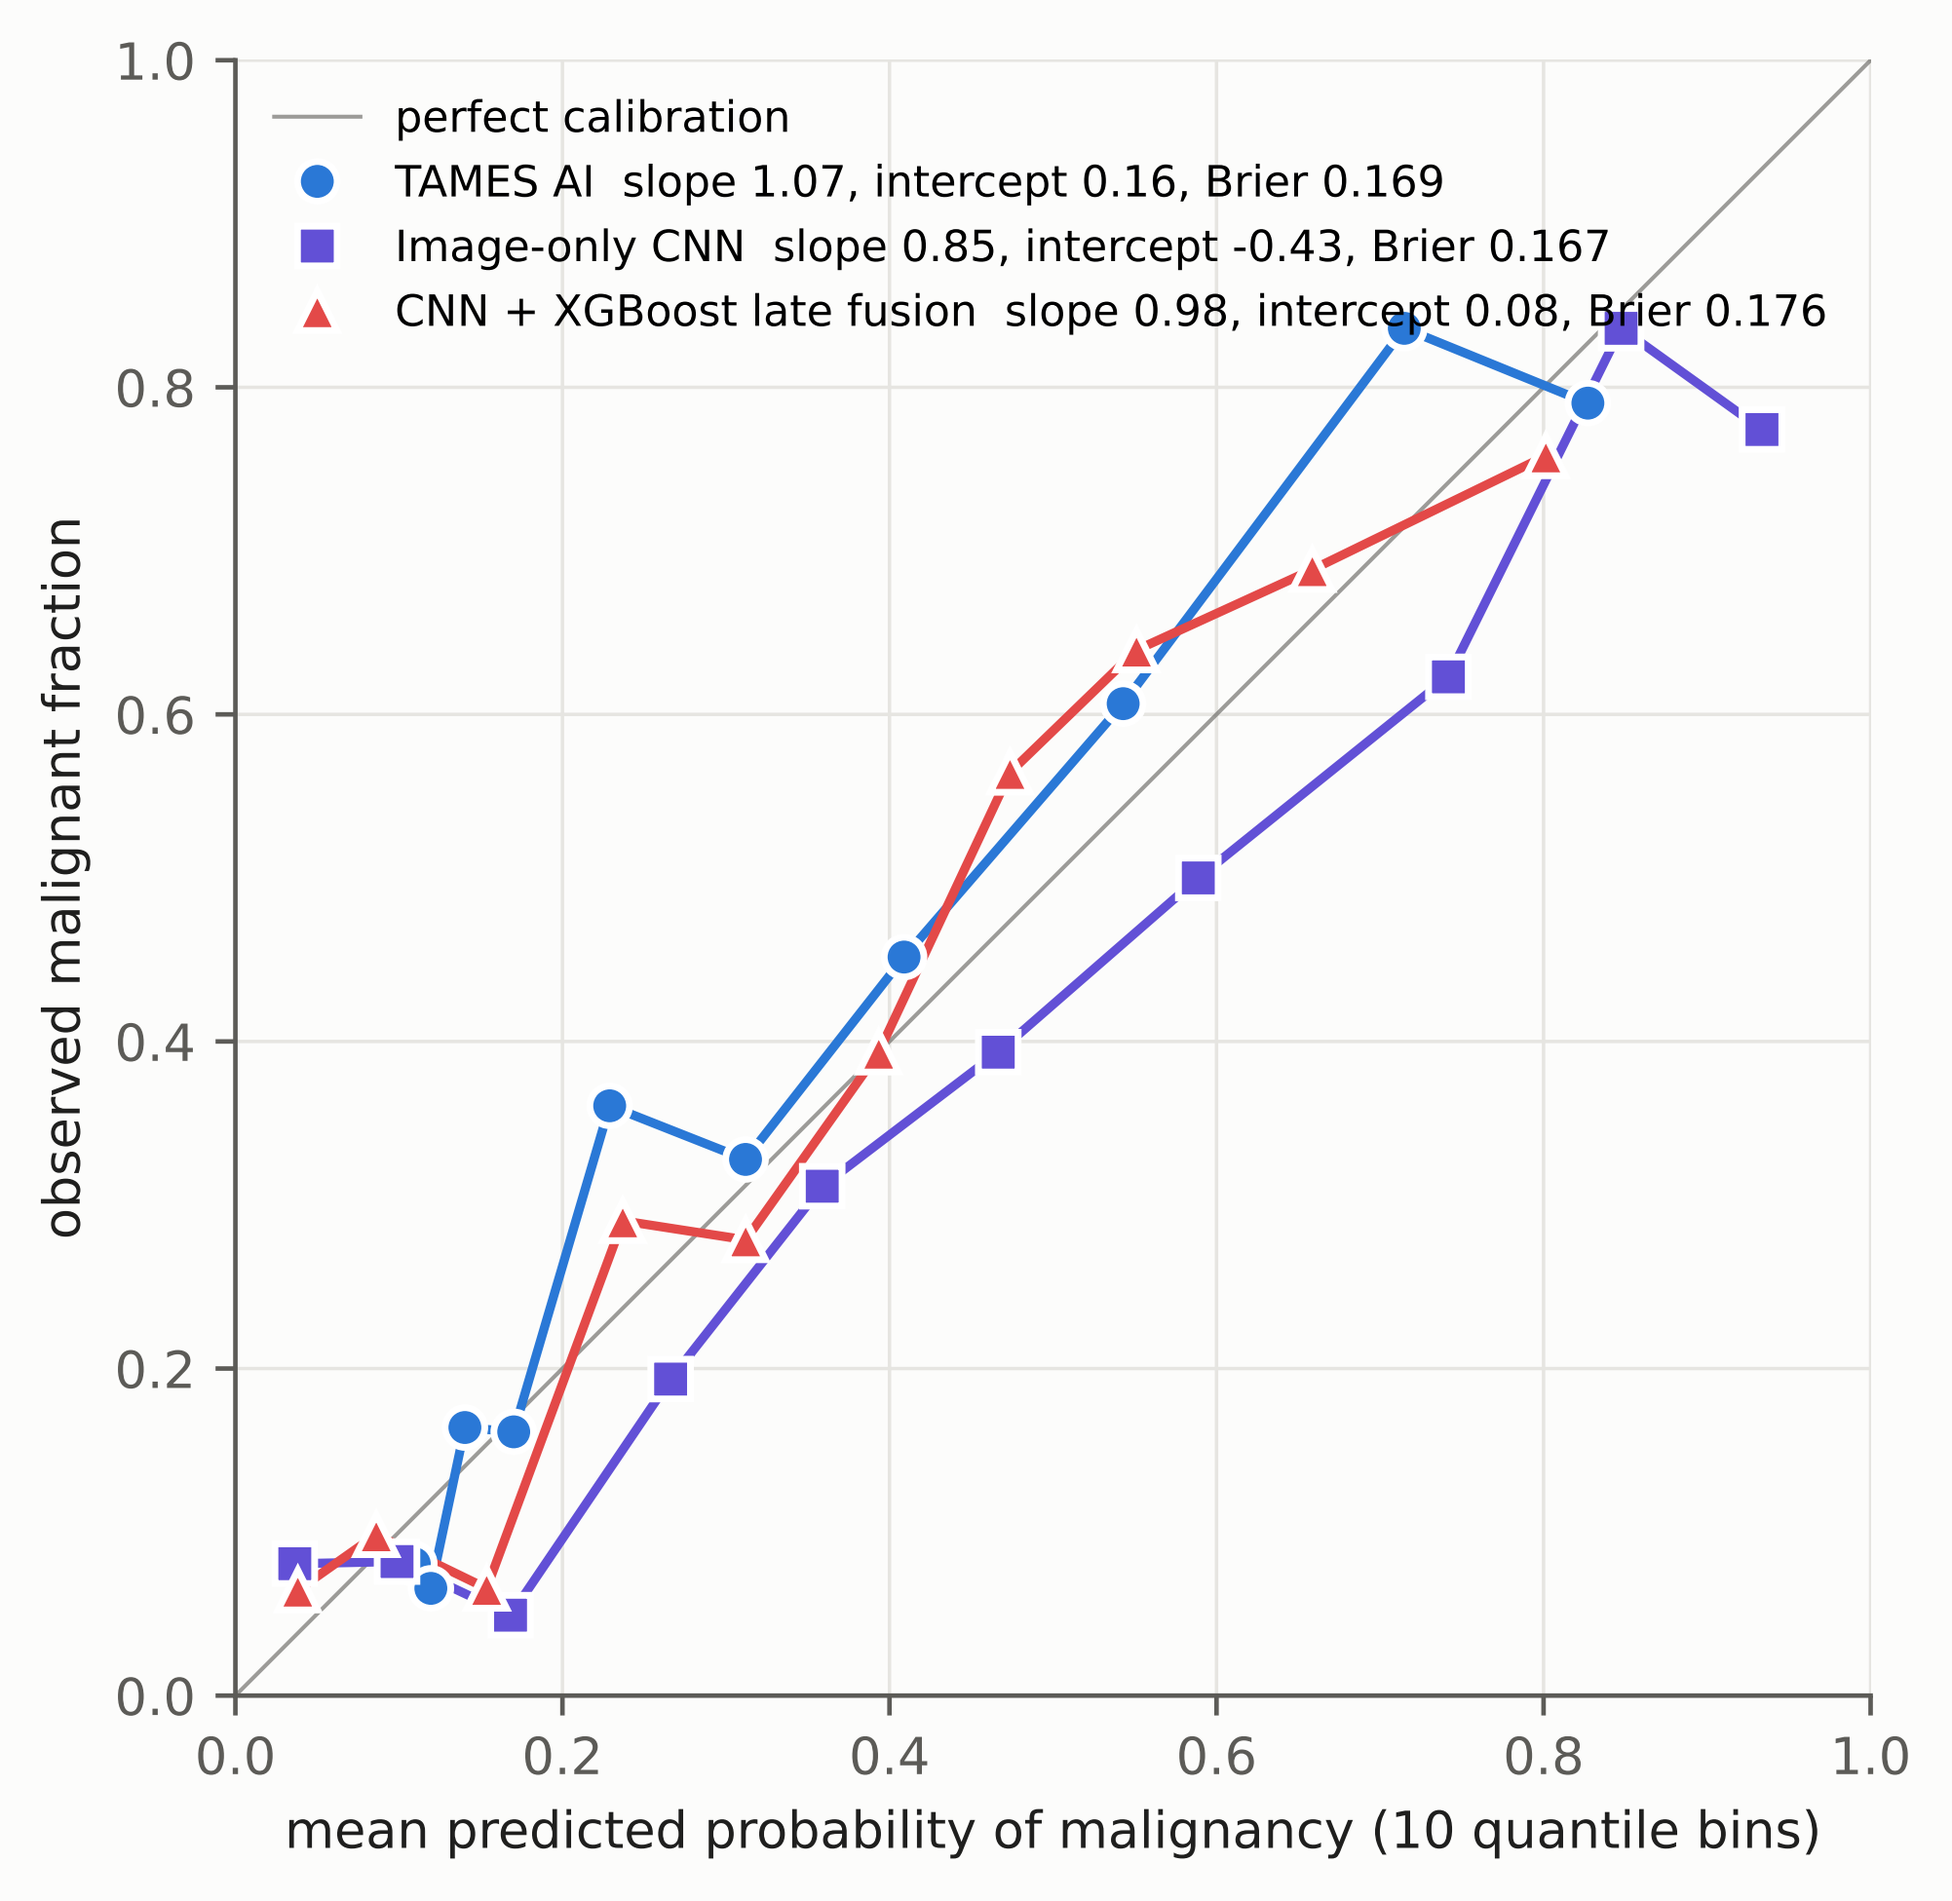
perfect calibration
TAMES AI slope 1.07, intercept 0.16, Brier 0.169
Image-only CNN slope 0.85, intercept -0.43, Brier 0.167
CNN + XGBoost late fusion slope 0.98, intercept 0.08, Brier 0.176
observed malignant fraction
mean predicted probability of malignancy (10 quantile bins)
0.0
0.2
0.4
0.6
0.8
1.0