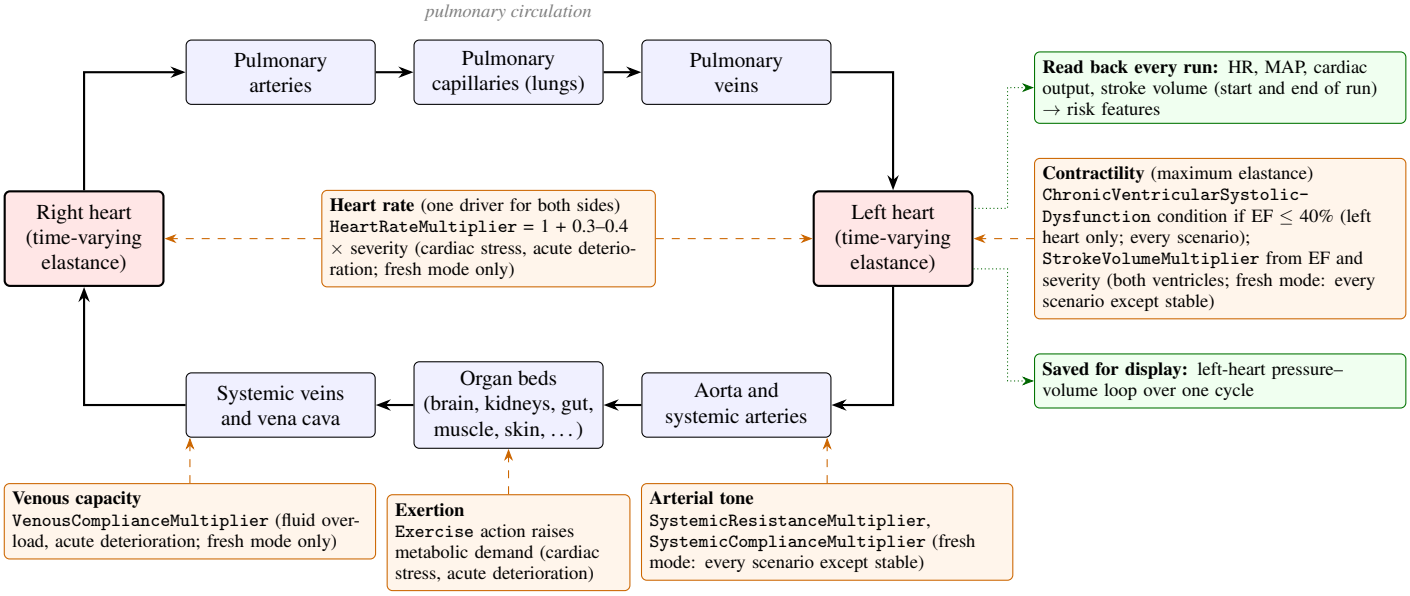


Continuous mode (both scenario-test experiments): each day re-issues only the contractility and arterial-tone multipliers, plus `Exercise` for the two exertion labels; the heart-rate and venous-capacity extras apply only in fresh mode.