


U2
LOGO_UDLABS
Upside Down Labs LOGO

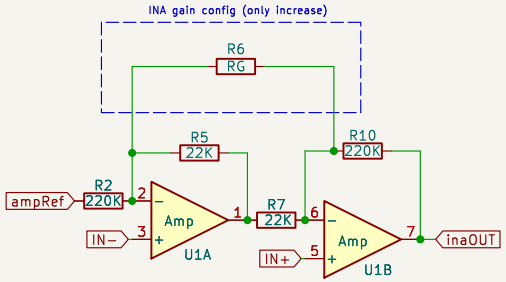



Removes high freqency noise.


11x Gain Instrumentation Amp (INA)

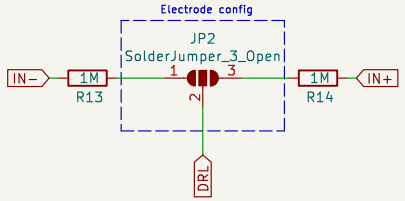


Bridge all three pads of the solder jumper (JP2) to configure for 2 Electrode operations instead of the 3 electrodes
Note: 2 electrodes will give noisier output than 3 electrodes!

Electrode reference


Create solder joint on JP1 to increase the Band Pass freqnecny range
Default: Narrow input frequency band, use when recording EEG, EOG
Configured: Wide input frequency band, use for ECG, EMG, and EOG

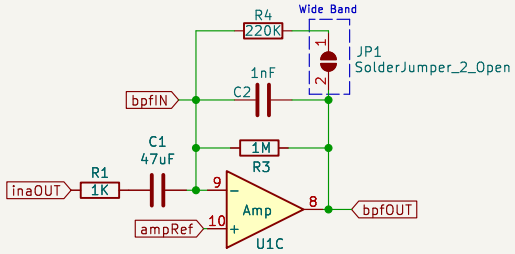

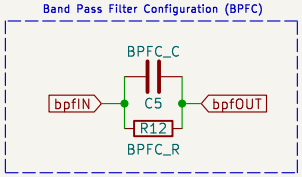


C5 (BPFC_C) & R12 (BPFC_R) on the back side of the PCB can be used to configure the bandpass filter. Use them to configure output Gain (decrease) & Band (frequency range).


1000x Gain Bandpass Filter

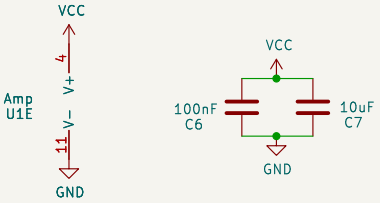

Power supply filtering

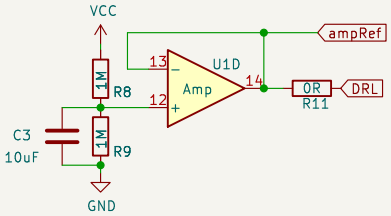

Amp Ref + Driven Right Leg (DRL)

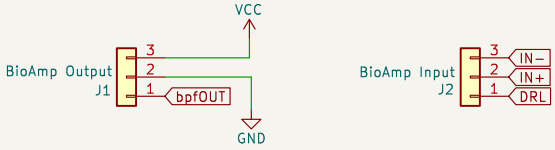

Header pins / Connectors

Quad−OpAmp based BioAmp
Signle chip biopotential amplifier
5v compatible EXG hardware
Records EMG, ECG, EOG, and EEG
Upside Down Labs

Sheet: /
File: BioAmp−EXG−Pill.kicad_sch

contact@upsidedownlabs.tech

Title: BioAmp EXG Pill

Size: A4	Date: 2023−04−27	**Rev: 1.0**
KiCad E.D.A. 8.0.8		Id: 1/1